


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046409.D
Acq On : 16 Dec 2021 10:03
Operator : SY/MD
Sample : BFB033
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB033

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Title : VOC Analysis
Last Update : Mon Dec 20 00:25:10 2021

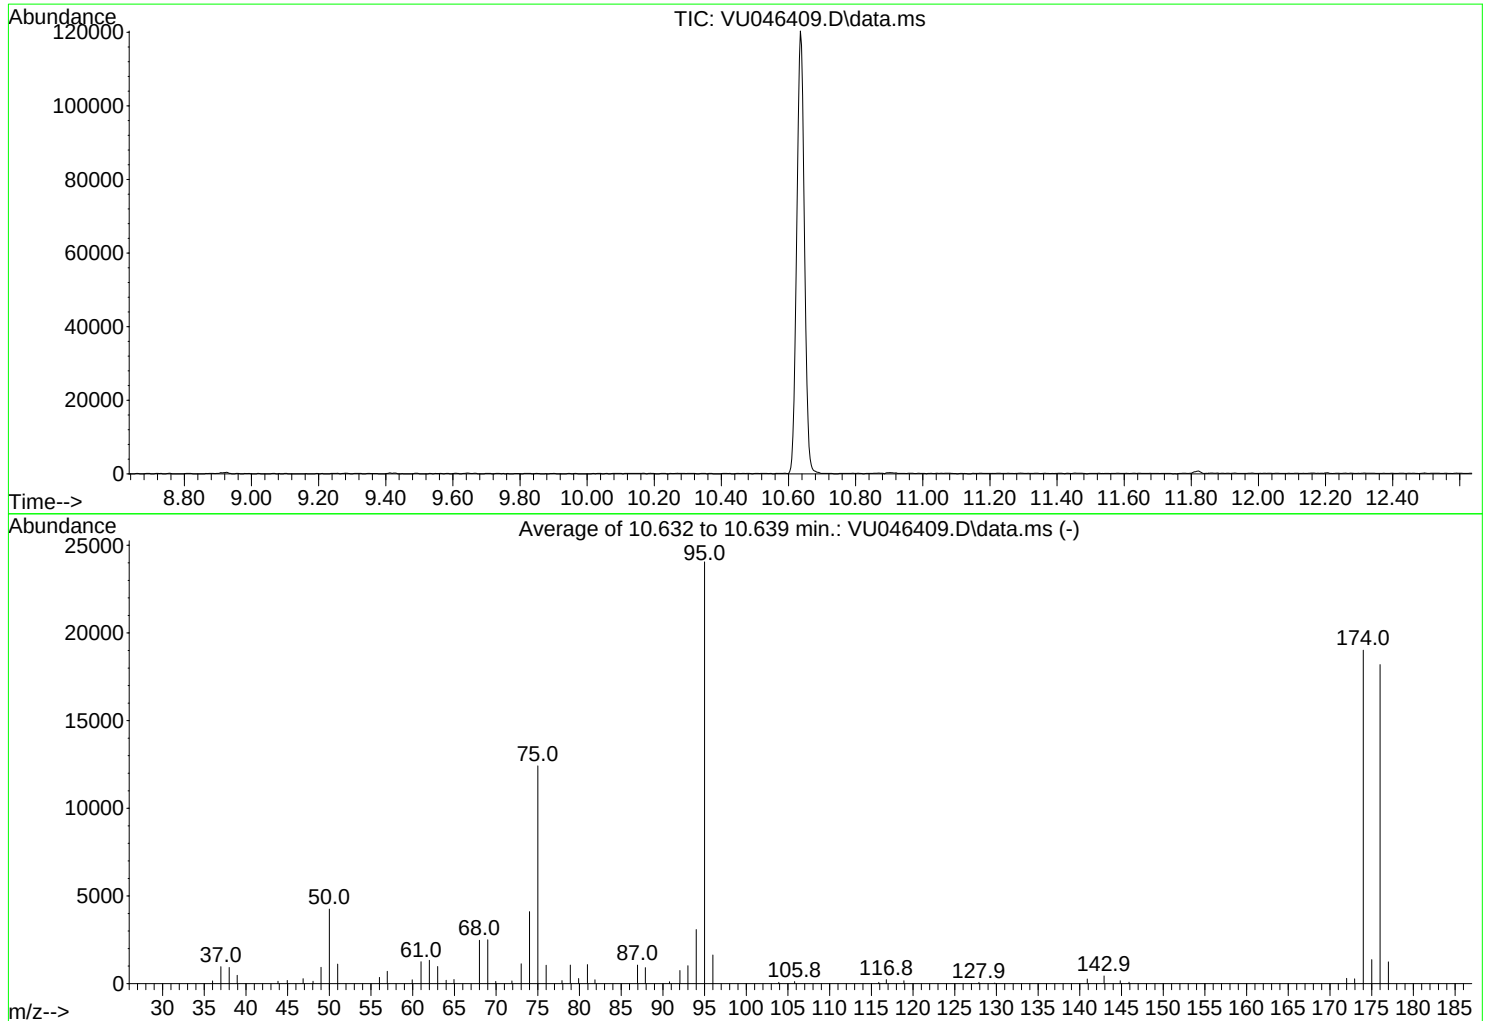

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	4257	PASS
75	95	30	80	51.6	12419	PASS
95	95	100	100	100.0	24056	PASS
96	95	5	9	6.8	1635	PASS
173	174	0.00	2	1.4	271	PASS
174	95	50	120	79.1	19019	PASS
175	174	5	9	7.2	1368	PASS
176	174	95	101	95.7	18192	PASS
177	176	5	9	6.8	1240	PASS

m/z	Abundance
43.80	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
36.10	167.0
37.00	987.0
38.00	883.0
38.90	448.0
43.90	289.0
45.00	185.0
46.80	289.0
48.00	151.0
49.00	987.0
50.00	4169.0
51.00	1096.0
56.00	327.0
56.90	733.0
60.00	214.0
61.00	1268.0
62.00	1328.0
63.00	991.0
64.00	179.0
65.00	220.0
68.00	2474.0
69.00	2479.0
70.00	125.0
71.90	158.0
73.00	1090.0
74.00	3948.0
75.00	11898.0
76.00	980.0
77.90	160.0
78.90	1016.0
79.90	282.0
80.90	1127.0
81.80	232.0
87.00	1039.0
87.90	920.0
90.80	111.0
92.00	669.0
93.00	937.0
94.00	2984.0
95.00	23592.0
96.00	1700.0
105.80	118.0
115.90	102.0
116.80	234.0
118.90	169.0
129.80	118.0
140.90	234.0
142.90	427.0
144.80	177.0
145.90	128.0
172.00	279.0
173.00	272.0
174.00	18168.0
175.00	1354.0
176.00	17064.0
177.00	1183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
36.00	155.0
37.00	1006.0
38.00	971.0
39.00	494.0
43.90	304.0
44.90	189.0
46.90	295.0
48.10	149.0
49.00	969.0
50.00	4446.0
51.00	1117.0
56.00	377.0
57.00	717.0
59.90	217.0
61.00	1312.0
62.00	1381.0
63.00	998.0
64.00	202.0
64.90	239.0
68.00	2524.0
69.00	2585.0
69.90	127.0
71.90	156.0
73.00	1169.0
74.00	4254.0
75.00	12814.0
76.00	1079.0
77.90	193.0
78.90	1093.0
79.90	294.0
80.90	1122.0
81.80	226.0
87.00	1066.0
87.90	956.0
90.80	119.0
92.10	775.0
93.00	1068.0
94.00	3208.0
95.00	24872.0
96.00	1705.0
103.90	100.0
105.80	121.0
115.90	106.0
116.80	236.0
118.90	178.0
127.90	111.0
140.90	277.0
142.90	458.0
144.80	160.0
145.90	119.0
172.00	306.0
173.00	286.0
174.00	19528.0
175.00	1390.0
176.00	18744.0
177.00	1249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	155.0
37.00	899.0
38.00	920.0
39.00	488.0
44.00	272.0
44.90	182.0
46.90	271.0
48.10	116.0
49.00	837.0
50.00	4156.0
51.00	1130.0
56.00	352.0
57.00	668.0
59.90	220.0
61.00	1162.0
62.00	1279.0
63.00	952.0
64.00	208.0
64.90	265.0
68.00	2409.0
69.00	2427.0
69.90	135.0
71.90	149.0
73.00	1143.0
74.00	4111.0
75.00	12546.0
76.00	1093.0
77.90	180.0
78.90	1060.0
79.90	299.0
81.00	1021.0
81.90	189.0
86.90	1082.0
87.90	858.0
90.80	109.0
92.10	800.0
93.00	1071.0
94.00	3071.0
95.00	23704.0
96.00	1500.0
103.90	112.0
105.80	107.0
116.80	202.0
118.90	156.0
127.90	102.0
140.90	272.0
142.90	437.0
144.90	157.0
172.00	321.0
172.90	254.0
174.00	19360.0
175.00	1359.0
176.00	18768.0
177.00	1288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033