

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052427.D
 Acq On : 16 Dec 2022 11:28
 Operator : JC/MD
 Sample : N6034-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 16 21:12:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	18252	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	16761	0.500	ug/L	0.01
11) 1,4-Dichlorobenzene-d4	11.742	152	8380	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	10380	0.483	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	96.000%
4) 1,2-Dichloroethane-d4	5.661	65	9376	0.460	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
7) 1,2-Dichloropropane-d6	6.639	67	11023	0.547	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	110.000%
8) Toluene-d8	7.830	98	14446	0.476	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.000%
10) 1,1,2,2-Tetrachloroeth...	10.679	84	11343	0.526	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.000%
Target Compounds						
6) Trichloroethene	6.489	95	320	0.017	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052427.D
Acq On : 16 Dec 2022 11:28
Operator : JC/MD
Sample : N6034-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 16 21:12:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

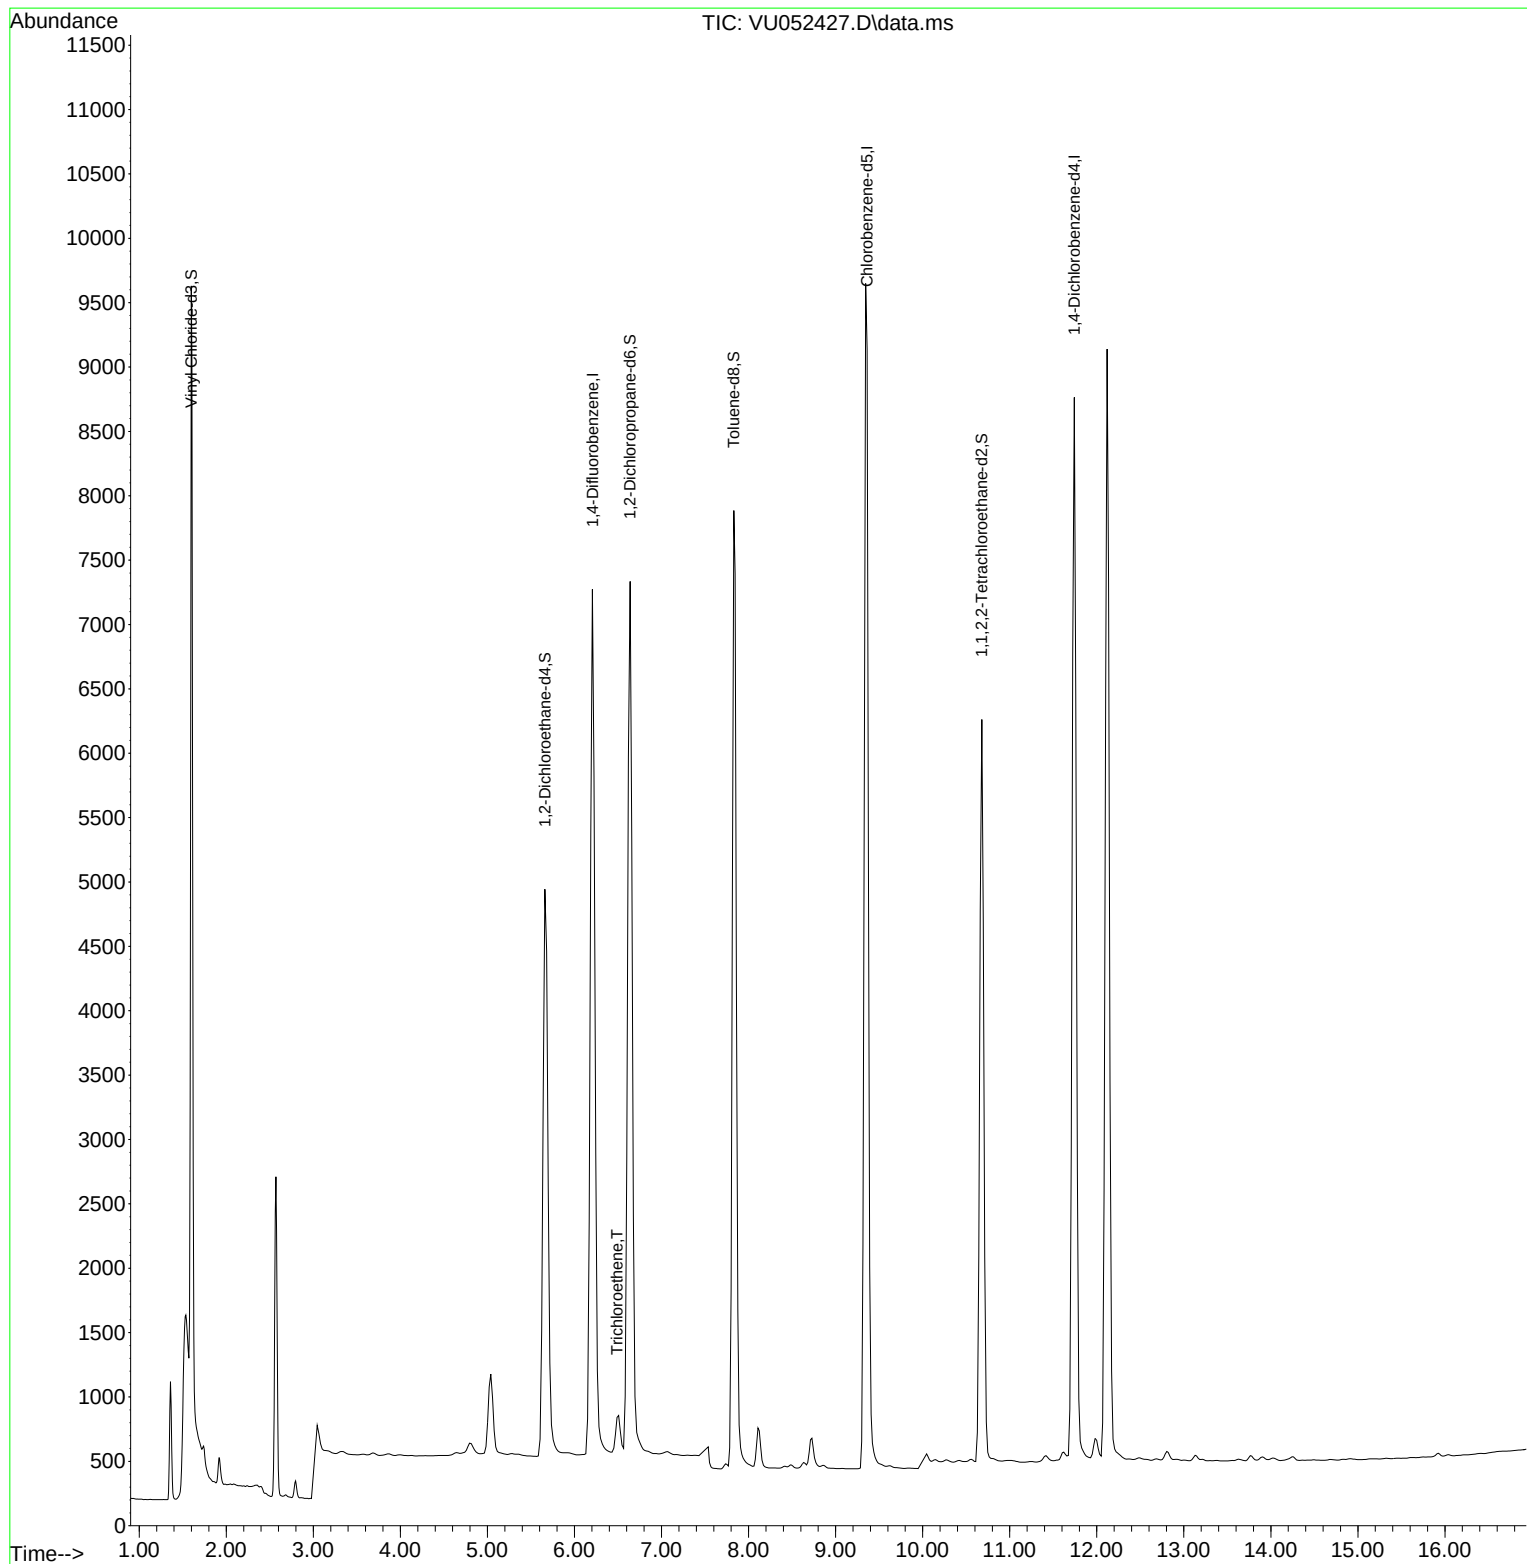

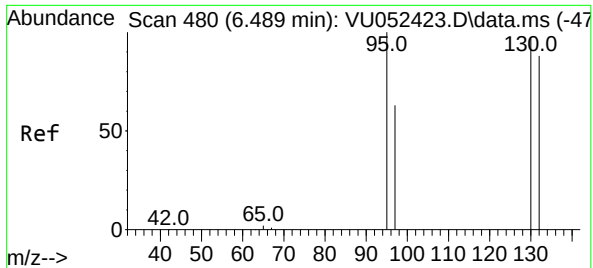

#6
 Trichloroethene
 Concen: 0.017 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052427.D
 Acq: 16 Dec 2022 11:28

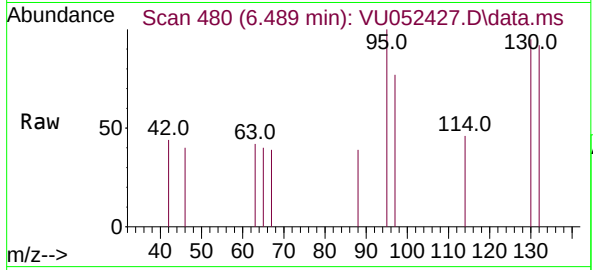

Tgt Ion: 95	Resp: 320
Ion Ratio	Lower Upper
95 100	
97 76.6	43.3 80.3
132 92.2	61.0 113.2
130 95.3	66.7 123.9

