

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052428.D
 Acq On : 16 Dec 2022 11:51
 Operator : JC/MD
 Sample : N6034-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 16 21:12:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	17804	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.346	117	16233	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.742	152	8014	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.599	65	10218	0.487	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	98.000%		
4) 1,2-Dichloroethane-d4	5.661	65	9204	0.463	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	92.000%		
7) 1,2-Dichloropropane-d6	6.639	67	10969	0.562	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	112.000%		
8) Toluene-d8	7.830	98	14621	0.497	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.000%		
10) 1,1,2,2-Tetrachloroeth...	10.679	84	11112	0.533	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	106.000%		
Target Compounds						
6) Trichloroethene	6.489	95	297	0.016	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052428.D
Acq On : 16 Dec 2022 11:51
Operator : JC/MD
Sample : N6034-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 16 21:12:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

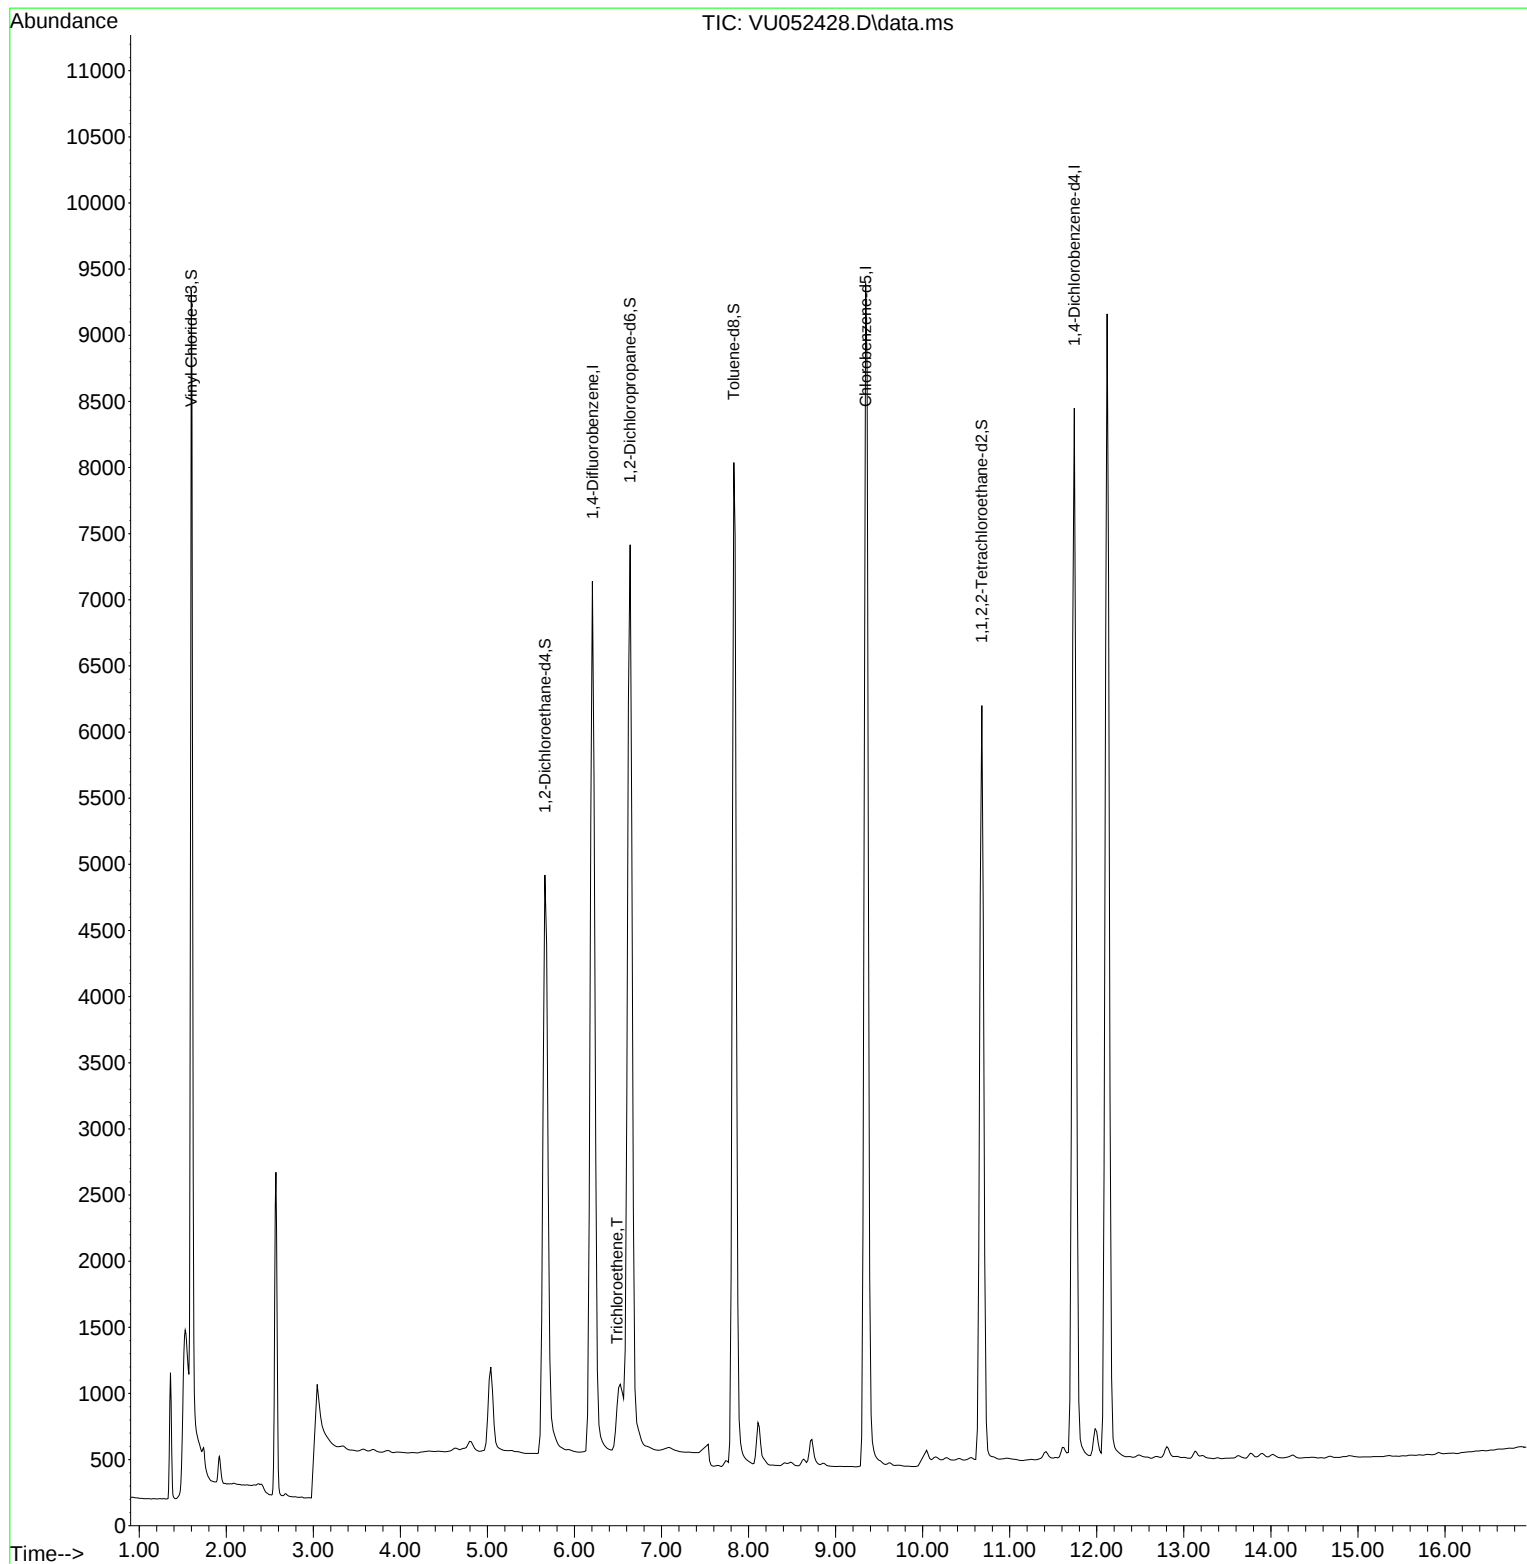

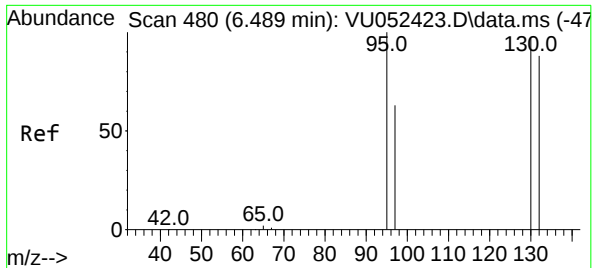

#6
 Trichloroethene
 Concen: 0.016 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052428.D
 Acq: 16 Dec 2022 11:51

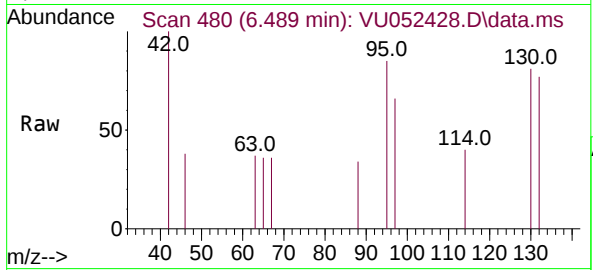

Tgt Ion: 95	Resp: 297
Ion Ratio	Lower Upper
95 100	
97 77.7	43.3 80.3
132 90.9	61.0 113.2
130 95.0	66.7 123.9

