

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052429.D
 Acq On : 16 Dec 2022 12:15
 Operator : JC/MD
 Sample : N6034-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 21:12:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	17465	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.346	117	15906	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.742	152	7879	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	10027	0.487	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	98.000%		
4) 1,2-Dichloroethane-d4	5.661	65	8855	0.454	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
7) 1,2-Dichloropropane-d6	6.639	67	10454	0.547	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	110.000%		
8) Toluene-d8	7.830	98	13829	0.480	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.000%		
10) 1,1,2,2-Tetrachloroeth...	10.679	84	10723	0.524	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	104.000%		
Target Compounds						
						Qvalue
6) Trichloroethene	6.489	95	262	0.015	ug/L	92
12) 1,2,3-Trichloropropane	10.748	75	61	0.005	ug/L #	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052429.D
Acq On : 16 Dec 2022 12:15
Operator : JC/MD
Sample : N6034-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 16 21:12:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration




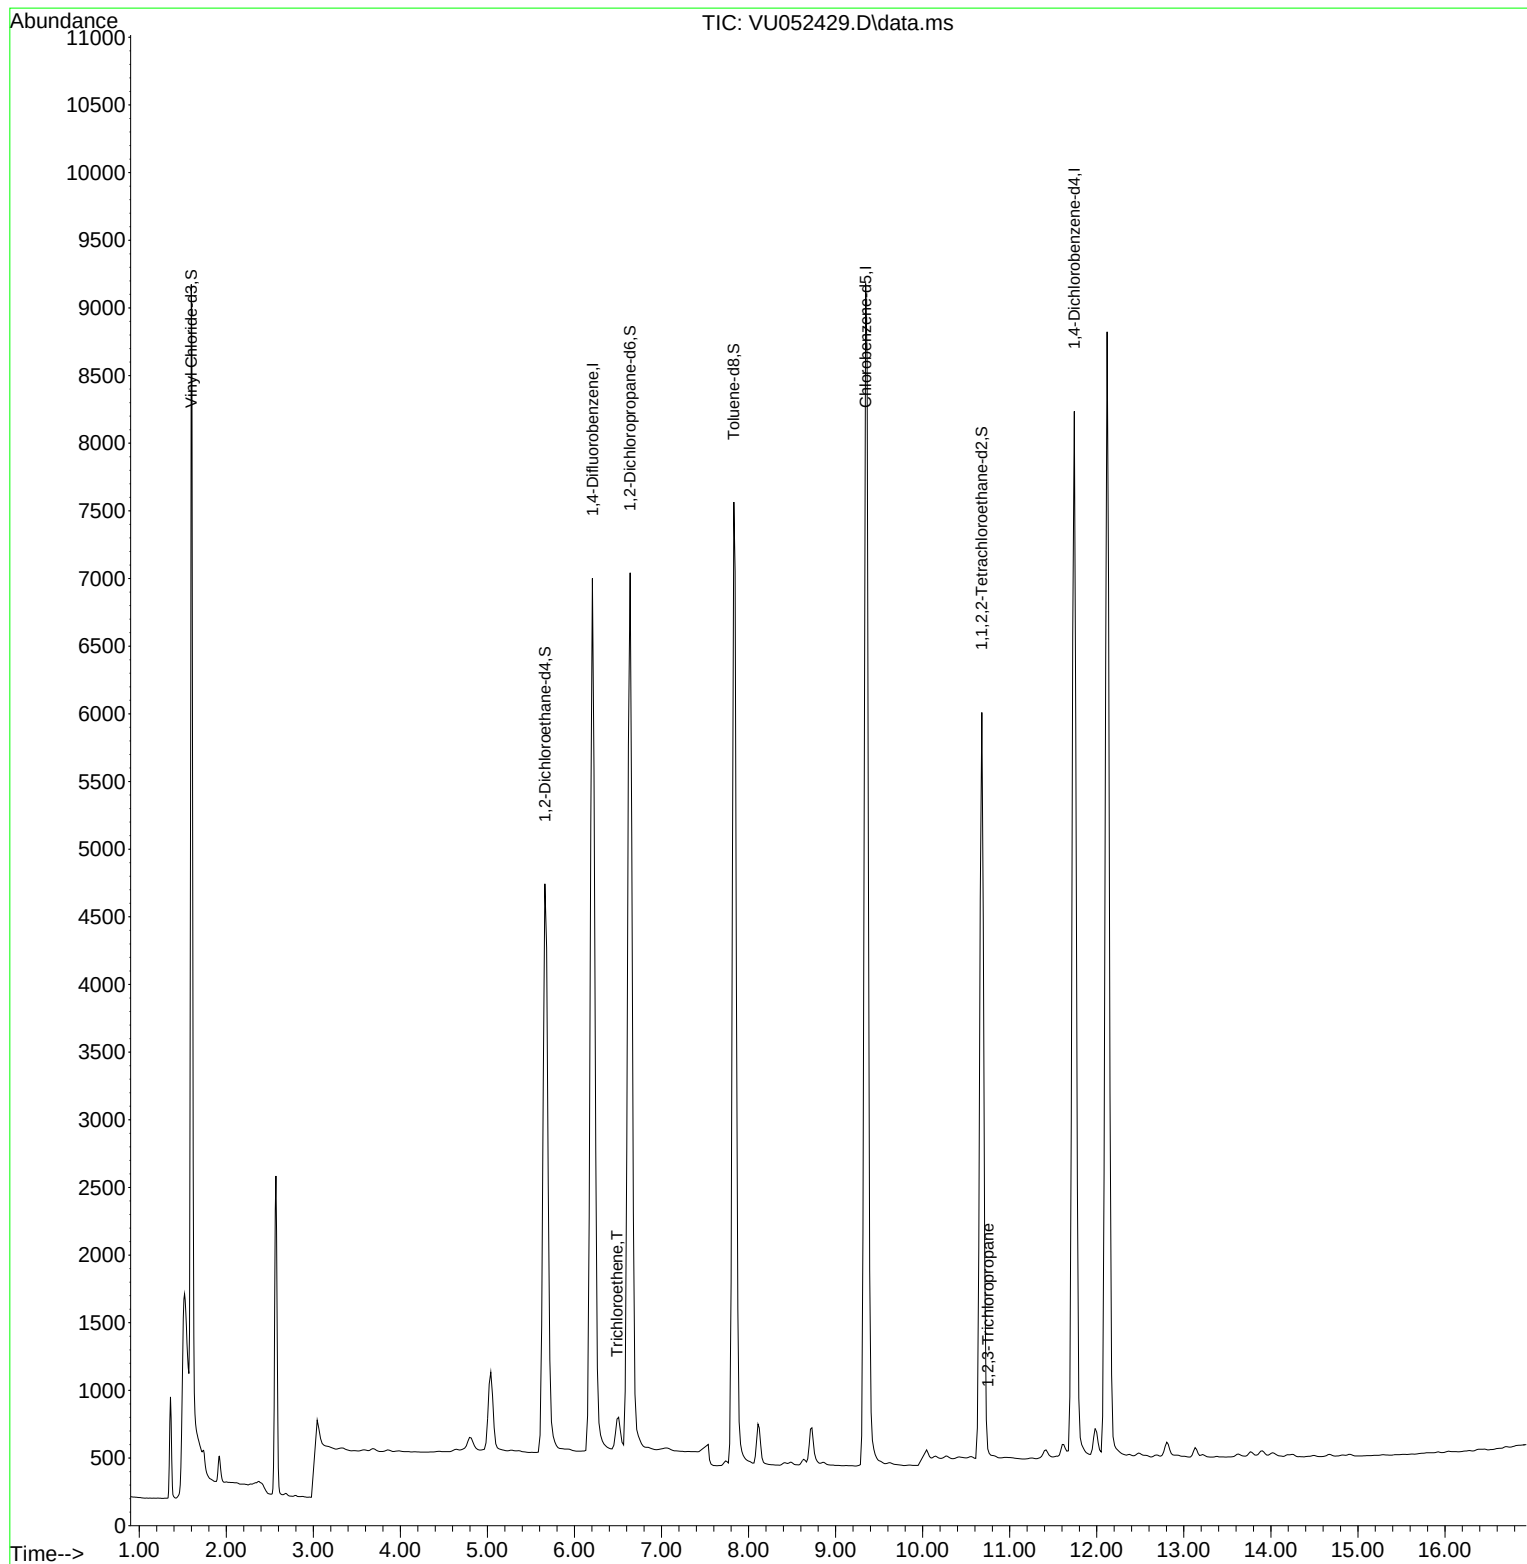


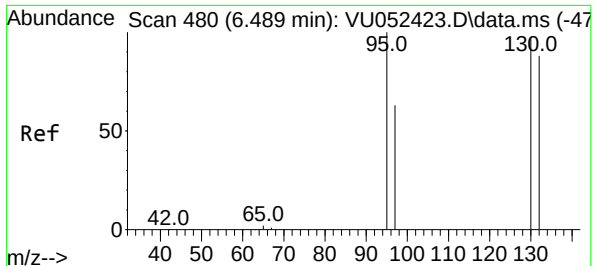

#6
Trichloroethene
Concen: 0.015 ug/L
RT: 6.489 min Scan# 480
Delta R.T. -0.000 min
Lab File: VU052429.D
Acq: 16 Dec 2022 12:15

Tgt Ion: 95 Resp: 262

Ion	Ratio	Lower	Upper
95	100		
97	78.8	43.3	80.3
132	92.9	61.0	113.2
130	94.7	66.7	123.9

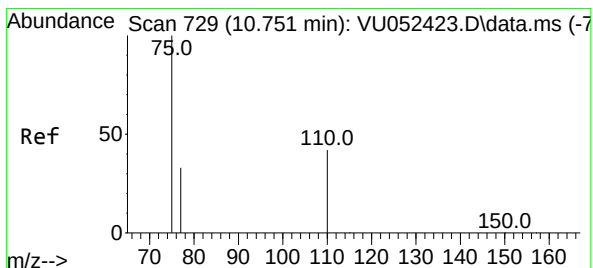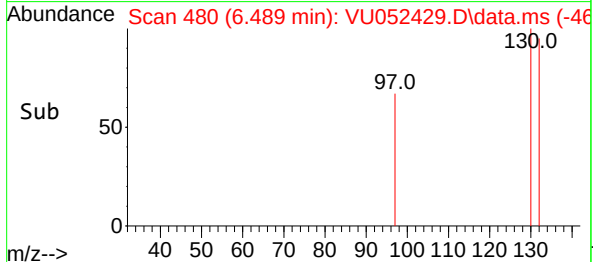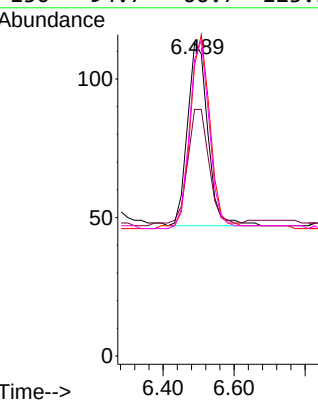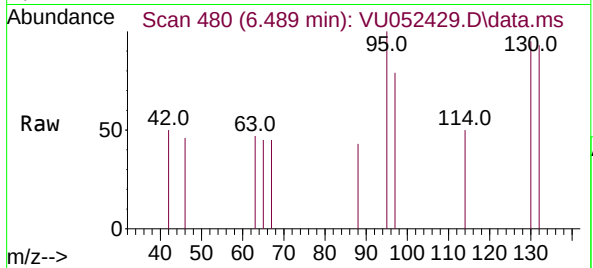

#12
1,2,3-Trichloropropane
Concen: 0.005 ug/L
RT: 10.748 min Scan# 729
Delta R.T. -0.003 min
Lab File: VU052429.D
Acq: 16 Dec 2022 12:15

Tgt Ion: 75 Resp: 61

Ion	Ratio	Lower	Upper
75	100		
110	59.0	32.2	48.2#
77	13.1	26.8	40.2#

