

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052430.D
 Acq On : 16 Dec 2022 12:37
 Operator : JC/MD
 Sample : N6034-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 21:12:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	17425	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.349	117	16081	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.745	152	7955	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	10455	0.509	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.660	65	9229	0.475	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
7) 1,2-Dichloropropane-d6	6.639	67	10943	0.566	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	114.000%
8) Toluene-d8	7.833	98	14545	0.500	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.682	84	11264	0.545	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.000%
Target Compounds						
6) Trichloroethene	6.489	95	234	0.013	ug/L	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052430.D
Acq On : 16 Dec 2022 12:37
Operator : JC/MD
Sample : N6034-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 16 21:12:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

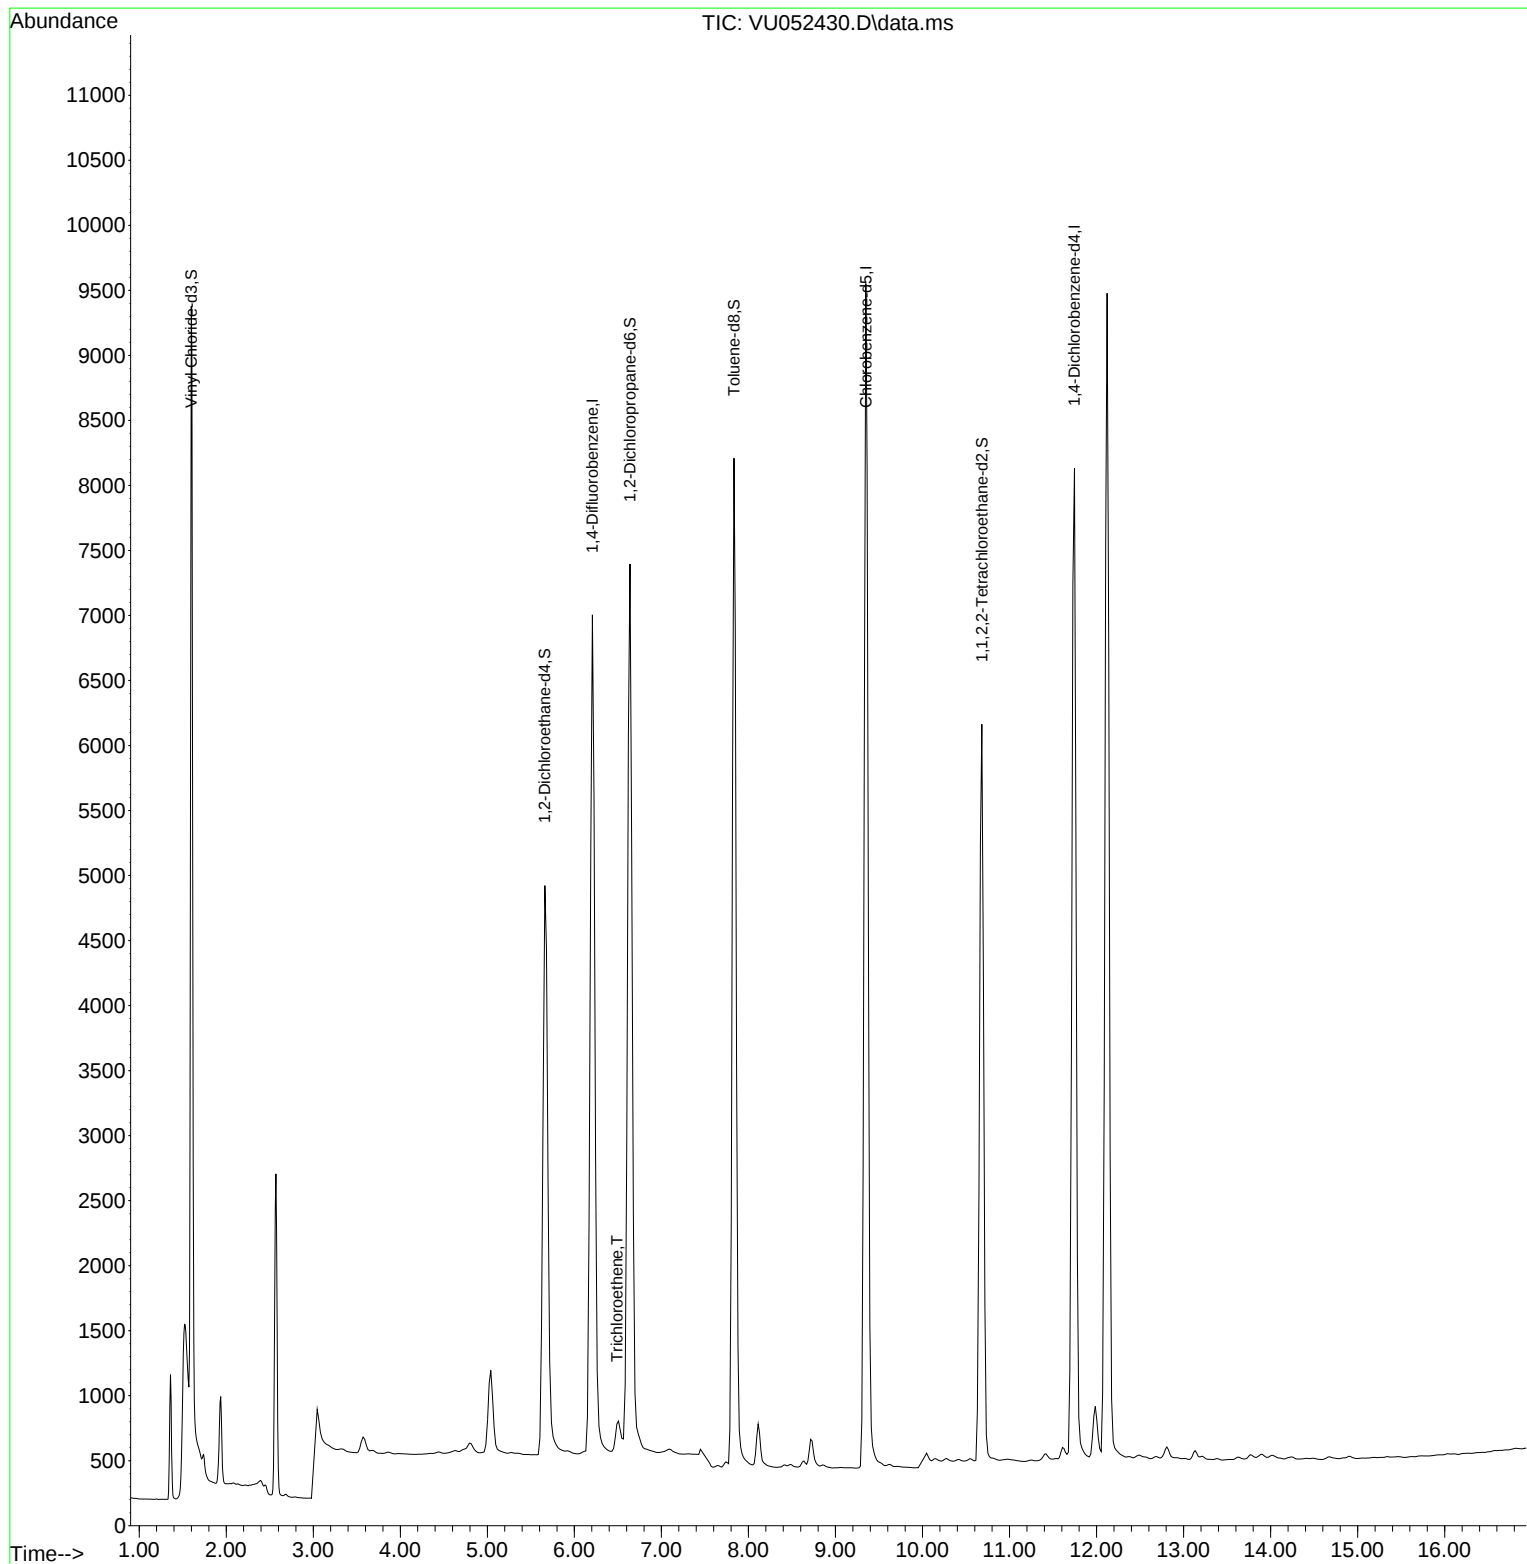

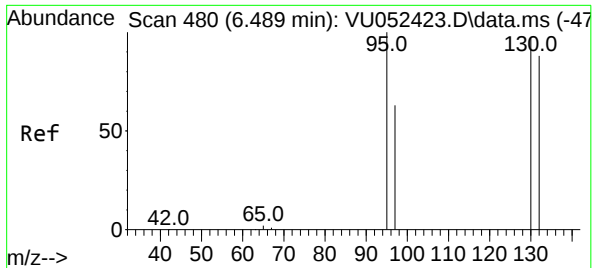

#6
 Trichloroethene
 Concen: 0.013 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052430.D
 Acq: 16 Dec 2022 12:37

Tgt Ion: 95 Resp: 234

Ion	Ratio	Lower	Upper
95	100		
97	79.6	43.3	80.3
132	94.4	61.0	113.2
130	97.2	66.7	123.9

