

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052433.D
 Acq On : 16 Dec 2022 13:42
 Operator : JC/MD
 Sample : N6050-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 21:12:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	17537	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.345	117	16322	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.741	152	8001	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	3444	0.167	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	34.000%#		
4) 1,2-Dichloroethane-d4	5.660	65	8626	0.441	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	88.000%		
7) 1,2-Dichloropropane-d6	6.639	67	10412	0.531	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	106.000%		
8) Toluene-d8	7.830	98	10586	0.358	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	72.000%		
10) 1,1,2,2-Tetrachloroeth...	10.679	84	10609	0.506	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	102.000%		
Target Compounds						
6) Trichloroethene	6.488	95	299	0.016	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052433.D
Acq On : 16 Dec 2022 13:42
Operator : JC/MD
Sample : N6050-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 16 21:12:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

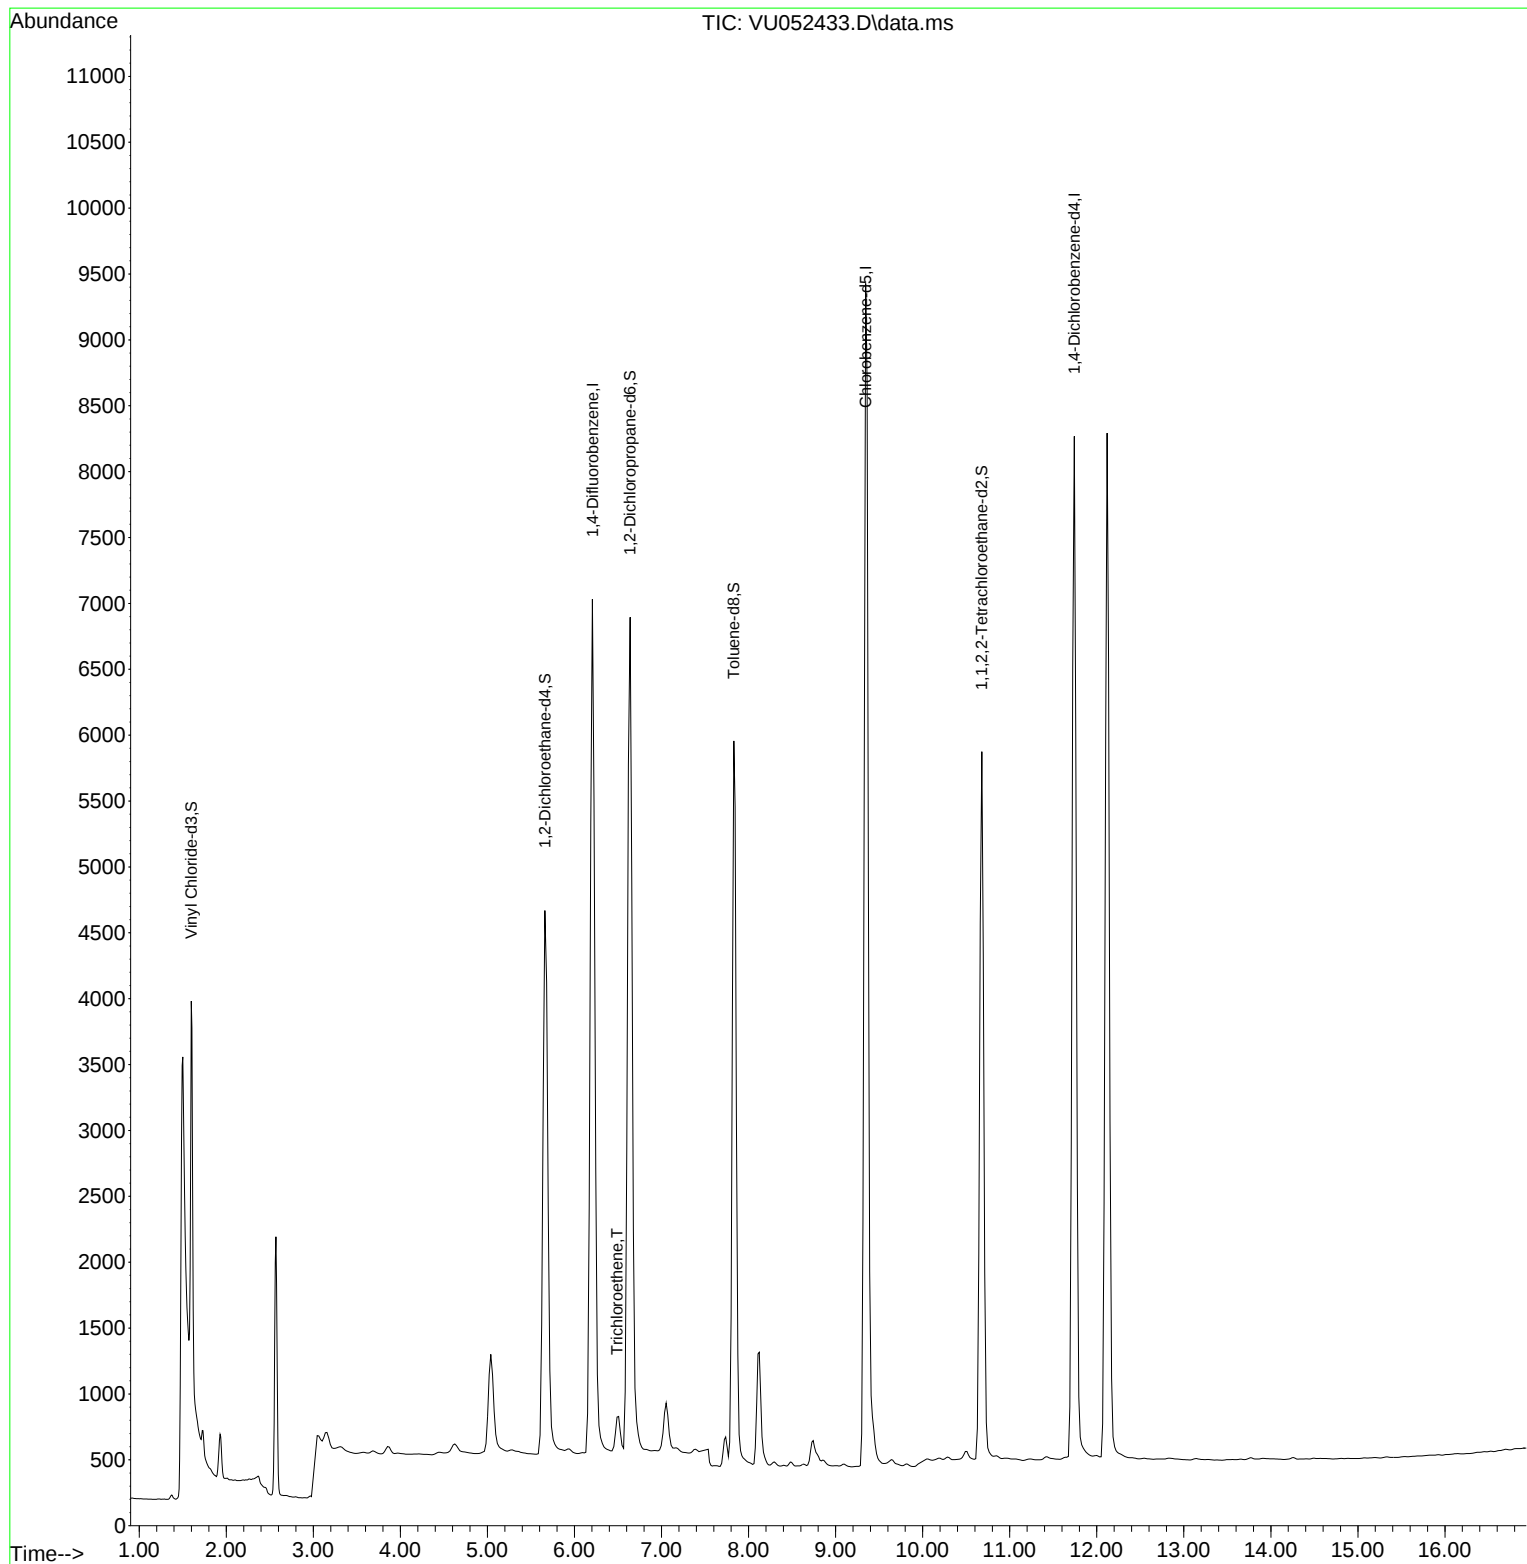

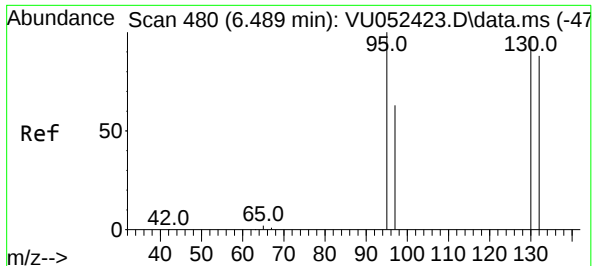

#6
 Trichloroethene
 Concen: 0.016 ug/L
 RT: 6.488 min Scan# 480
 Delta R.T. -0.001 min
 Lab File: VU052433.D
 Acq: 16 Dec 2022 13:42

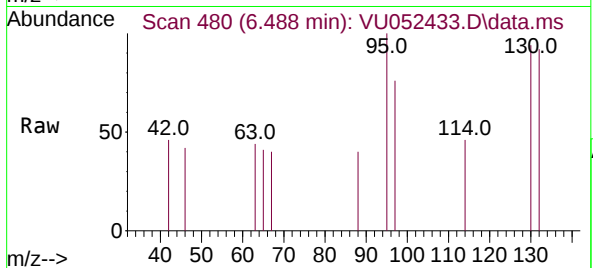

Tgt Ion: 95	Resp: 299
Ion Ratio	Lower Upper
95 100	
97 75.8	43.3 80.3
132 91.9	61.0 113.2
130 94.4	66.7 123.9

