

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052437.D
 Acq On : 16 Dec 2022 15:30
 Operator : JC/MD
 Sample : N6050-01RE
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 16 21:13:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	15401	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	14352	0.500	ug/L	0.01
11) 1,4-Dichlorobenzene-d4	11.741	152	7128	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	497	0.027	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	6.000%#
4) 1,2-Dichloroethane-d4	5.661	65	7636	0.444	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	88.000%
7) 1,2-Dichloropropane-d6	6.639	67	8837	0.512	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	102.000%
8) Toluene-d8	7.830	98	6491	0.250	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	50.000%#
10) 1,1,2,2-Tetrachloroeth...	10.679	84	9548	0.518	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
6) Trichloroethene	6.489	95	480	0.030	ug/L	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052437.D
Acq On : 16 Dec 2022 15:30
Operator : JC/MD
Sample : N6050-01RE
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 16 21:13:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

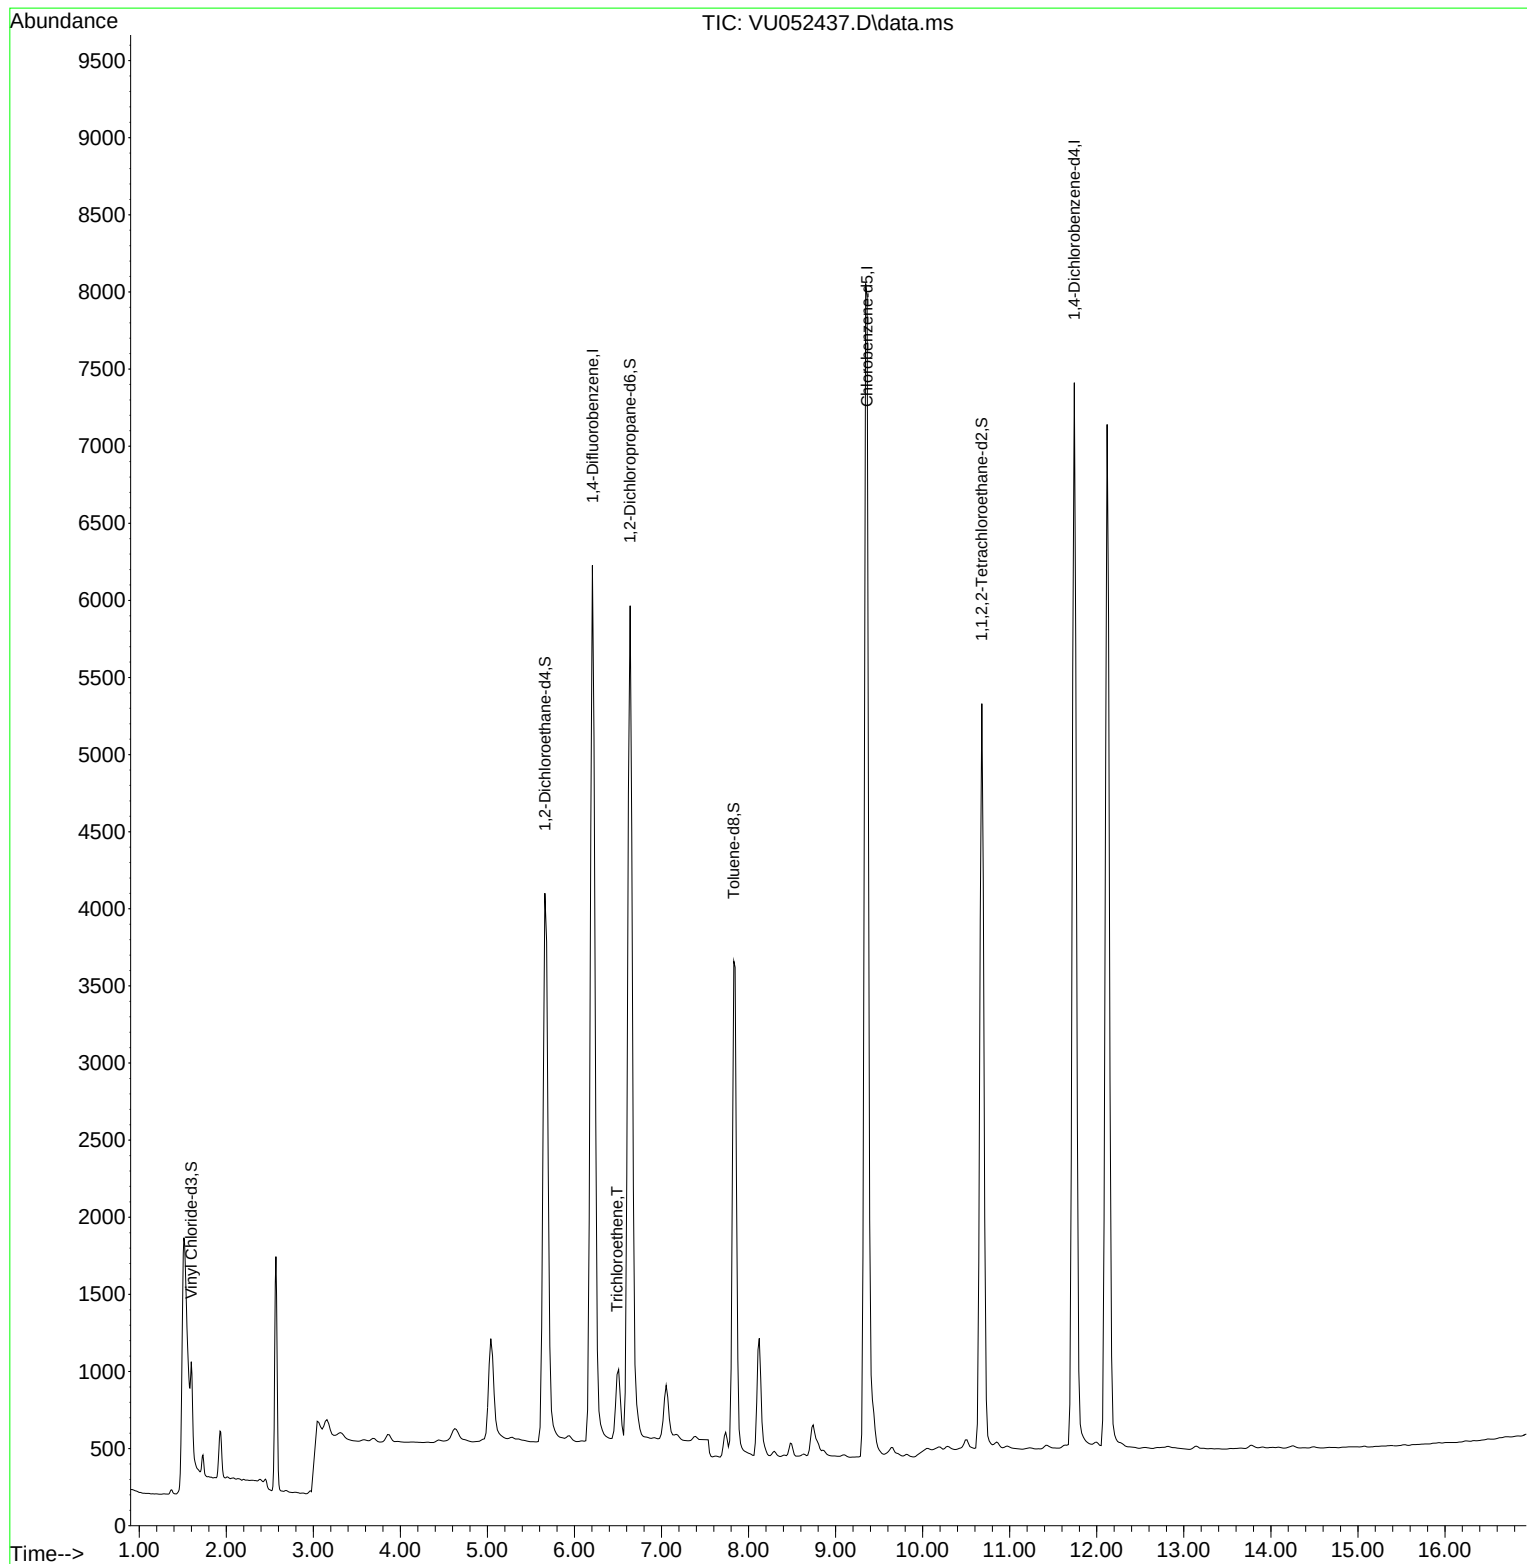

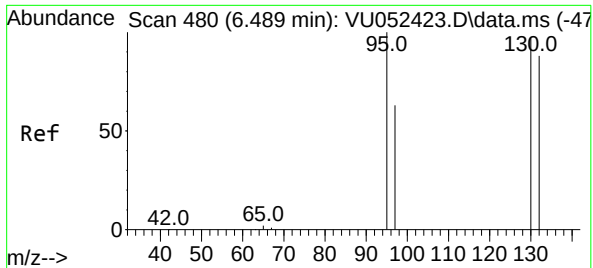

#6
 Trichloroethene
 Concen: 0.030 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052437.D
 Acq: 16 Dec 2022 15:30

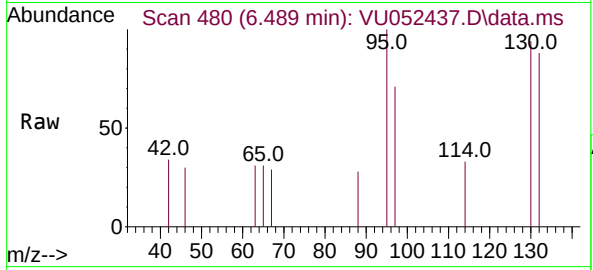

Tgt Ion: 95 Resp: 480

Ion	Ratio	Lower	Upper
95	100		
97	71.3	43.3	80.3
132	88.3	61.0	113.2
130	94.2	66.7	123.9

