

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052438.D
 Acq On : 16 Dec 2022 15:53
 Operator : JC/MD
 Sample : N6050-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 16 21:13:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	16793	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	15038	0.500	ug/L	0.01
11) 1,4-Dichlorobenzene-d4	11.742	152	7348	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.599	65	10097	0.510	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 102.000%			
4) 1,2-Dichloroethane-d4	5.661	65	9013	0.481	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 96.000%			
7) 1,2-Dichloropropane-d6	6.639	67	10372	0.574	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 114.000%			
8) Toluene-d8	7.830	98	13314	0.489	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 98.000%			
10) 1,1,2,2-Tetrachloroeth...	10.679	84	10986	0.568	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 114.000%			
Target Compounds						
						Qvalue
6) Trichloroethene	6.489	95	287	0.017	ug/L	95
13) 1,2-Dibromo-3-chloropr...	12.907	75	40	0.016	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052438.D
Acq On : 16 Dec 2022 15:53
Operator : JC/MD
Sample : N6050-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 16 21:13:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration




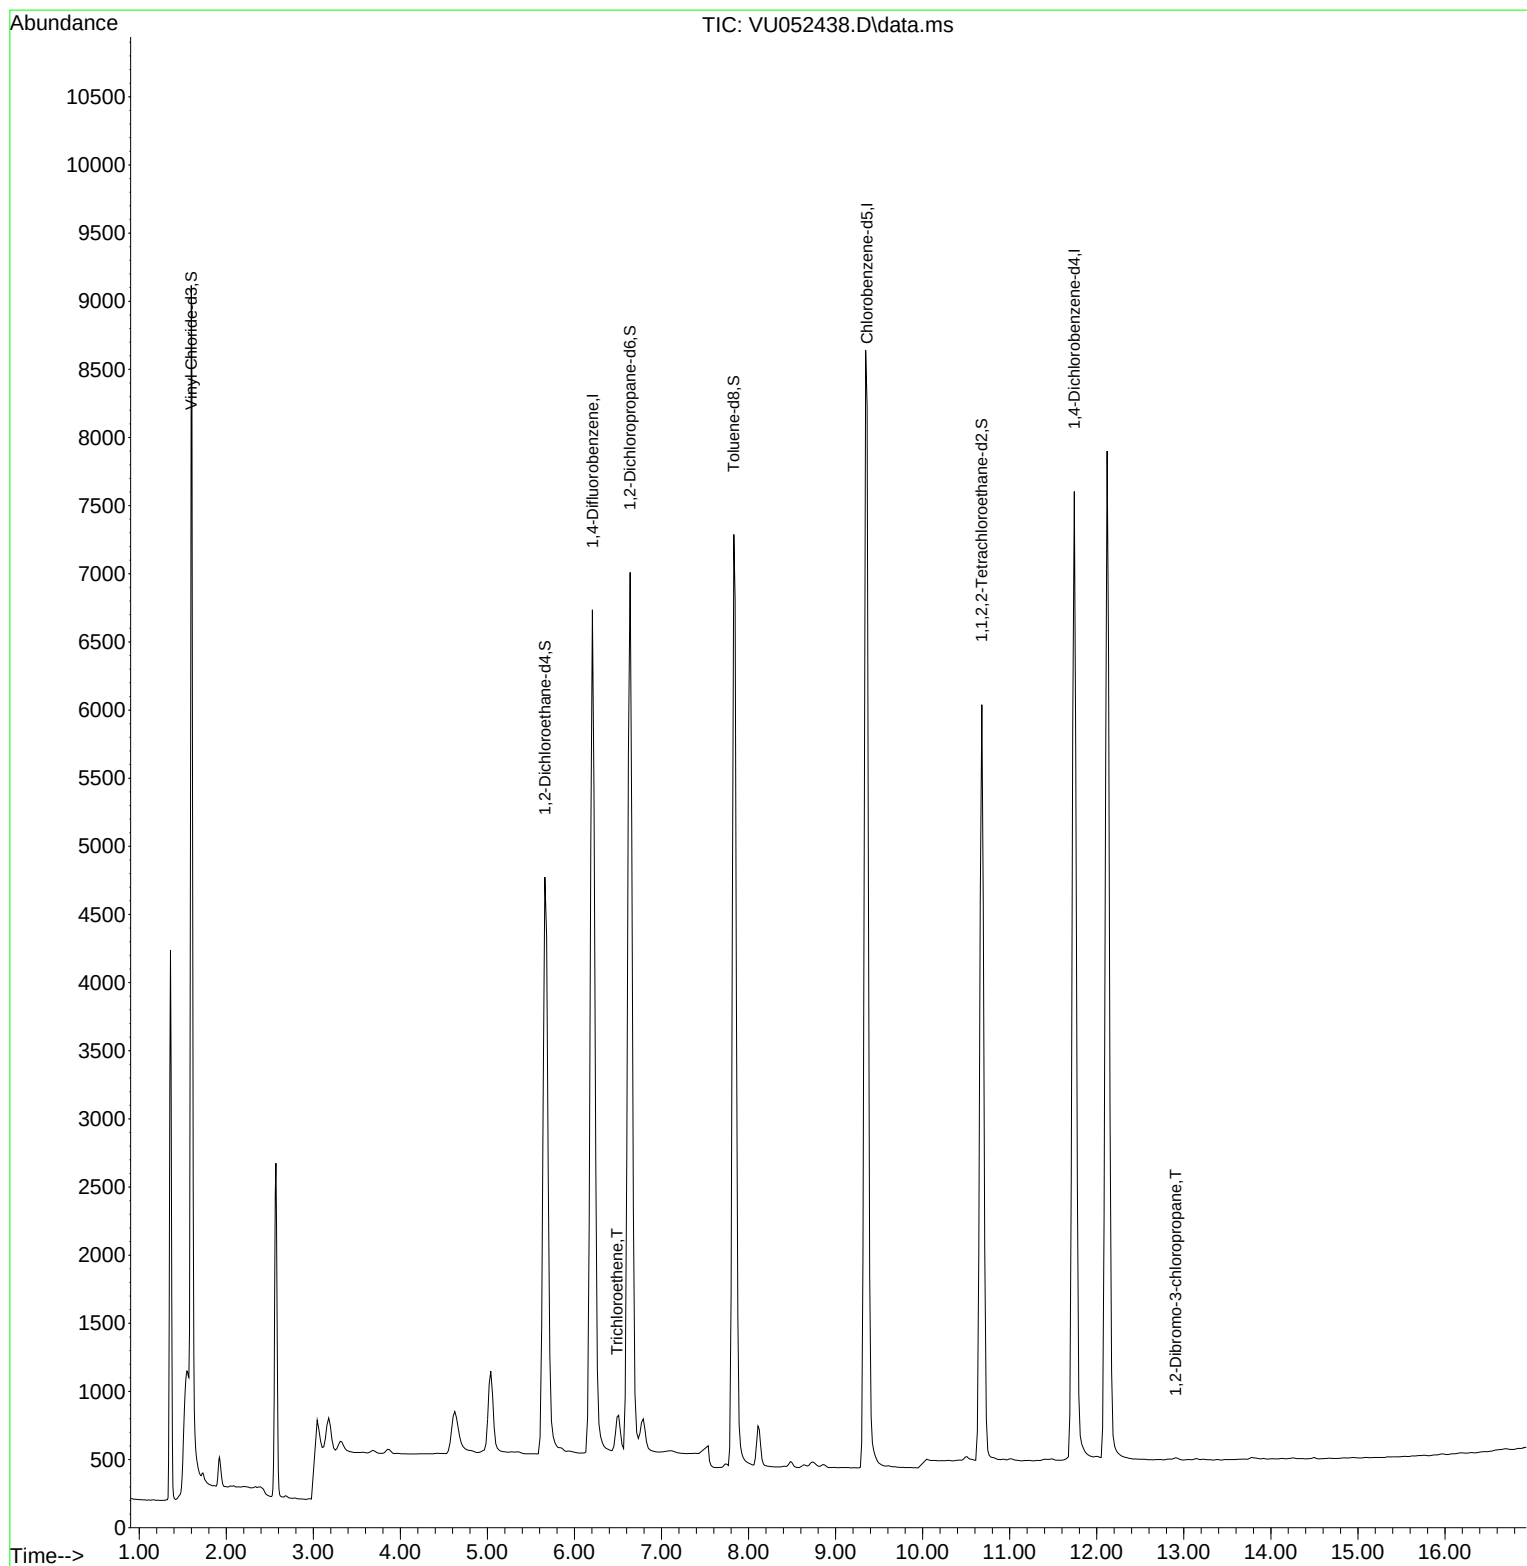


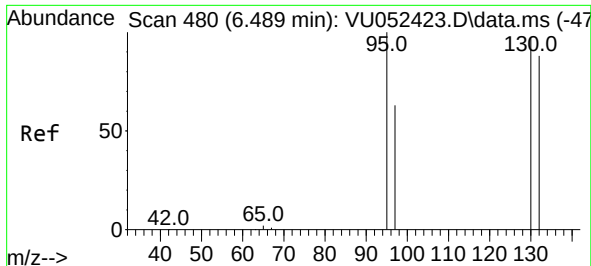

#6
 Trichloroethene
 Concen: 0.017 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052438.D
 Acq: 16 Dec 2022 15:53

Tgt Ion: 95 Resp: 287

Ion	Ratio	Lower	Upper
95	100		
97	75.4	43.3	80.3
132	88.5	61.0	113.2
130	95.9	66.7	123.9

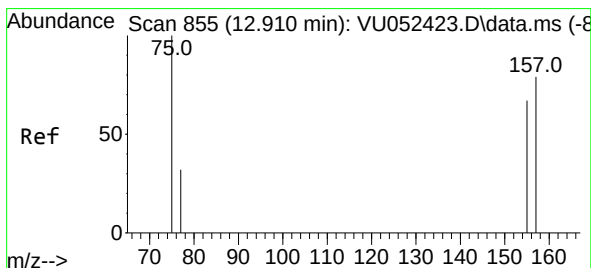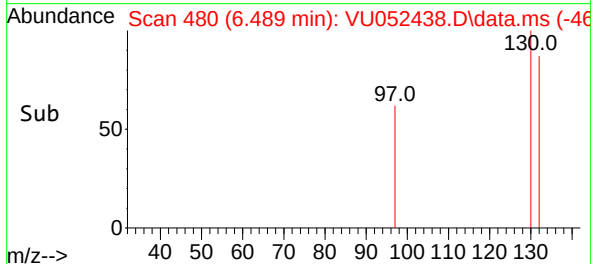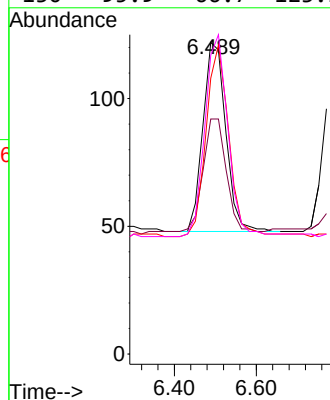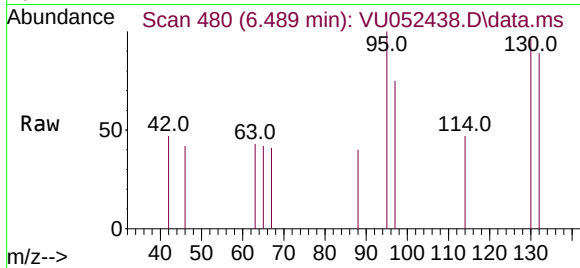

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.016 ug/L
 RT: 12.907 min Scan# 855
 Delta R.T. -0.003 min
 Lab File: VU052438.D
 Acq: 16 Dec 2022 15:53

Tgt Ion: 75 Resp: 40

Ion	Ratio	Lower	Upper
75	100		
157	74.6	62.8	94.2
155	74.6	54.4	81.6

