

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052439.D
 Acq On : 16 Dec 2022 16:17
 Operator : JC/MD
 Sample : N6050-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Dec 16 21:13:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	17059	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	15429	0.500	ug/L	0.01
11) 1,4-Dichlorobenzene-d4	11.742	152	7509	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.599	65	10797	0.537	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 108.000%			
4) 1,2-Dichloroethane-d4	5.661	65	9053	0.475	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 96.000%			
7) 1,2-Dichloropropane-d6	6.639	67	10618	0.573	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 114.000%			
8) Toluene-d8	7.830	98	13530	0.484	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 96.000%			
10) 1,1,2,2-Tetrachloroeth...	10.679	84	11094	0.559	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 112.000%			
Target Compounds						
6) Trichloroethene	6.489	95	192	0.011	ug/L	Qvalue # 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052439.D
Acq On : 16 Dec 2022 16:17
Operator : JC/MD
Sample : N6050-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Dec 16 21:13:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

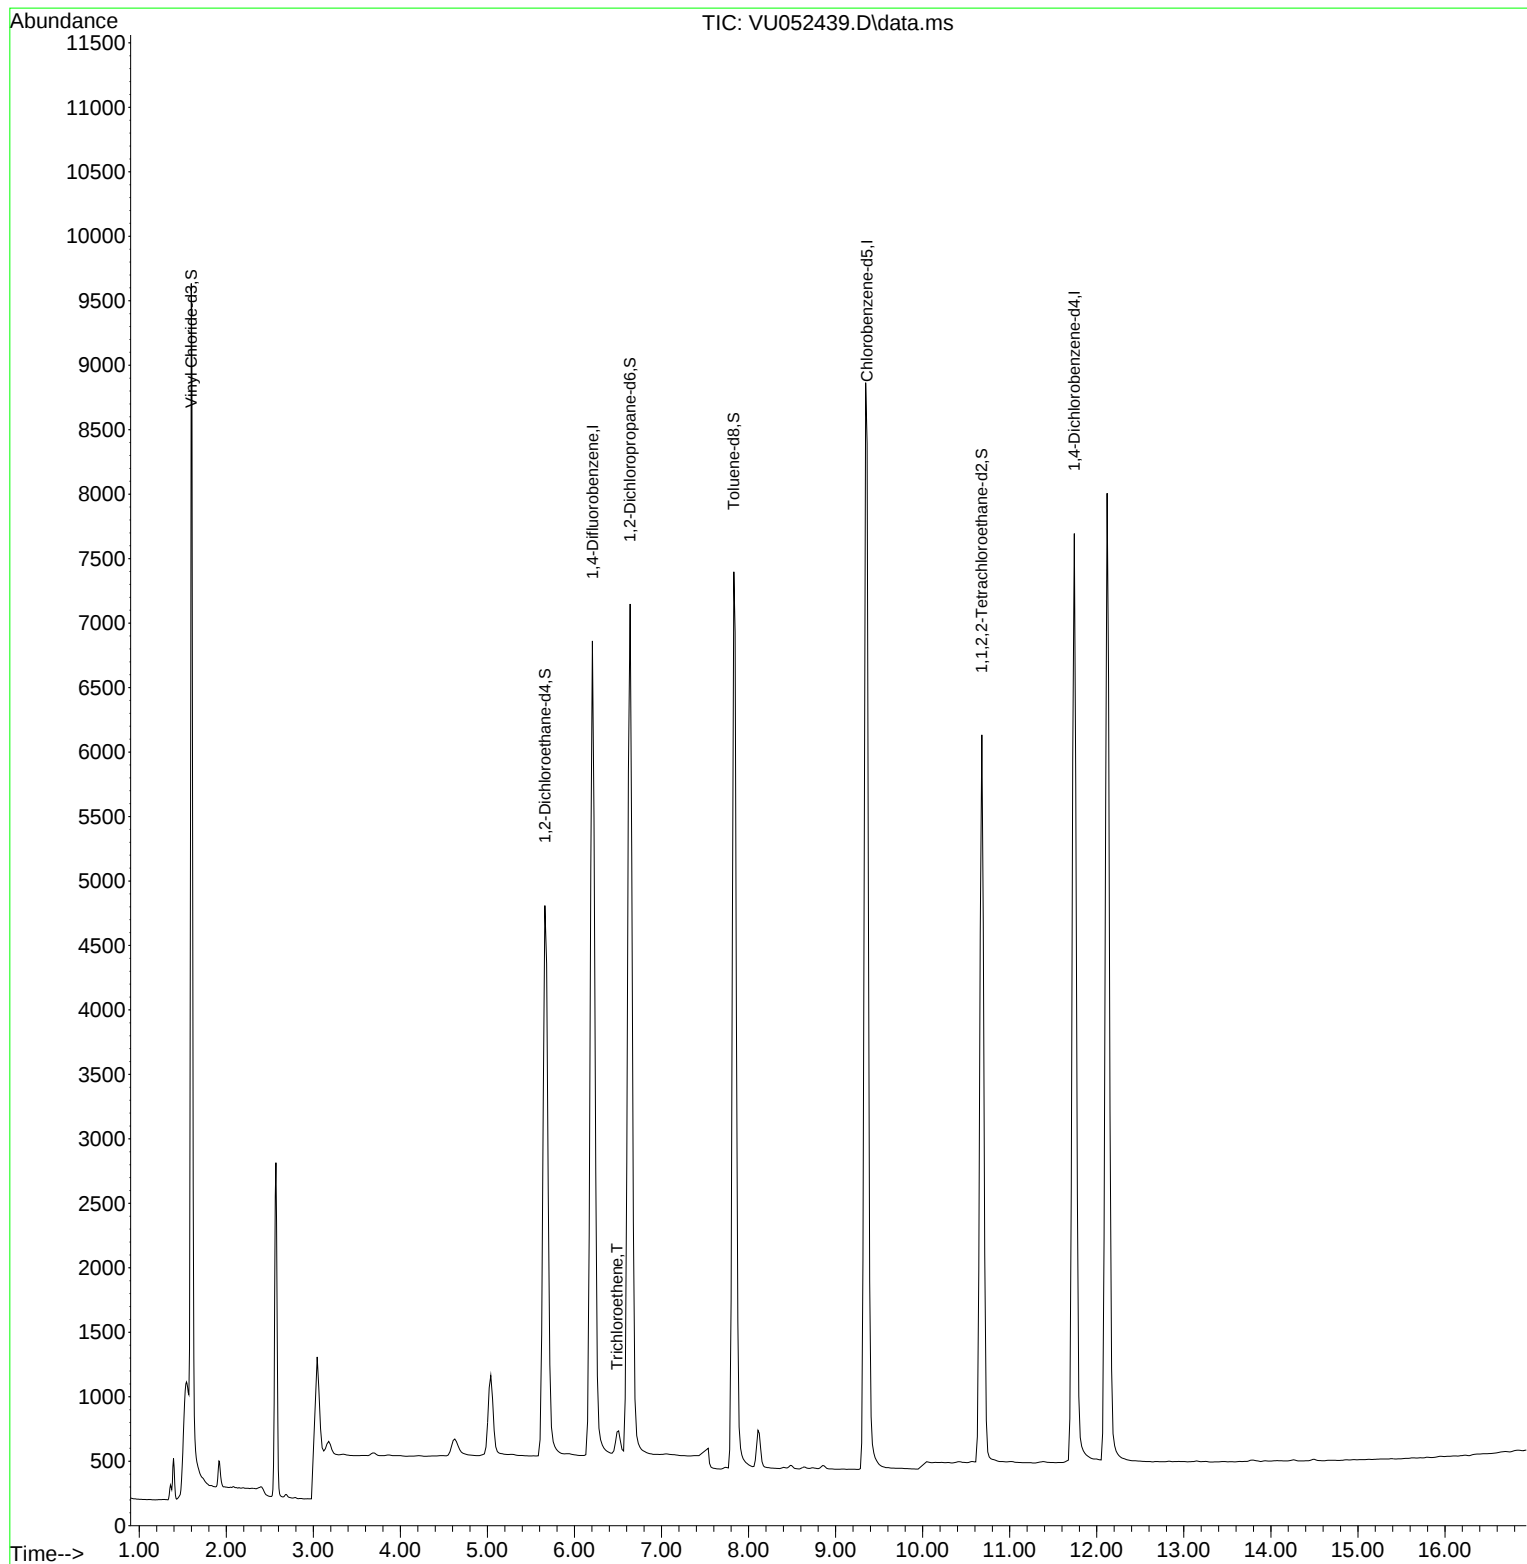

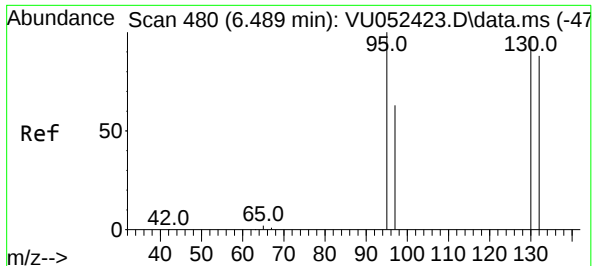

#6
 Trichloroethene
 Concen: 0.011 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052439.D
 Acq: 16 Dec 2022 16:17

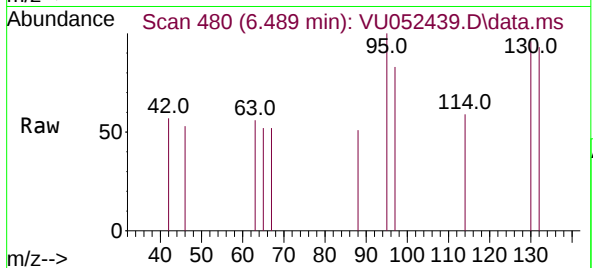

Tgt Ion: 95	Resp: 192
Ion Ratio	Lower Upper
95 100	
97 83.3	43.3 80.3#
132 92.7	61.0 113.2
130 95.8	66.7 123.9

