

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052444.D
 Acq On : 16 Dec 2022 18:14
 Operator : JC/MD
 Sample : N6034-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 16 21:14:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	15922	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.346	117	14537	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.742	152	7201	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	12461	0.664	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	132.000%#
4) 1,2-Dichloroethane-d4	5.661	65	11111	0.625	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	126.000%
7) 1,2-Dichloropropane-d6	6.639	67	13130	0.752	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	150.000%#
8) Toluene-d8	7.830	98	16209	0.616	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	124.000%
10) 1,1,2,2-Tetrachloroeth...	10.679	84	13831	0.740	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	148.000%#
Target Compounds						
6) Trichloroethene	6.489	95	208	0.013	ug/L	Qvalue # 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052444.D
Acq On : 16 Dec 2022 18:14
Operator : JC/MD
Sample : N6034-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 16 21:14:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

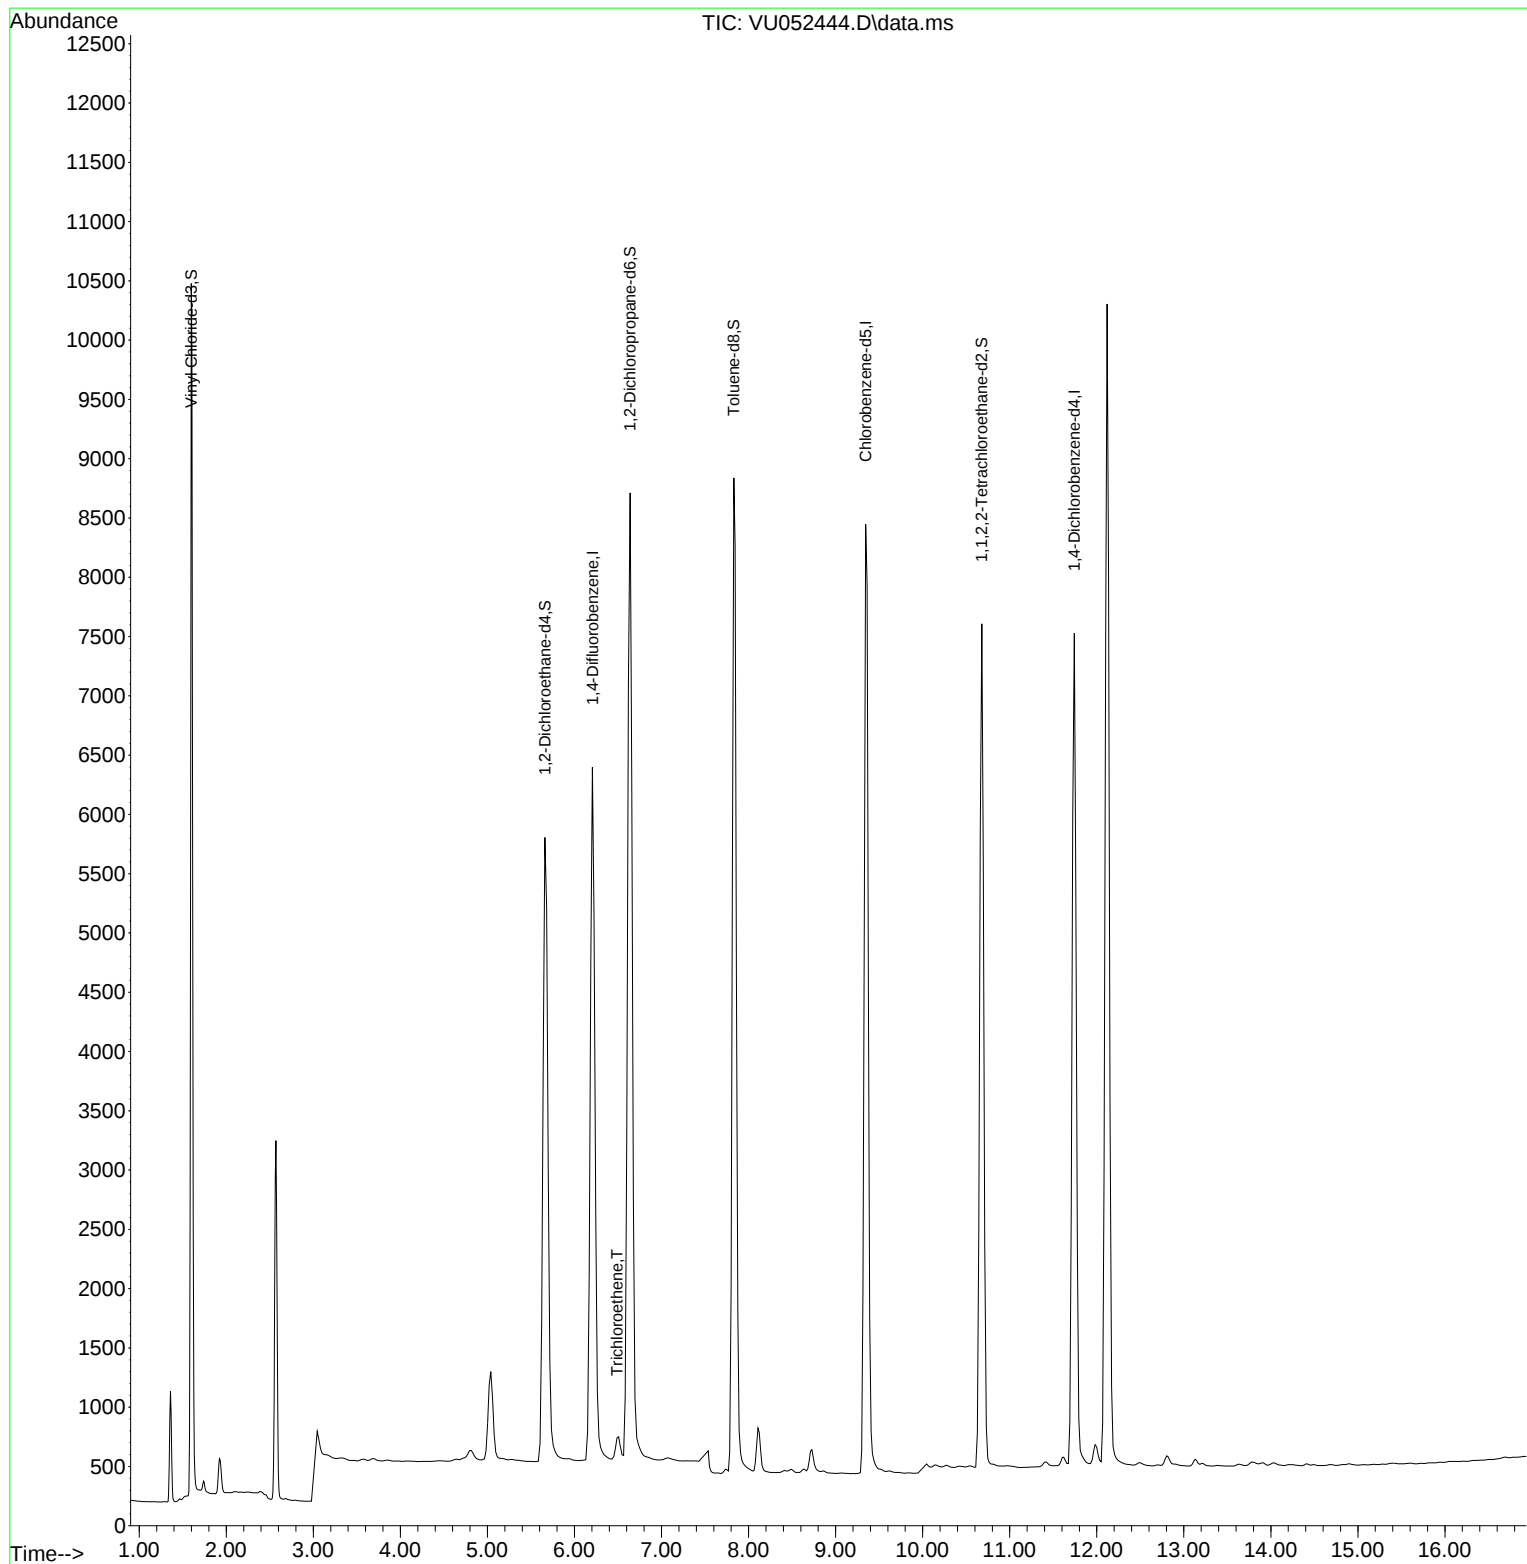

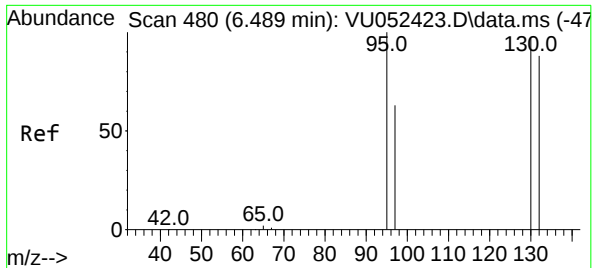

#6
 Trichloroethene
 Concen: 0.013 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052444.D
 Acq: 16 Dec 2022 18:14

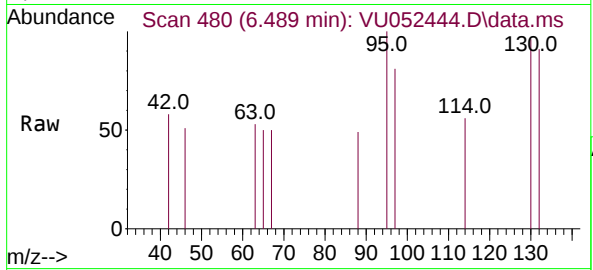

Tgt Ion: 95	Resp: 208
Ion Ratio	Lower Upper
95 100	
97 81.0	43.3 80.3#
132 91.0	61.0 113.2
130 96.0	66.7 123.9

