

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052447.D
 Acq On : 16 Dec 2022 19:24
 Operator : JC/MD
 Sample : N6034-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Quant Time: Dec 16 21:14:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	14963	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.349	117	13323	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.745	152	6462	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.599	65	8978	0.509	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.661	65	8294	0.497	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
7) 1,2-Dichloropropane-d6	6.639	67	9202	0.575	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	114.000%
8) Toluene-d8	7.833	98	11159	0.463	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
10) 1,1,2,2-Tetrachloroeth...	10.682	84	10003	0.584	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	116.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.606	62	351	0.018	ug/L #	3
6) Trichloroethene	6.489	95	3699	0.248	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052447.D
Acq On : 16 Dec 2022 19:24
Operator : JC/MD
Sample : N6034-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1





Quant Time: Dec 16 21:14:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

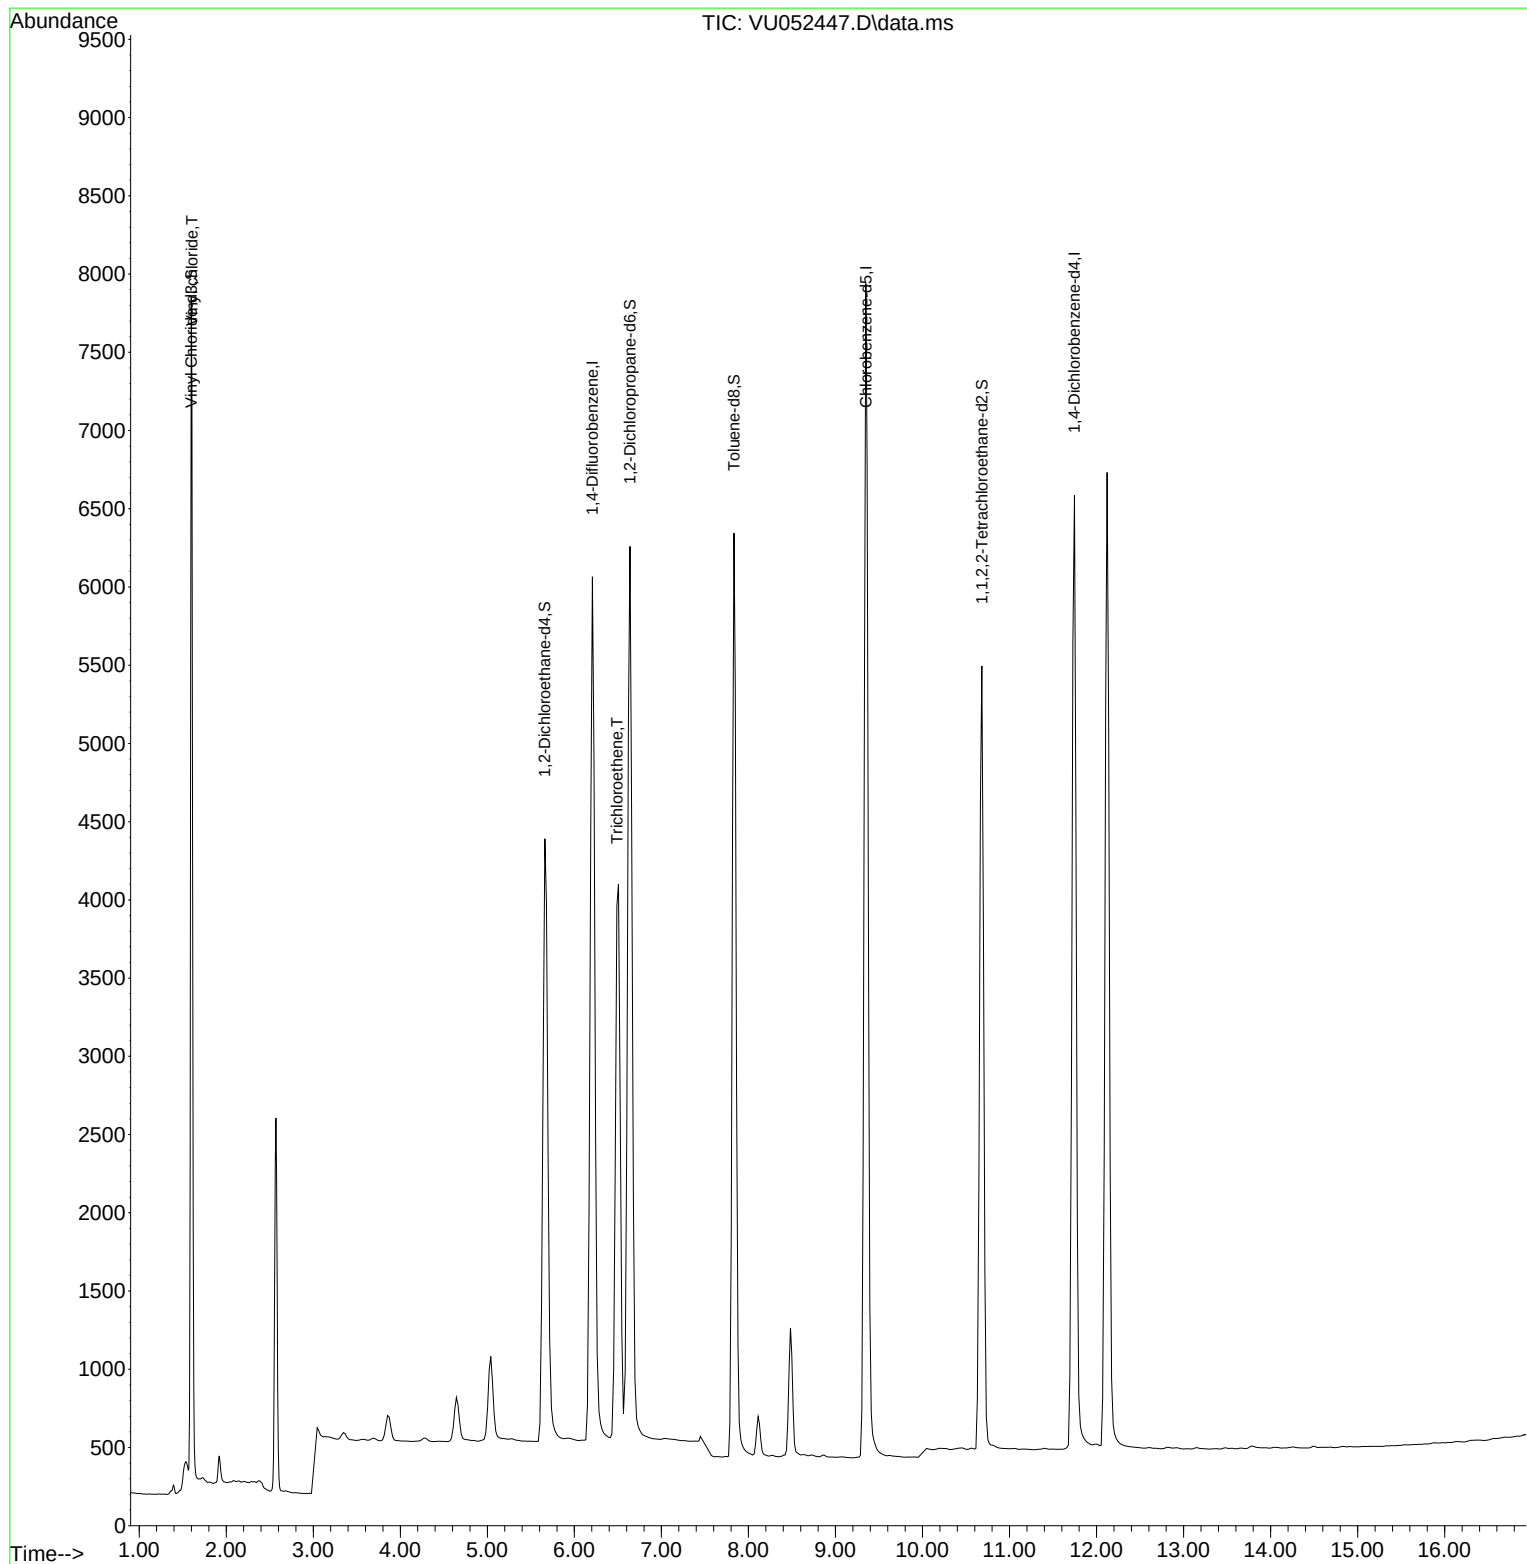

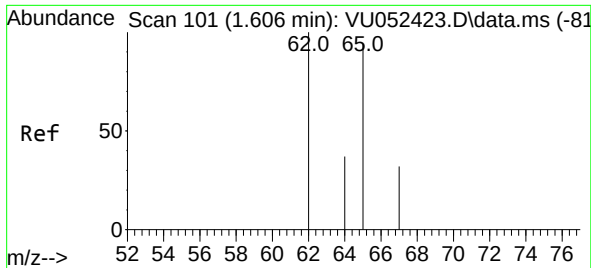

#3
 Vinyl chloride
 Concen: 0.018 ug/L
 RT: 1.606 min Scan# 101
 Delta R.T. 0.007 min
 Lab File: VU052447.D
 Acq: 16 Dec 2022 19:24

Tgt Ion: 62 Resp: 351
 Ion Ratio Lower Upper
 62 100
 64 89.0 23.7 43.9#

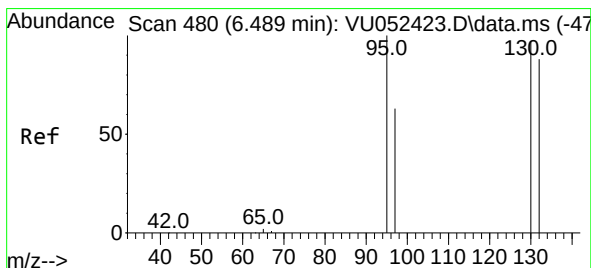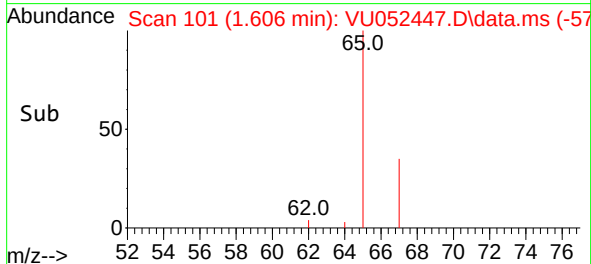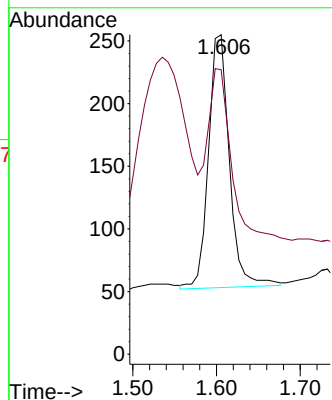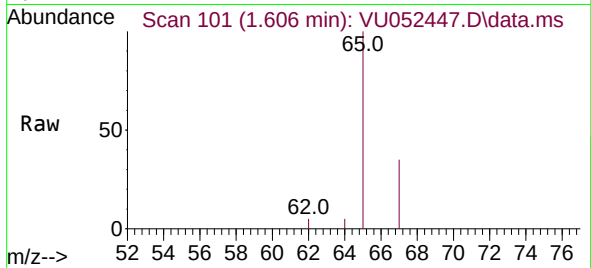

#6
 Trichloroethene
 Concen: 0.248 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052447.D
 Acq: 16 Dec 2022 19:24

Tgt Ion: 95 Resp: 3699
 Ion Ratio Lower Upper
 95 100
 97 65.0 43.3 80.3
 132 89.8 61.0 113.2
 130 97.6 66.7 123.9

