

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052449.D
 Acq On : 16 Dec 2022 20:09
 Operator : JC/MD
 Sample : N6034-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: Dec 16 21:14:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	15516	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.346	117	14778	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.742	152	6806	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	9868	0.540	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	108.000%
4) 1,2-Dichloroethane-d4	5.661	65	8643	0.499	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
7) 1,2-Dichloropropane-d6	6.639	67	9786	0.551	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	110.000%
8) Toluene-d8	7.830	98	12384	0.463	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
10) 1,1,2,2-Tetrachloroeth...	10.679	84	10544	0.555	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	112.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.606	62	7012	0.354	ug/L	95
6) Trichloroethene	6.489	95	113677	6.872	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052449.D
Acq On : 16 Dec 2022 20:09
Operator : JC/MD
Sample : N6034-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1





Quant Time: Dec 16 21:14:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

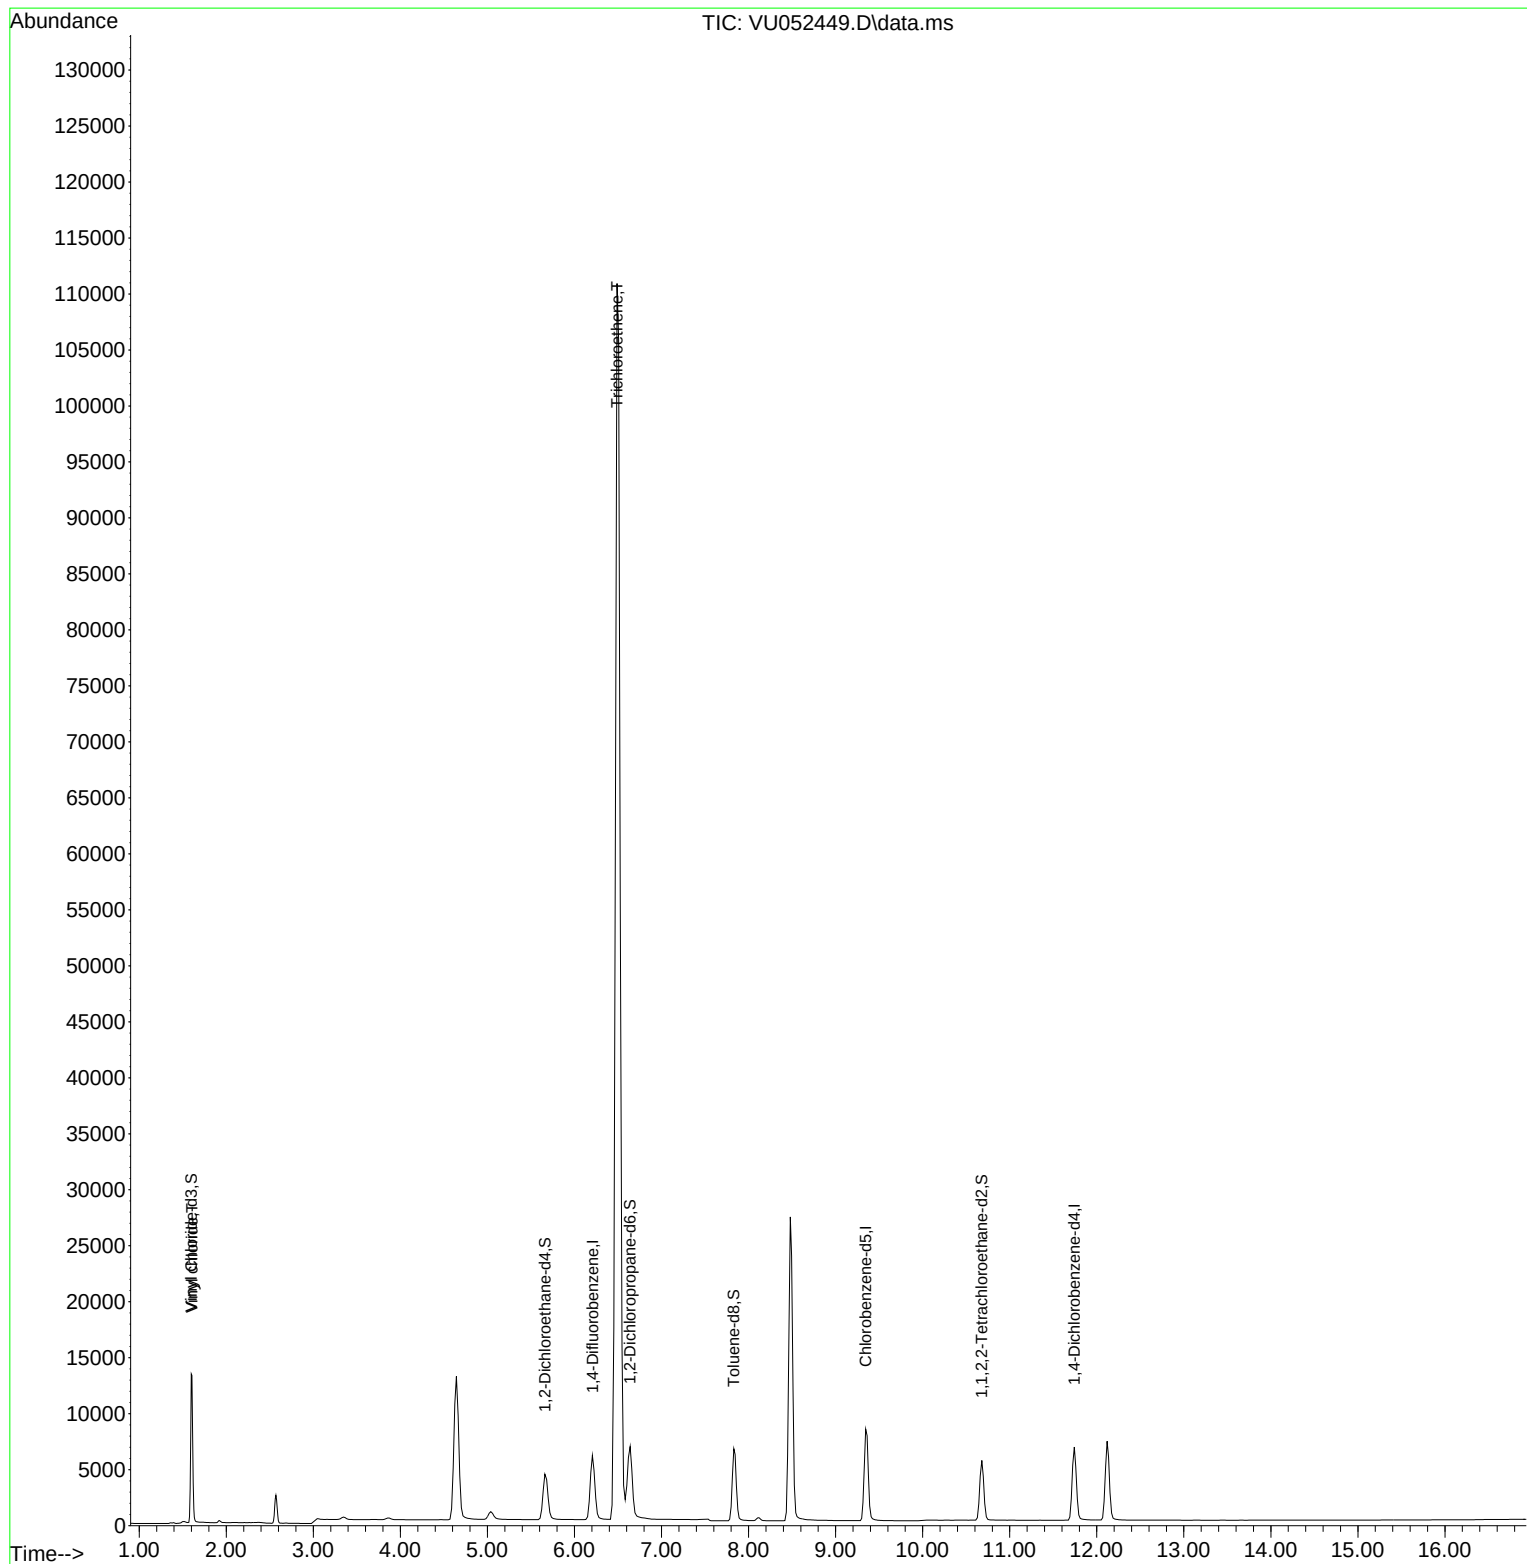

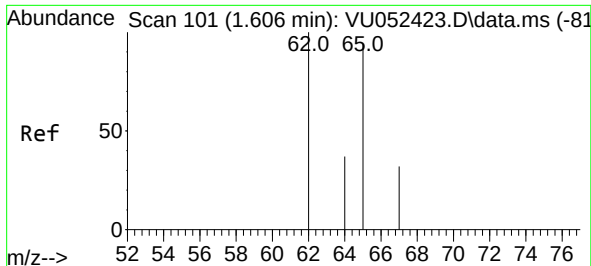

#3
 Vinyl chloride
 Concen: 0.354 ug/L
 RT: 1.606 min Scan# 101
 Delta R.T. 0.007 min
 Lab File: VU052449.D
 Acq: 16 Dec 2022 20:09

Tgt Ion: 62 Resp: 7012
 Ion Ratio Lower Upper
 62 100
 64 36.8 23.7 43.9

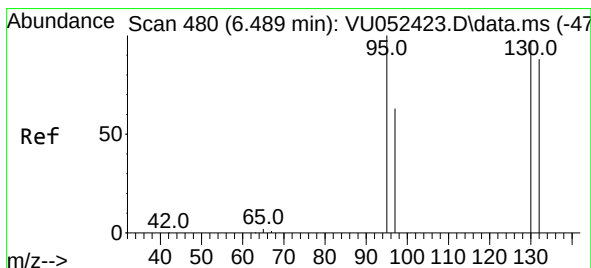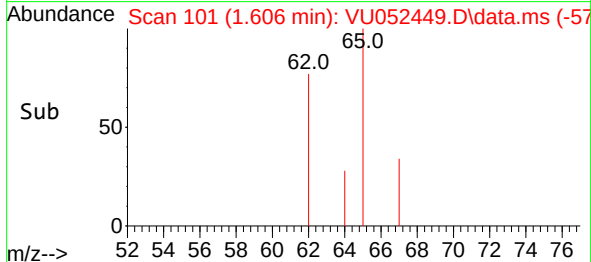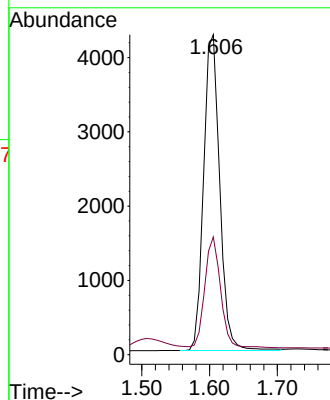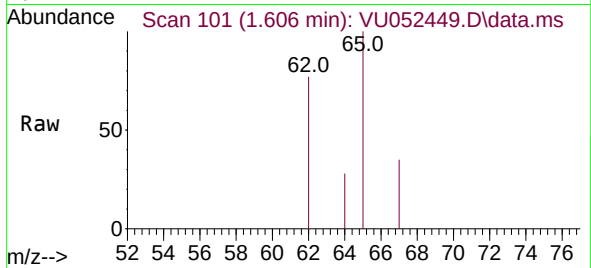

#6
 Trichloroethene
 Concen: 6.872 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052449.D
 Acq: 16 Dec 2022 20:09

Tgt Ion: 95 Resp: 113677
 Ion Ratio Lower Upper
 95 100
 97 63.3 43.3 80.3
 132 92.0 61.0 113.2
 130 98.3 66.7 123.9

