
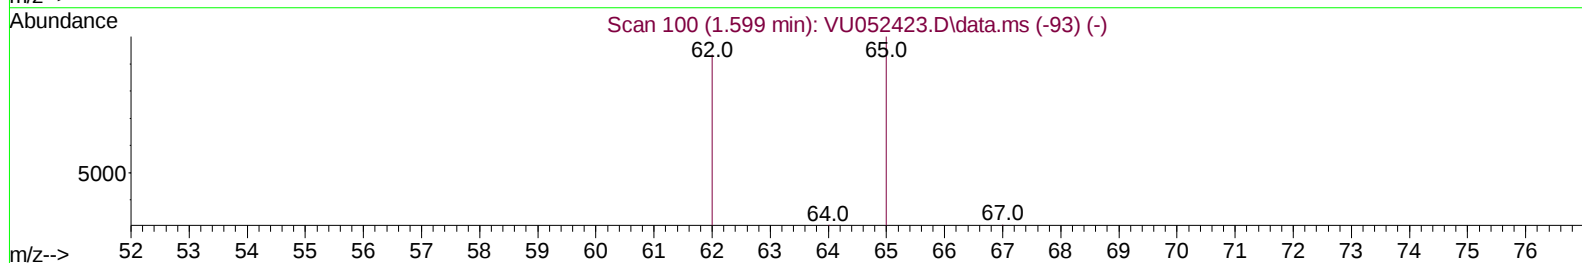
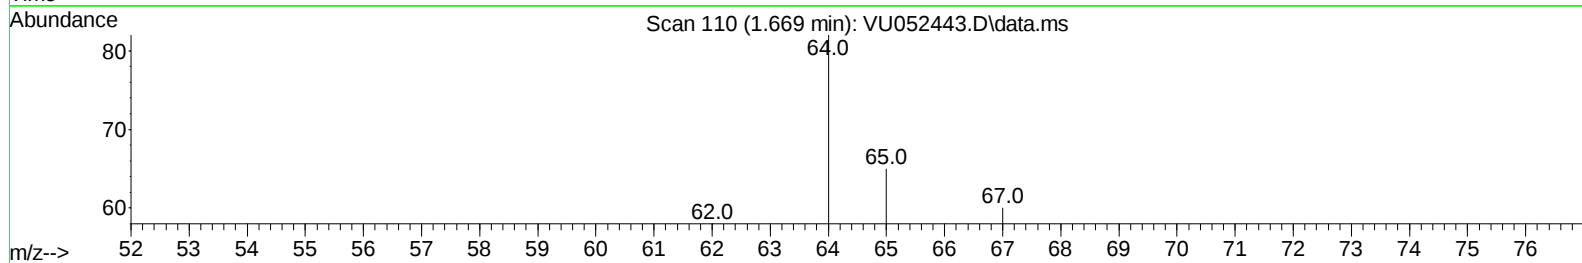


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052443.D
Acq On : 16 Dec 2022 17:51
Operator : JC/MD
Sample : N6034-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 16 21:13:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

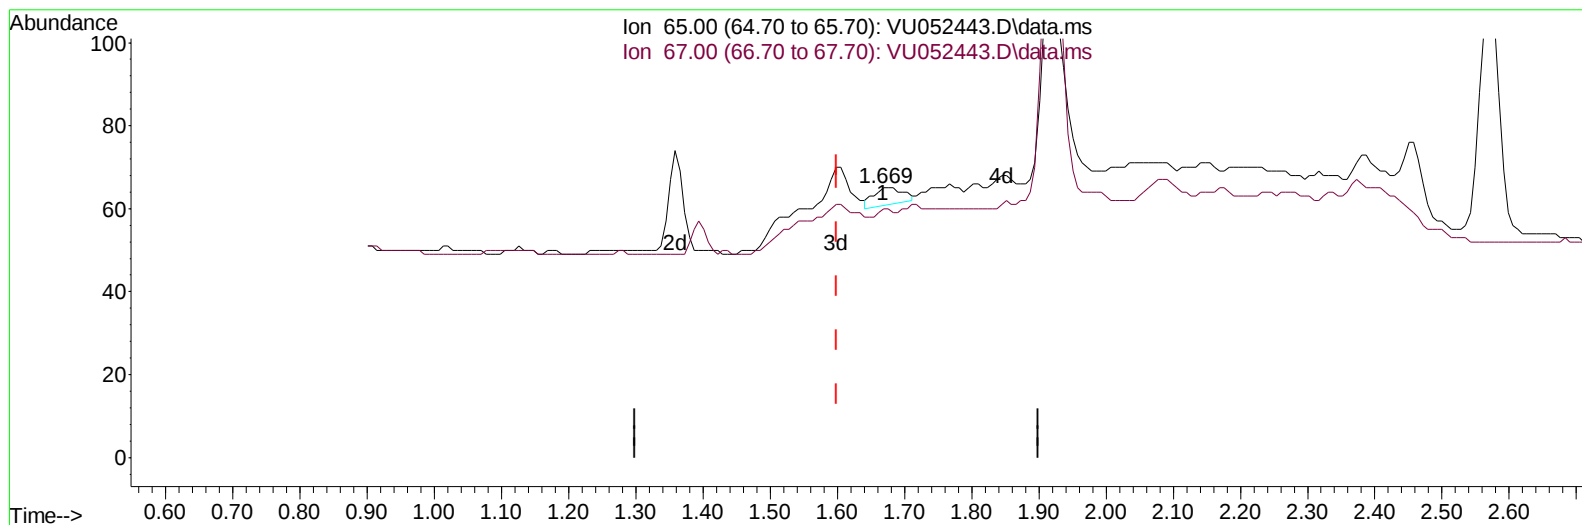

TIC: VU052443.D\data.ms

(2) Vinyl Chloride-d3 (S)




1.669min (+ 0.070) 0.00 ug/L

response 13

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	32.90	23.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052443.D
Acq On : 16 Dec 2022 17:51
Operator : JC/MD
Sample : N6034-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 16 21:13:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

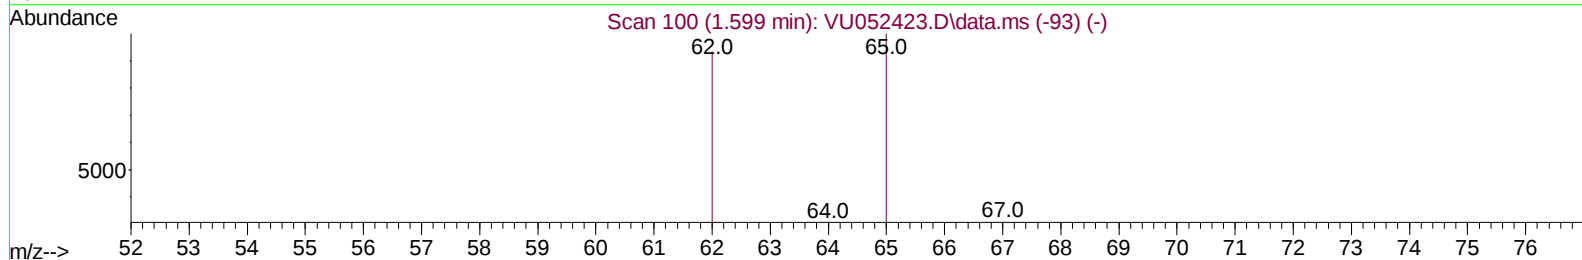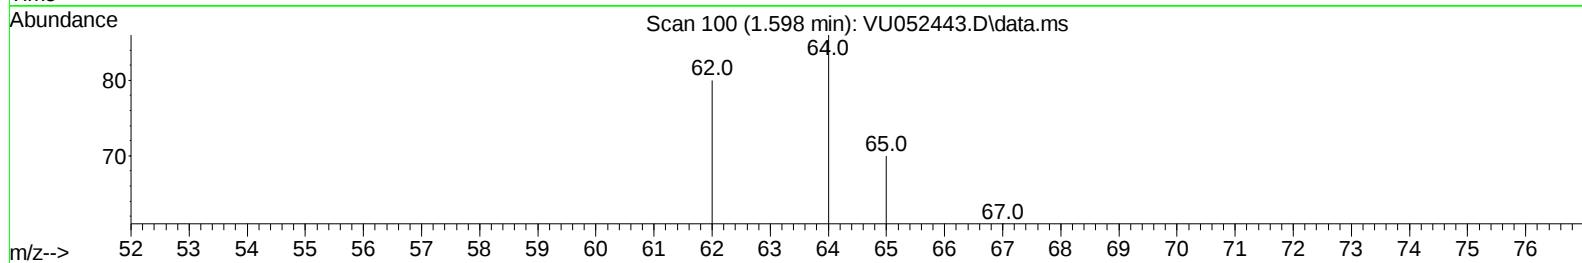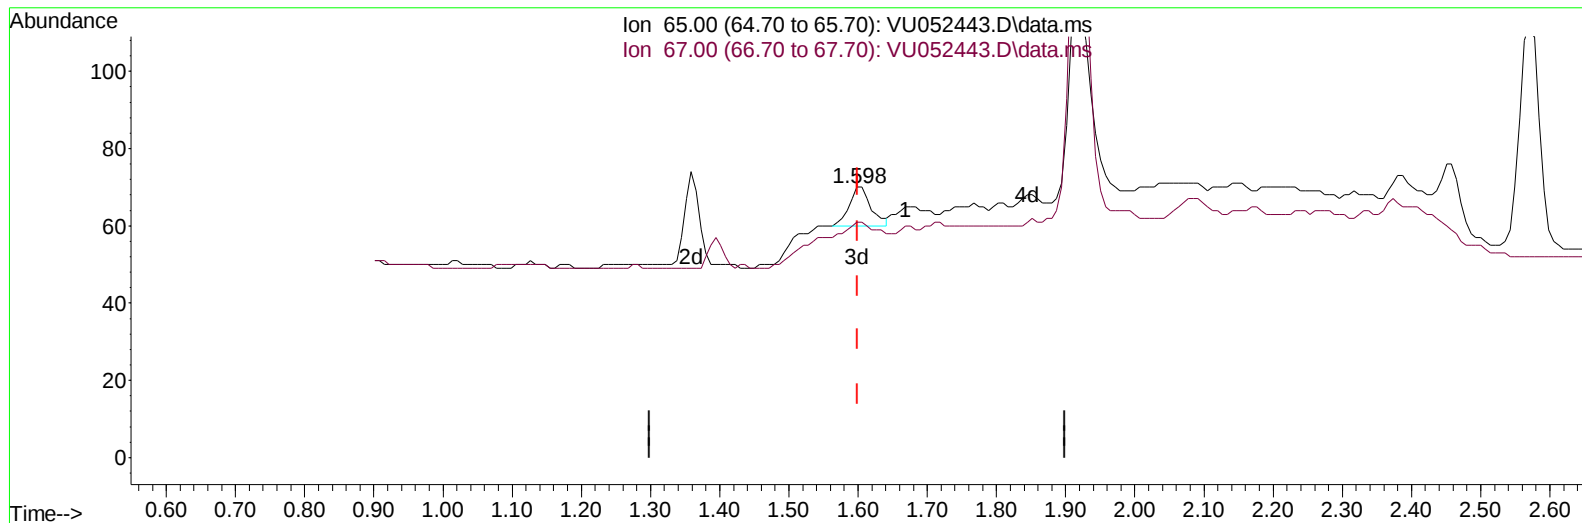

TIC: VU052443.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.598min (-0.001) 0.00 ug/L m

response 22

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	32.90	13.64#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052443.D
 Acq On : 16 Dec 2022 17:51
 Operator : JC/MD
 Sample : N6034-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 16 21:13:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	16845	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	15238	0.500	ug/L	0.01
11) 1,4-Dichlorobenzene-d4	11.741	152	7417	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	22m	0.001	ug/L	0.00
Spiked Amount	0.500	Range 40 - 130	Recovery	=	0.000%#	
4) 1,2-Dichloroethane-d4	5.661	65	8761	0.466	ug/L	0.00
Spiked Amount	0.500	Range 70 - 130	Recovery	=	94.000%	
7) 1,2-Dichloropropane-d6	6.639	67	9972	0.545	ug/L	0.00
Spiked Amount	0.500	Range 60 - 140	Recovery	=	108.000%	
8) Toluene-d8	7.845	98	407	0.015	ug/L	0.01
Spiked Amount	0.500	Range 70 - 130	Recovery	=	2.000%#	
10) 1,1,2,2-Tetrachloroeth...	10.679	84	10904	0.557	ug/L	0.00
Spiked Amount	0.500	Range 65 - 120	Recovery	=	112.000%	

Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052443.D
Acq On : 16 Dec 2022 17:51
Operator : JC/MD
Sample : N6034-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 16 21:13:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

