

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
 Data File : VU052426.D
 Acq On : 16 Dec 2022 11:04
 Operator : JC/MD
 Sample : N6034-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 16 21:11:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	17725	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	15874	0.500	ug/L	0.01
11) 1,4-Dichlorobenzene-d4	11.742	152	7804	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.599	65	10948	0.524	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	104.000%
4) 1,2-Dichloroethane-d4	5.661	65	9157	0.463	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
7) 1,2-Dichloropropane-d6	6.639	67	10623	0.557	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	112.000%
8) Toluene-d8	7.830	98	14514	0.505	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.679	84	10983	0.538	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.606	62	1053	0.047	ug/L #	1
6) Trichloroethene	6.489	95	12575	0.708	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121622\
Data File : VU052426.D
Acq On : 16 Dec 2022 11:04
Operator : JC/MD
Sample : N6034-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1





Quant Time: Dec 16 21:11:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

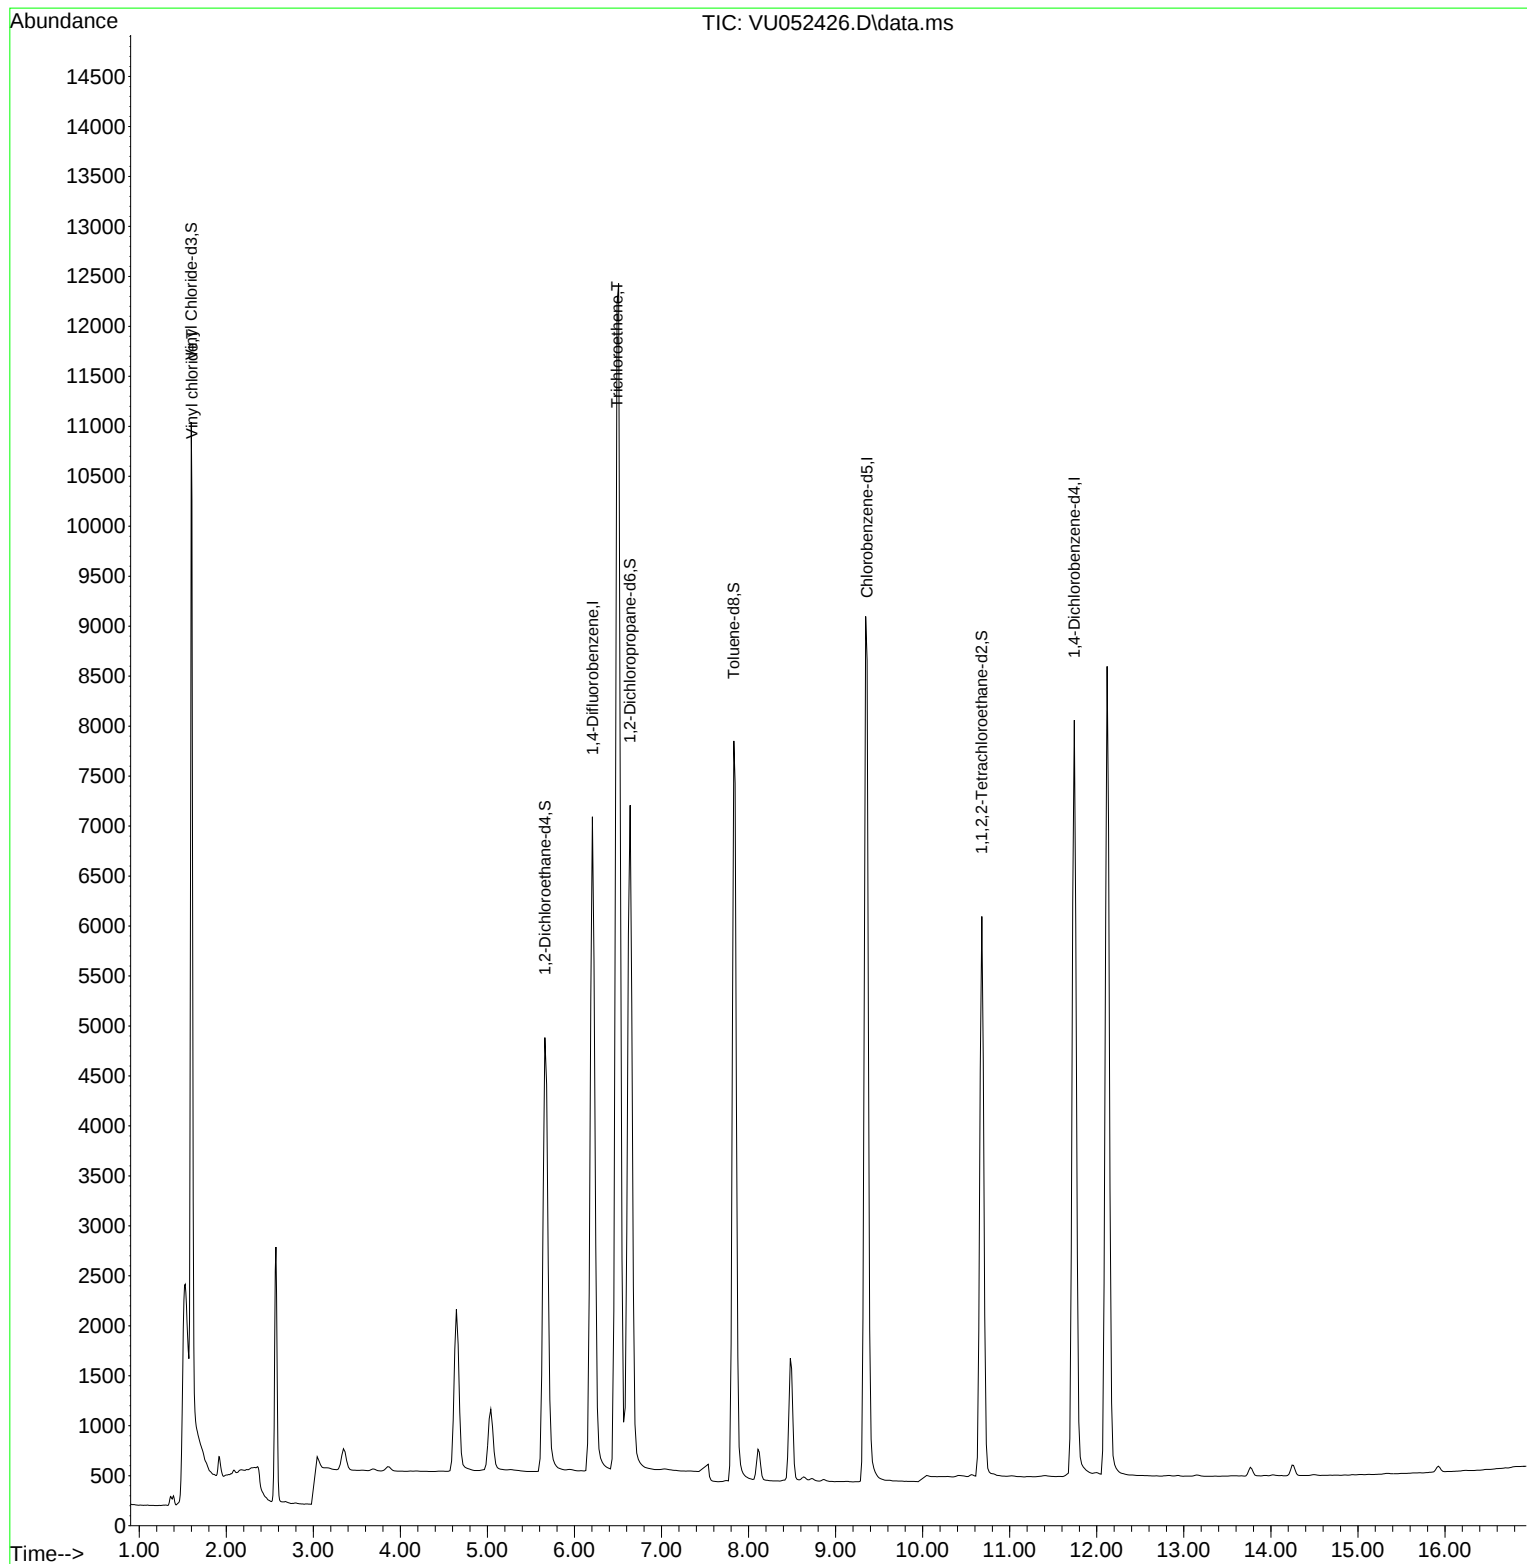

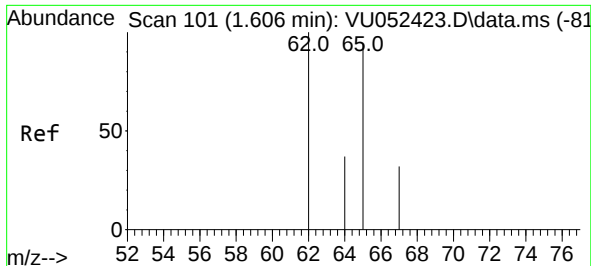

#3
 Vinyl chloride
 Concen: 0.047 ug/L
 RT: 1.606 min Scan# 101
 Delta R.T. 0.007 min
 Lab File: VU052426.D
 Acq: 16 Dec 2022 11:04

Tgt Ion: 62 Resp: 1053
 Ion Ratio Lower Upper
 62 100
 64 191.2 23.7 43.9#

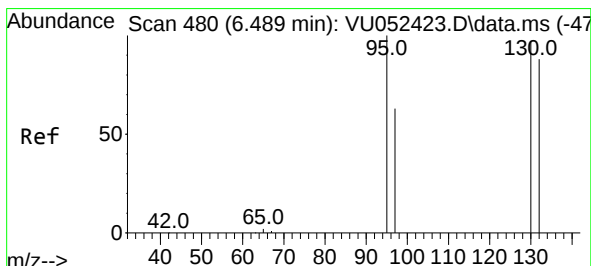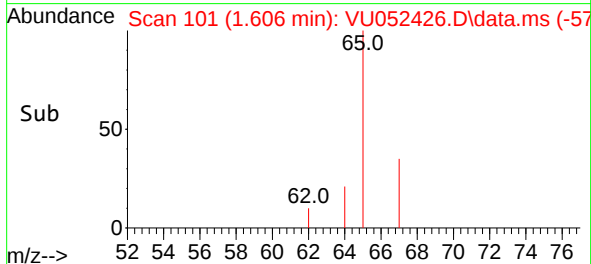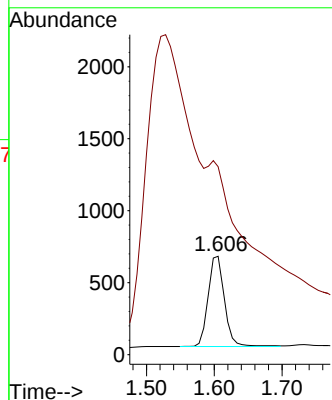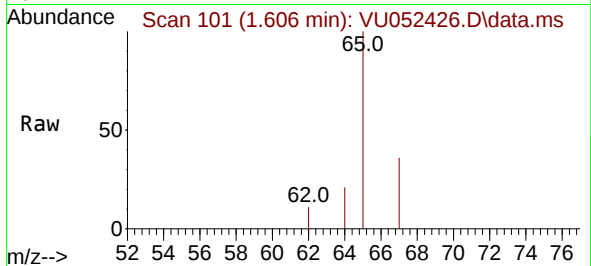

#6
 Trichloroethene
 Concen: 0.708 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052426.D
 Acq: 16 Dec 2022 11:04

Tgt Ion: 95 Resp: 12575
 Ion Ratio Lower Upper
 95 100
 97 63.4 43.3 80.3
 132 89.2 61.0 113.2
 130 96.0 66.7 123.9

