

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121623\
 Data File : VU056938.D
 Acq On : 16 Dec 2023 19:41
 Operator : MD/SY
 Sample : 05810-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C88

Quant Time: Dec 16 23:48:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 15 01:53:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	193439	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	204687	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	80363	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	66005	3.981	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.600%
7) Chloroethane-d5	1.907	69	54552	4.397	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%
11) 1,1-Dichloroethene-d2	2.560	65	29480	4.155	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.200%
20) 2-Butanone-d5	4.621	46	186870	57.068	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.140%
24) Chloroform-d	5.055	84	157850	5.027	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	5.698	65	79638	5.360	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.200%
32) Benzene-d6	5.721	84	287380	4.527	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	6.685	67	94183	4.740	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.800%
41) Toluene-d8	7.894	98	225198	3.969	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.400%
43) trans-1,3-Dichloroprop...	8.177	79	31763	4.122	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	8.631	63	139377	47.954	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.900%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	74027	5.149	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.000%
66) 1,2-Dichlorobenzene-d4	12.190	152	78314	4.957	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.200%
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.570	96	4246	0.270	ug/L	# 1
17) Methyl tert-butyl Ether	3.354	73	638297	18.330	ug/L	99
19) 1,1-Dichloroethane	3.859	63	218739	7.142	ug/L	98
22) cis-1,2-Dichloroethene	4.663	96	10160	0.587	ug/L	96
25) Chloroform	5.081	83	24266	0.756	ug/L	96
34) Trichloroethene	6.537	95	18299	0.927	ug/L	92
47) Tetrachloroethene	8.550	164	4961	0.359	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121623\
Data File : VU056938.D
Acq On : 16 Dec 2023 19:41
Operator : MD/SY
Sample : 05810-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C88

Quant Time: Dec 16 23:48:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 15 01:53:53 2023
Response via : Initial Calibration

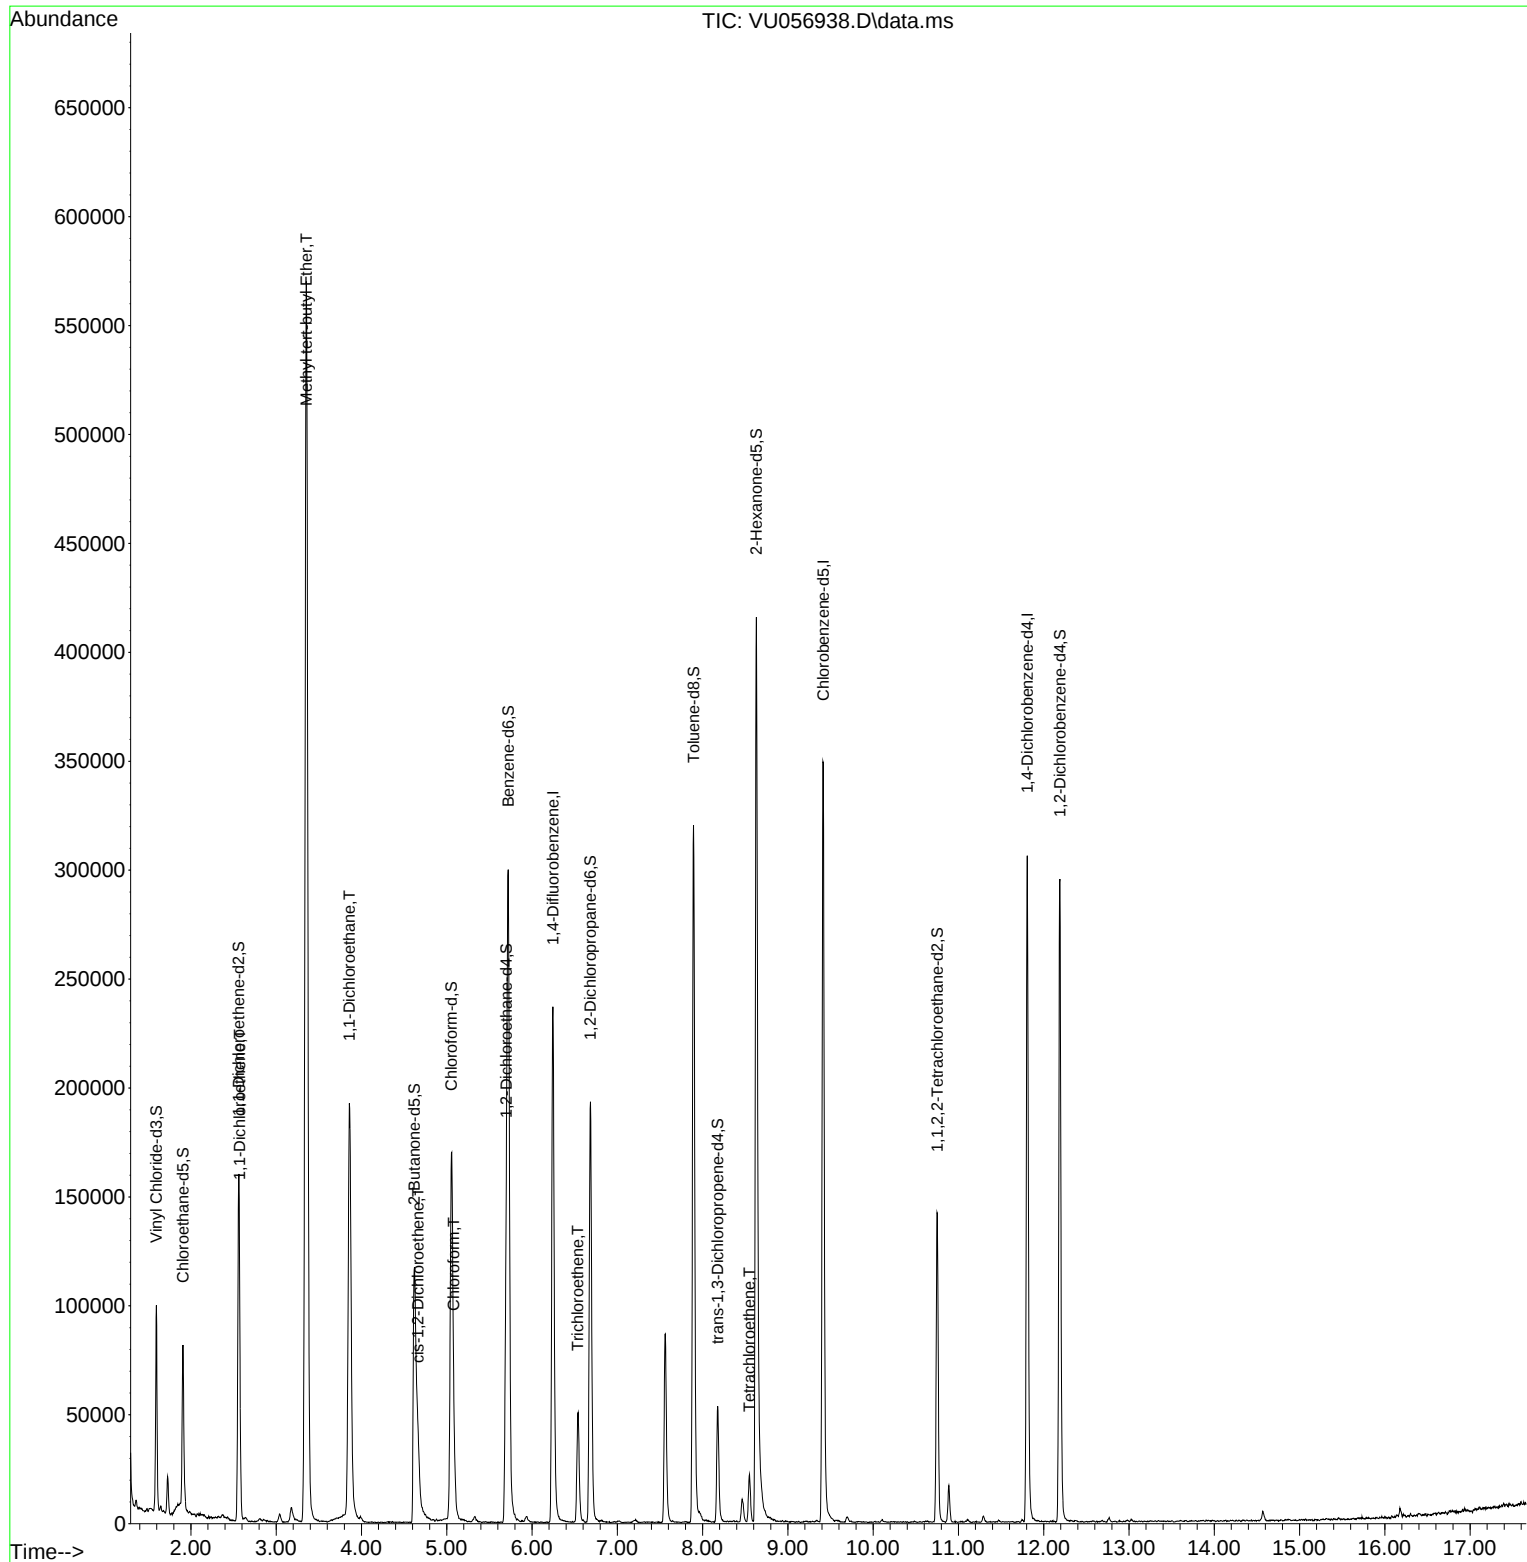

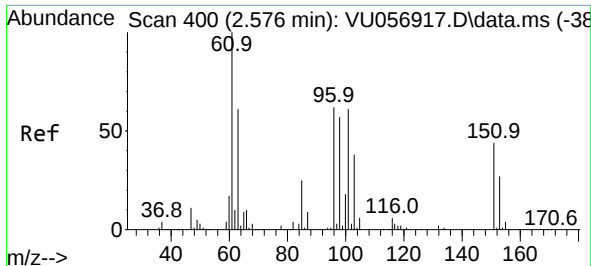

#12

1,1-Dichloroethene

Concen: 0.270 ug/L

RT: 2.570 min Scan# 398

Delta R.T. -0.007 min

Lab File: VU056938.D

Acq: 16 Dec 2023 19:41

Instrument :

MSVOA_U

ClientSampleId :

F7C88





Tgt Ion: 96 Resp: 4246

Ion Ratio Lower Upper

96 100

61 317.4 119.0 221.0#

63 1763.6 88.7 164.7#

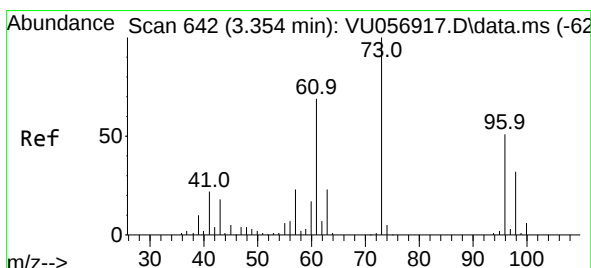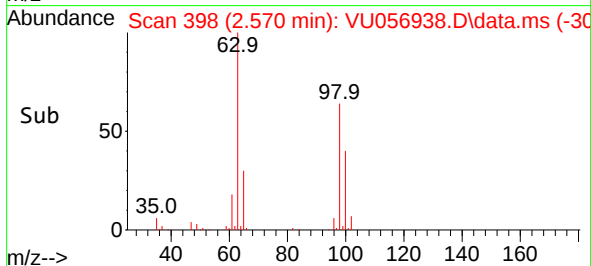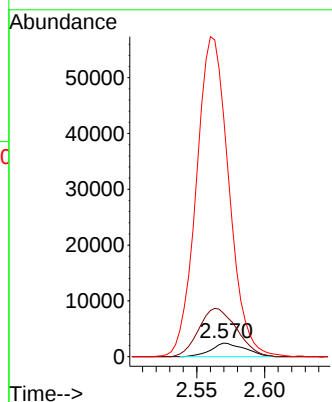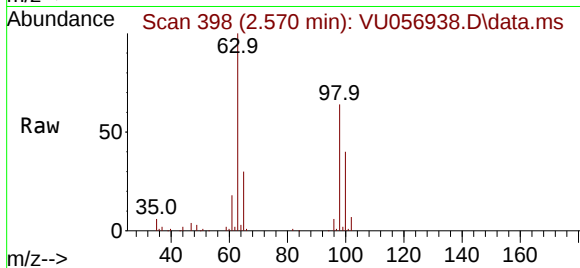

#17

Methyl tert-butyl Ether

Concen: 18.330 ug/L

RT: 3.354 min Scan# 642

Delta R.T. -0.000 min

Lab File: VU056938.D

Acq: 16 Dec 2023 19:41




Tgt Ion: 73 Resp: 638297


Ion Ratio Lower Upper

73 100

43 18.3 14.4 21.6

57 22.0 17.8 26.8

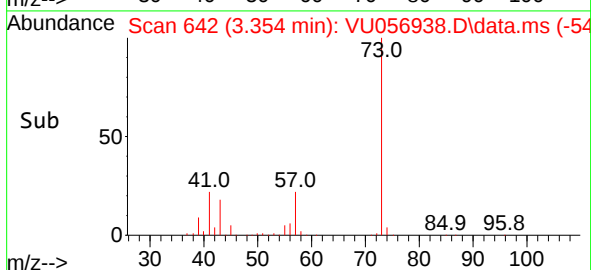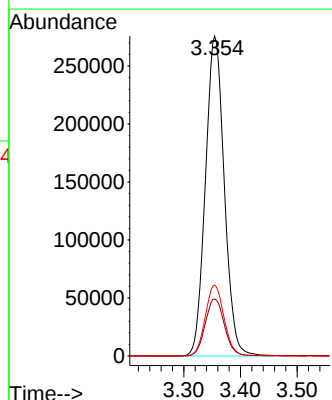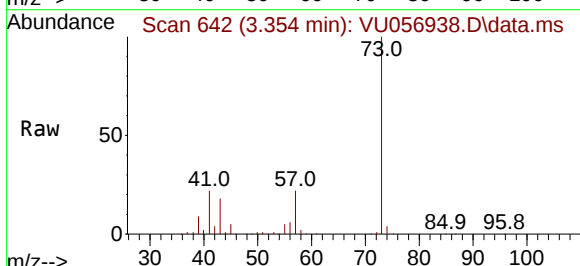

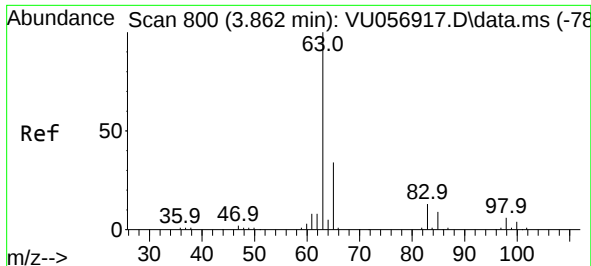

#19

1,1-Dichloroethane

Concen: 7.142 ug/L

RT: 3.859 min Scan# 799

Delta R.T. -0.003 min

Lab File: VU056938.D

Acq: 16 Dec 2023 19:41

Instrument :

MSVOA_U

ClientSampleId :

F7C88





Tgt Ion: 63 Resp: 218739

Ion Ratio Lower Upper

63 100

65 32.9 22.9 42.5

83 12.8 10.1 18.9

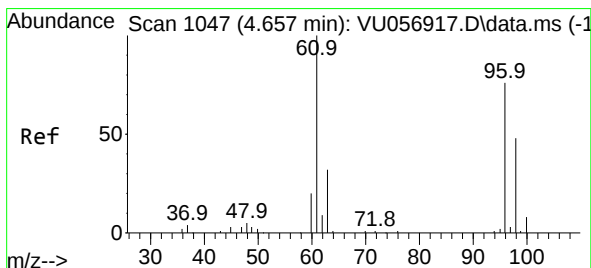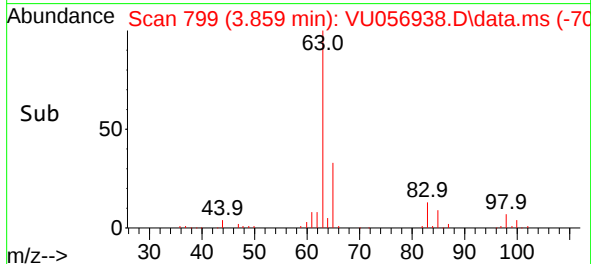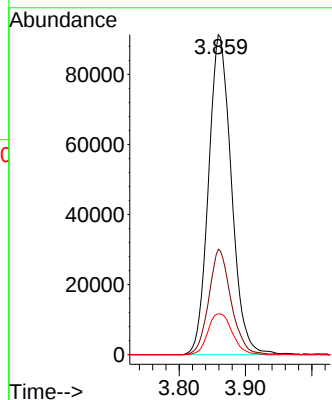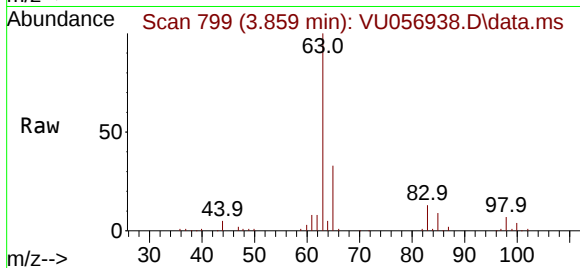

#22

cis-1,2-Dichloroethene

Concen: 0.587 ug/L

RT: 4.663 min Scan# 1049

Delta R.T. 0.003 min

Lab File: VU056938.D

Acq: 16 Dec 2023 19:41




Tgt Ion: 96 Resp: 10160


Ion Ratio Lower Upper

96 100

61 126.6 91.3 169.6

98 66.6 44.2 82.0


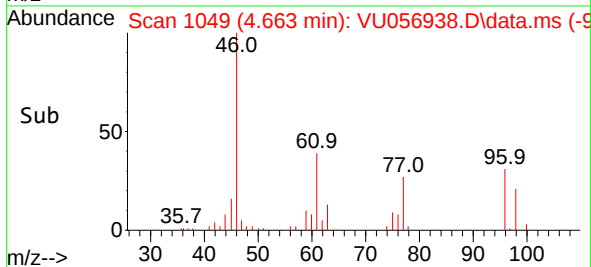
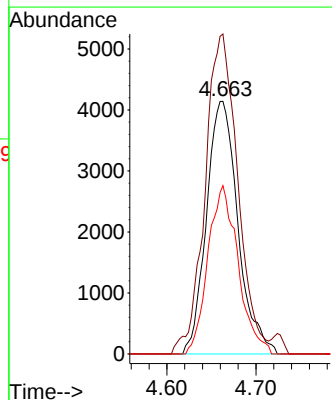
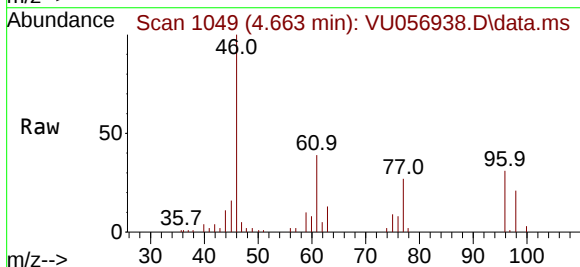


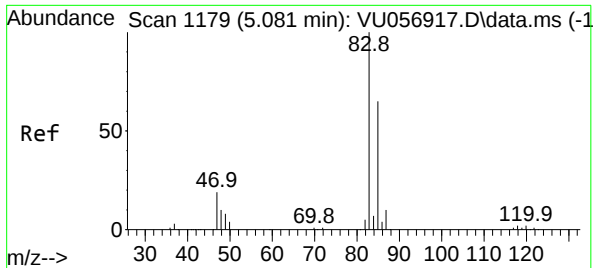

#25
Chloroform
Concen: 0.756 ug/L
RT: 5.081 min Scan# 1179
Delta R.T. -0.000 min
Lab File: VU056938.D
Acq: 16 Dec 2023 19:41




Instrument :
MSVOA_U
ClientSampleId :
F7C88


Tgt Ion: 83 Resp: 24266
Ion Ratio Lower Upper
83 100
85 68.9 45.8 85.0

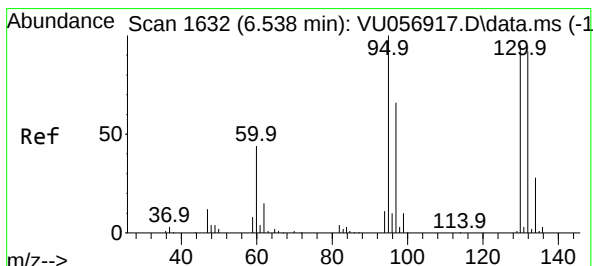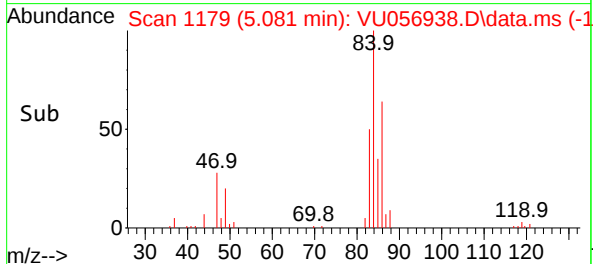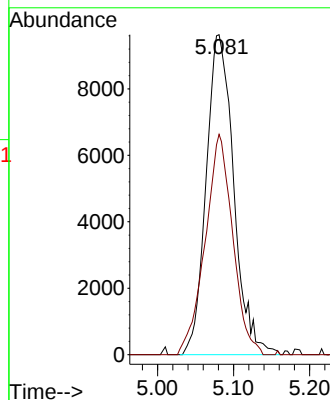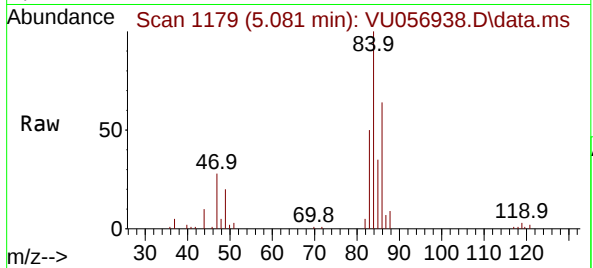

#34
Trichloroethene
Concen: 0.927 ug/L
RT: 6.537 min Scan# 1632
Delta R.T. -0.000 min
Lab File: VU056938.D
Acq: 16 Dec 2023 19:41


Tgt Ion: 95 Resp: 18299
Ion Ratio Lower Upper
95 100
97 63.8 46.1 85.5
132 79.7 63.6 118.0
130 86.8 66.4 123.4

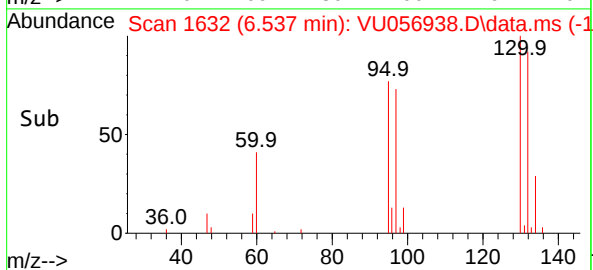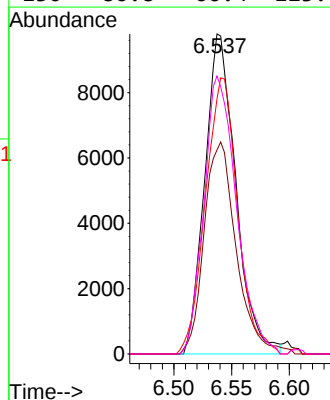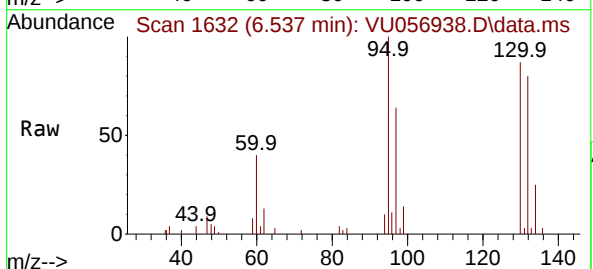

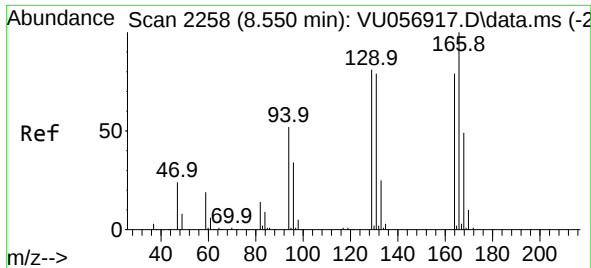

#47
 Tetrachloroethene
 Concen: 0.359 ug/L
 RT: 8.550 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VU056938.D
 Acq: 16 Dec 2023 19:41

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C88

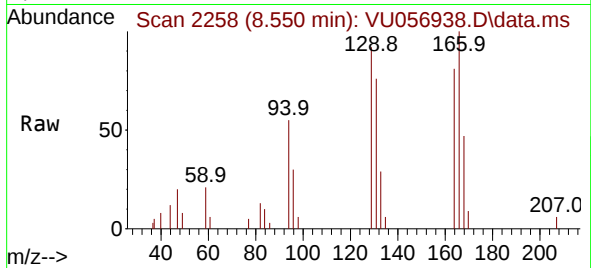

Tgt Ion:	164	Resp:	4961
Ion	Ratio	Lower	Upper
164	100		
129	112.5	73.4	136.4
131	93.6	71.5	132.9
166	122.9	92.7	172.1

