

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121623\
 Data File : VU056925.D
 Acq On : 16 Dec 2023 14:26
 Operator : MD/SY
 Sample : 05810-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C32

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.387	25	30	43	rVB	10303	12120	1.50%	0.174%
2	1.596	86	95	106	rVB	99188	114060	14.13%	1.638%
3	1.904	184	191	206	rVB	82104	113776	14.10%	1.634%
4	2.567	383	397	412	rBV3	223233	434759	53.88%	6.244%
5	3.181	576	588	600	rBV2	7019	18259	2.26%	0.262%
6	4.618	1023	1035	1080	rBV	114265	320131	39.67%	4.598%
7	5.055	1156	1171	1205	rVB	168199	386516	47.90%	5.551%
8	5.718	1358	1377	1404	rBV2	307517	806963	100.00%	11.589%
9	6.245	1526	1541	1568	rBV	242464	481000	59.61%	6.908%
10	6.685	1662	1678	1698	rBV	196980	389231	48.23%	5.590%
11	7.563	1939	1951	1971	rBV	87862	162412	20.13%	2.332%
12	7.894	2041	2054	2075	rBV	331292	595370	73.78%	8.550%
13	8.177	2130	2142	2162	rBV2	57023	98887	12.25%	1.420%
14	8.467	2218	2232	2244	rBV3	14999	28018	3.47%	0.402%
15	8.550	2246	2258	2272	rBV	141741	240501	29.80%	3.454%
16	8.631	2272	2283	2319	rBV	416174	803192	99.53%	11.535%
17	9.412	2514	2526	2548	rBV	351813	614442	76.14%	8.824%
18	10.753	2931	2943	2960	rBV	141471	237866	29.48%	3.416%
19	10.888	2974	2985	2999	rVB2	26983	43893	5.44%	0.630%
20	11.807	3259	3271	3294	rBV	318655	528934	65.55%	7.596%
21	12.187	3377	3389	3412	rBV	312264	532757	66.02%	7.651%




Sum of corrected areas: 6963087

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121623\
Data File : VU056925.D
Acq On : 16 Dec 2023 14:26
Operator : MD/SY
Sample : 05810-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

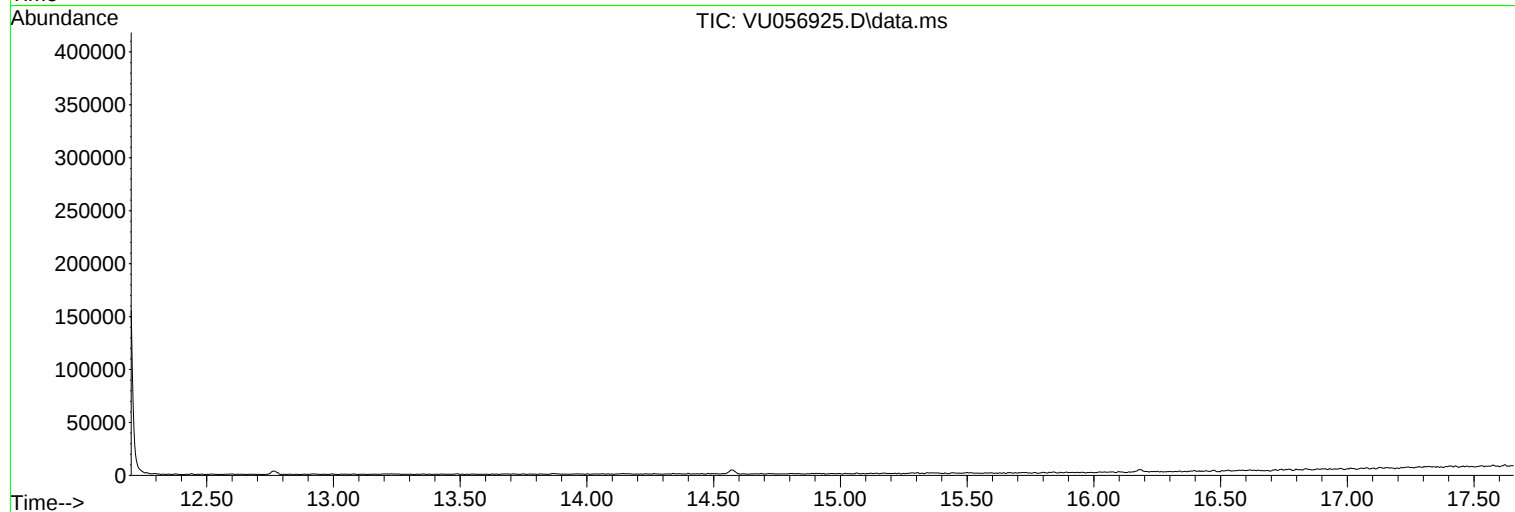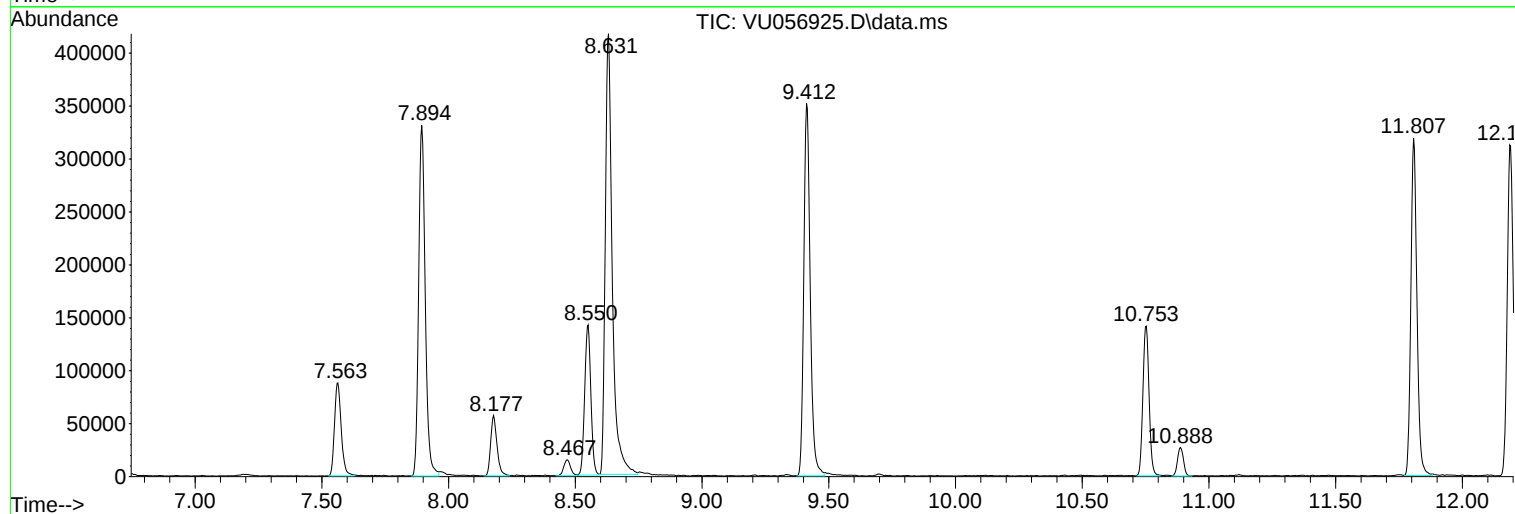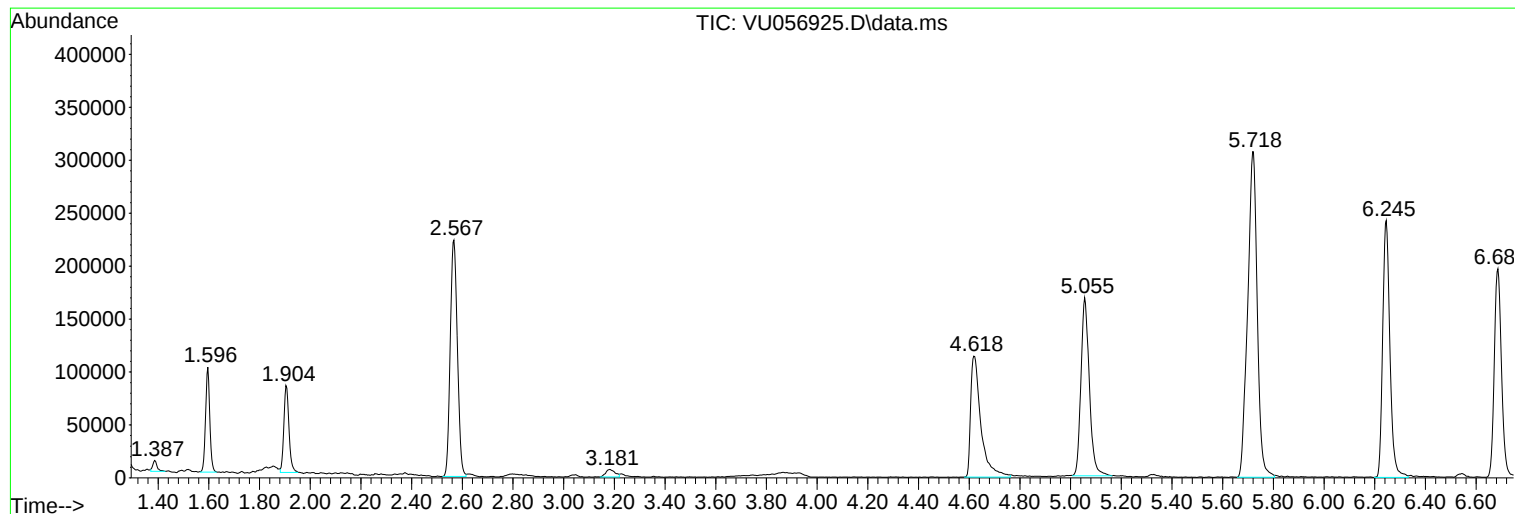

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121623\
Data File : VU056925.D
Acq On : 16 Dec 2023 14:26
Operator : MD/SY
Sample : 05810-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121623\
Data File : VU056925.D
Acq On : 16 Dec 2023 14:26
Operator : MD/SY
Sample : 05810-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc