
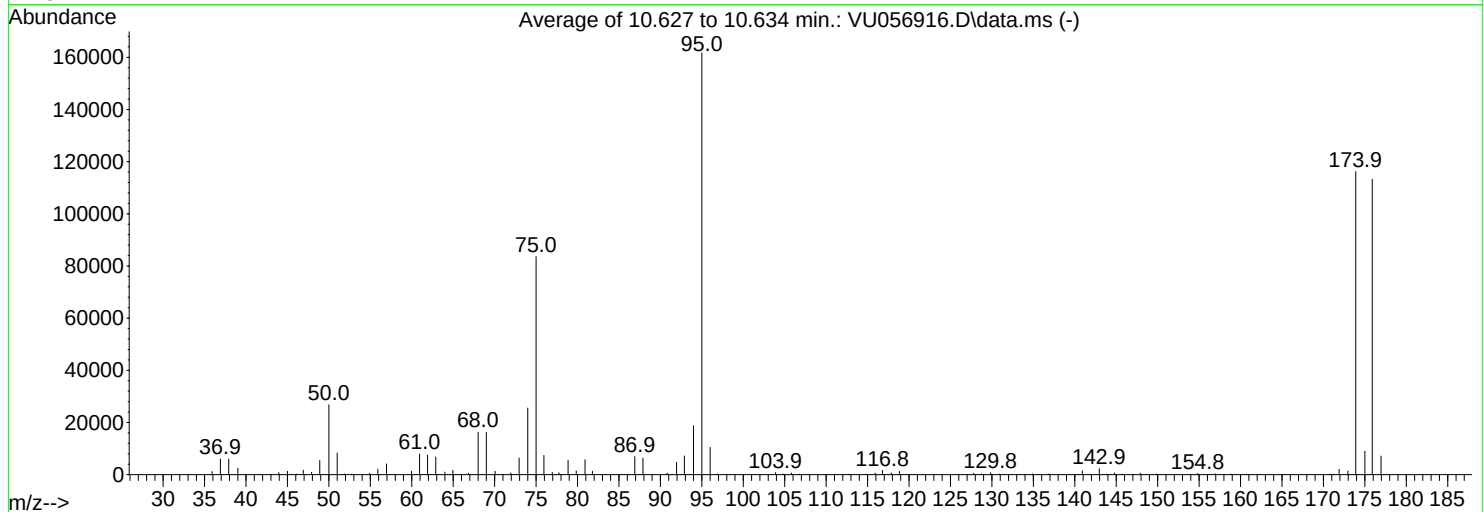


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121623\
Data File : VU056916.D
Acq On : 16 Dec 2023 09:39
Operator : MD/SY
Sample : BFB094
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB094

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 19 02:36:03 2023

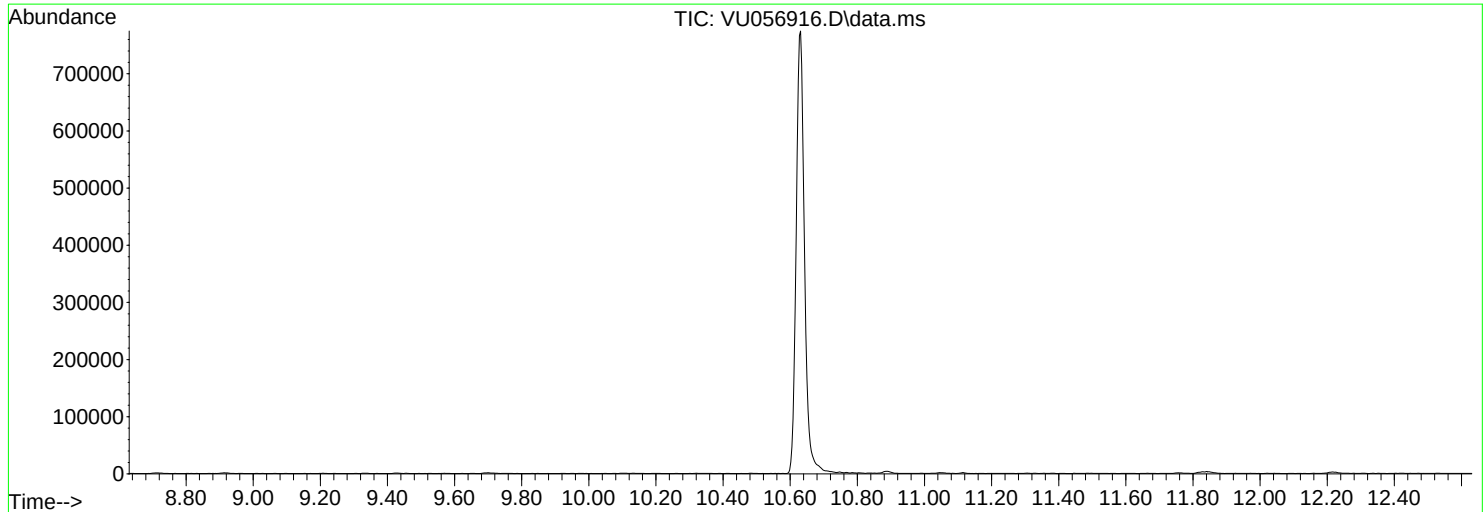

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	26805	PASS
75	95	30	80	51.7	83643	PASS
95	95	100	100	100.0	161707	PASS
96	95	5	9	6.4	10413	PASS
173	174	0.00	2	1.2	1419	PASS
174	95	50	120	71.8	116157	PASS
175	174	5	9	7.7	8928	PASS
176	174	95	101	97.5	113227	PASS
177	176	5	9	6.3	7140	PASS

m/z	Abundance
39.60	170.0
40.10	204.0
43.80	371.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
35.90	1169.0
36.90	6354.0
37.90	5948.0
39.00	2387.0
40.00	344.0
41.90	194.0
43.00	131.0
44.00	1205.0
45.00	1261.0
46.10	354.0
46.90	1746.0
47.90	879.0
48.90	5675.0
50.00	28432.0
51.00	8545.0
51.90	338.0
52.80	243.0
54.90	583.0
55.90	2190.0
57.00	4280.0
57.80	160.0
60.00	1475.0
60.90	7648.0
61.90	7817.0
62.90	7099.0
63.90	958.0
65.00	1746.0
65.90	164.0
66.80	604.0
68.00	16840.0
69.00	16824.0
70.00	1326.0
72.00	672.0
72.90	6951.0
74.00	26304.0
75.00	85904.0
76.00	7605.0
77.00	908.0
77.70	701.0
78.90	5685.0
79.80	1315.0
80.90	5755.0
81.80	1377.0
83.00	101.0
86.10	461.0
86.90	7389.0
87.90	6781.0
90.80	520.0
91.90	4746.0
92.90	7492.0
94.00	19048.0
95.00	165312.0
96.00	10679.0
96.90	296.0
103.90	725.0
104.80	255.0
105.80	626.0
106.80	176.0
107.80	103.0
109.90	114.0
111.00	230.0
112.80	151.0
114.90	221.0
115.90	616.0
116.80	1690.0
117.90	652.0
118.90	1355.0
127.80	464.0
128.80	297.0
129.80	786.0
130.90	216.0
134.80	328.0
136.80	266.0
139.00	121.0
140.90	1480.0
141.80	157.0
142.90	2270.0
143.90	111.0
144.80	646.0
145.70	307.0
147.00	142.0
147.90	533.0
149.80	164.0
154.80	391.0
156.90	323.0
158.90	173.0
160.70	244.0
170.80	213.0
171.20	182.0
171.90	1792.0
172.90	1522.0
173.90	116240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

175.00	9391.0
175.90	112952.0
177.00	7063.0
177.90	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
35.90	1253.0
36.90	6163.0
37.90	6189.0
39.00	2537.0
39.90	339.0
41.90	134.0
44.00	1231.0
45.00	1448.0
46.00	236.0
46.90	1801.0
47.90	940.0
48.90	5547.0
50.00	27512.0
51.00	8484.0
51.90	330.0
52.80	217.0
54.90	479.0
55.90	2184.0
56.90	4278.0
57.80	144.0
58.20	117.0
60.00	1368.0
60.90	8216.0
61.90	7631.0
62.90	7099.0
64.00	944.0
64.90	1754.0
65.90	189.0
66.90	597.0
68.00	16808.0
69.00	16728.0
70.00	1404.0
71.00	150.0
71.90	720.0
72.90	6462.0
74.00	26312.0
75.00	85976.0
75.90	7690.0
76.90	869.0
77.70	779.0
78.90	5706.0
79.90	1402.0
80.90	5886.0
81.80	1377.0
82.90	110.0
86.90	7102.0
87.90	6584.0
90.80	634.0
92.00	4900.0
92.90	7405.0
94.00	19512.0
95.00	165888.0
96.00	10721.0
96.90	321.0
103.90	836.0
104.80	227.0
105.80	656.0
106.80	165.0
107.90	132.0
109.90	159.0
111.00	165.0
112.70	154.0
114.80	242.0
115.90	559.0
116.80	1664.0
117.90	596.0
118.80	1209.0
127.80	616.0
128.70	288.0
129.80	801.0
130.90	273.0
133.90	105.0
134.90	316.0
136.90	316.0
139.00	108.0
140.90	1503.0
141.70	143.0
143.00	2301.0
143.90	174.0
144.80	715.0
145.70	267.0
147.00	169.0
147.90	592.0
149.80	261.0
154.80	426.0
157.00	348.0
158.80	250.0
160.70	239.0
170.80	227.0
171.90	2121.0
173.00	1439.0
173.90	119192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

175.00	9253.0
175.90	117200.0
176.90	7361.0
177.90	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
35.90	1076.0
36.90	5479.0
37.90	5813.0
39.00	2487.0
39.80	335.0
44.00	1140.0
45.00	1252.0
46.00	124.0
46.90	1553.0
47.90	828.0
48.90	5051.0
50.00	24472.0
51.00	7776.0
51.90	321.0
52.70	159.0
54.90	390.0
55.90	1971.0
57.00	3842.0
57.90	125.0
58.10	124.0
59.90	1186.0
61.00	7812.0
61.90	6948.0
62.90	6141.0
64.10	1002.0
64.90	1532.0
65.90	185.0
66.90	482.0
68.00	15128.0
69.00	15024.0
70.10	1216.0
71.00	156.0
71.90	738.0
73.00	5643.0
74.00	23944.0
75.00	79048.0
76.00	6876.0
76.90	848.0
77.80	667.0
78.80	5270.0
79.90	1456.0
80.90	5436.0
81.80	1323.0
82.90	108.0
86.90	6308.0
87.90	5604.0
90.80	695.0
91.90	4556.0
92.90	6708.0
94.00	17720.0
95.00	153920.0
96.00	9838.0
96.90	259.0
103.90	803.0
104.80	234.0
105.80	658.0
106.80	142.0
107.90	144.0
109.90	150.0
111.00	134.0
112.70	119.0
114.80	208.0
115.90	492.0
116.80	1358.0
117.80	540.0
118.80	1137.0
127.80	630.0
128.70	298.0
129.90	708.0
130.90	301.0
133.90	100.0
135.00	283.0
136.90	324.0
140.90	1477.0
141.70	169.0
142.90	2208.0
143.80	221.0
144.80	670.0
145.70	208.0
146.90	134.0
147.90	518.0
149.90	308.0
154.90	425.0
156.90	364.0
158.80	277.0
160.80	174.0
170.80	258.0
171.90	2235.0
173.00	1296.0
173.90	113040.0
175.00	8140.0
175.90	109528.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

176.906995.0

177.90121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094