

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU121718\
 Data File : VU028750.D
 Acq On : 18 Dec 2018 03:59
 Operator : MD/SY
 Sample : J6413-02DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-2RDL

Quant Time: Dec 18 08:33:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 07 00:39:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	89486	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	158493	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	140243	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	55887	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	70560	51.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.34%	
35) Dibromofluoromethane	4.88	113	53796	53.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.88%	
50) Toluene-d8	7.57	98	200177	50.73	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.46%	
62) 4-Bromofluorobenzene	10.30	95	66282	44.95	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.90%	
Target Compounds						
11) Tert butyl alcohol	2.82	59	54720	179.850	ug/l	99
19) Methyl tert-butyl Ether	3.00	73	39348	10.418	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU121718\
Data File : VU028750.D
Acq On : 18 Dec 2018 03:59
Operator : MD/SY
Sample : J6413-02DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-2RDL

Quant Time: Dec 18 08:33:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 07 00:39:42 2018
Response via : Initial Calibration

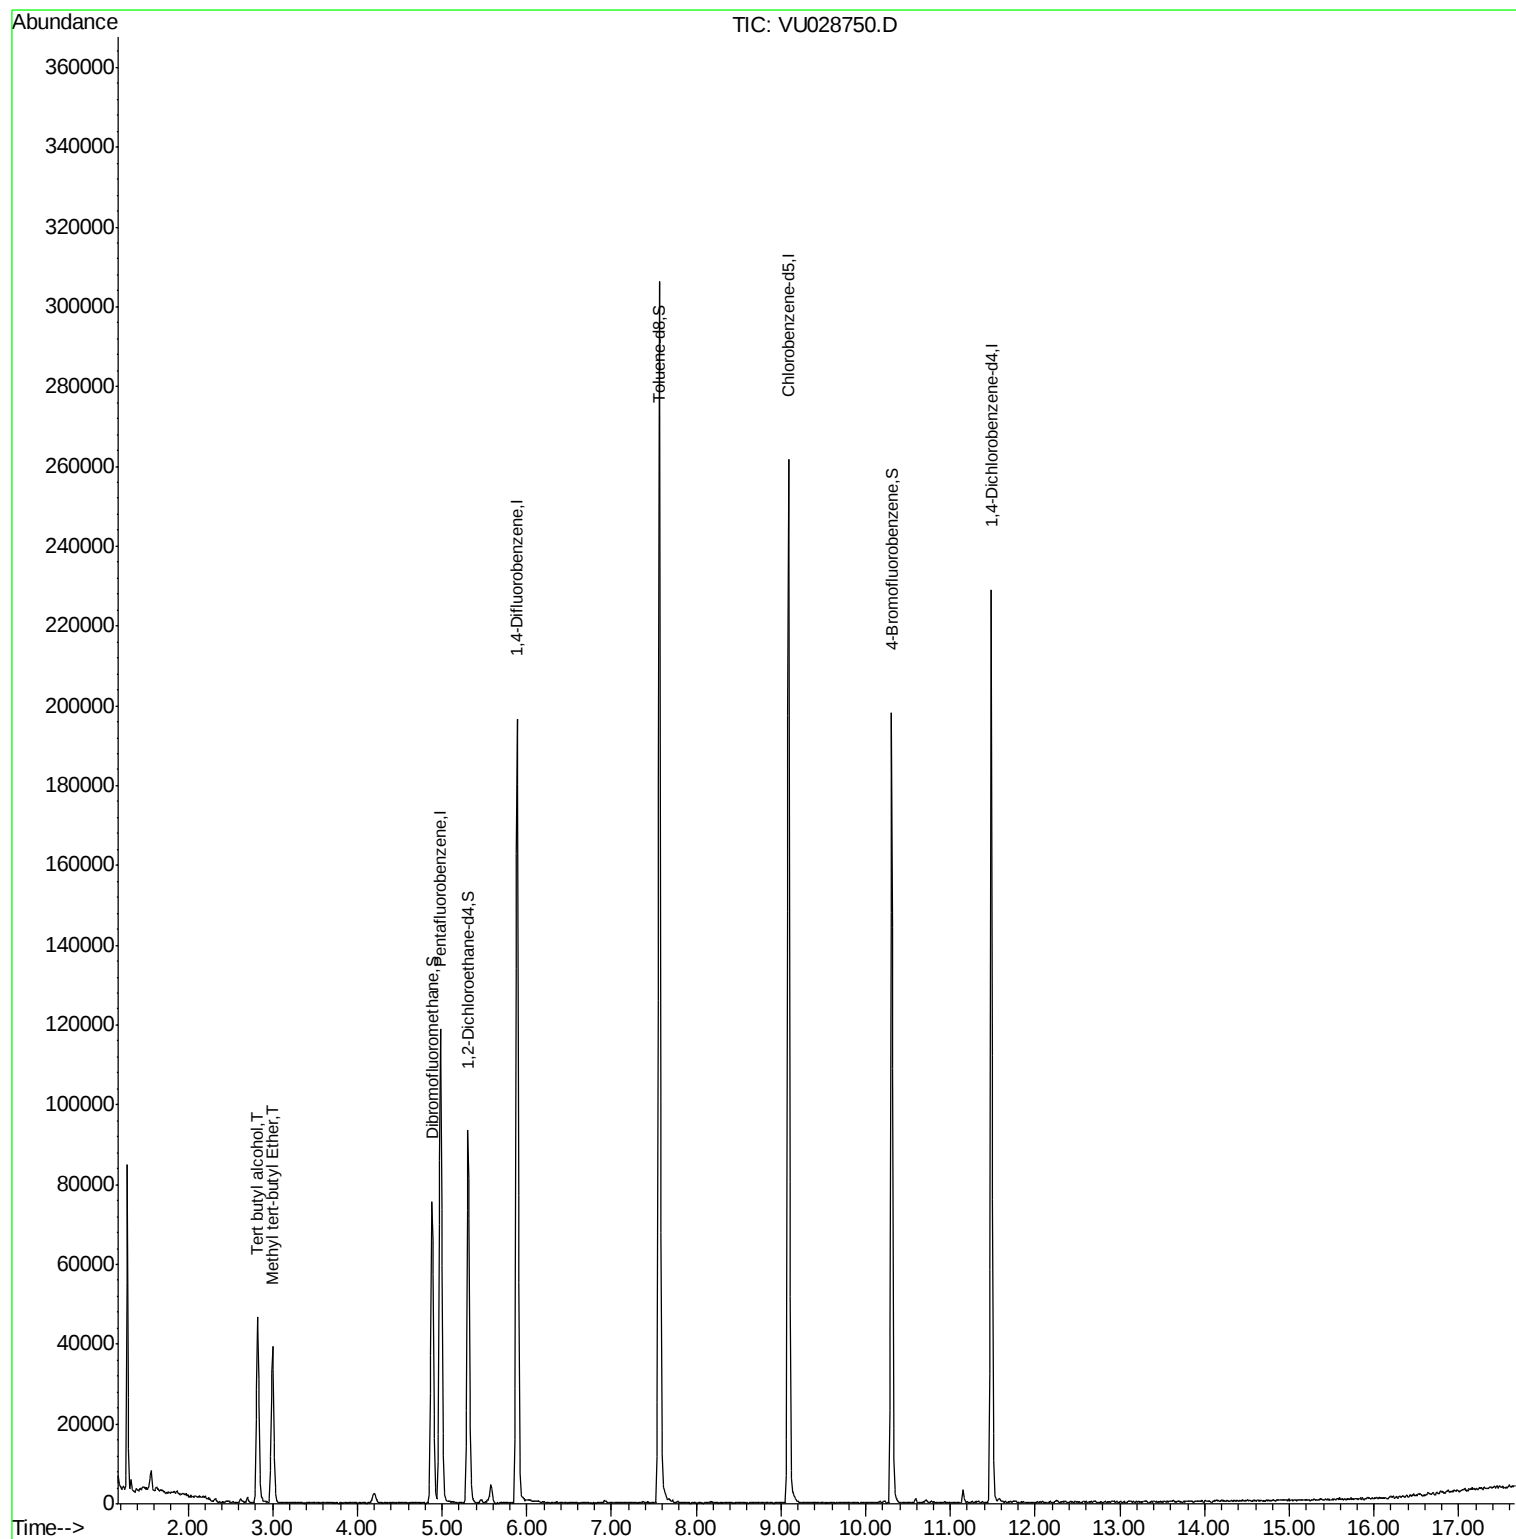

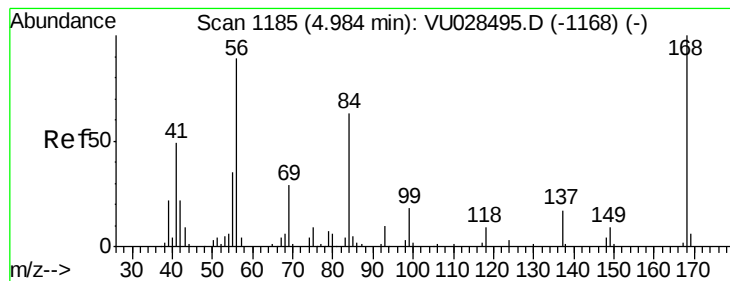

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1185

Delta R.T. -0.00 min

Lab File: VU028750.D

Acq: 18 Dec 2018 03:59

Instrument :

MSVOA_U

ClientSampleId :


MW-2RDL

Tgt Ion:168 Resp: 89486

Ion Ratio Lower Upper

168 100

99 59.8 46.6 69.8

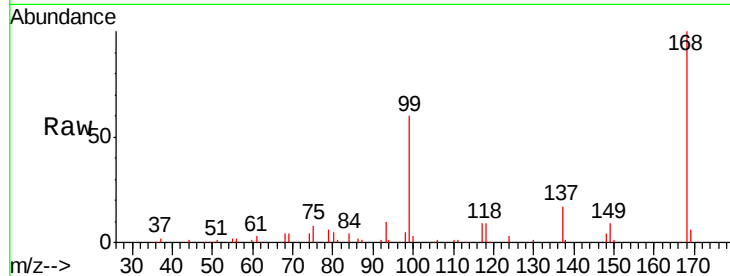

Abundance Ion 167.90 (167.60 to 168.60): VU028495.D (-1168) (-)

Ion 98.90 (98.60 to 99.60): VU028495.D (-1168) (-)

4.98

40000

30000



20000

10000

0

4.90 4.95 5.00 5.05 5.10

Time-->

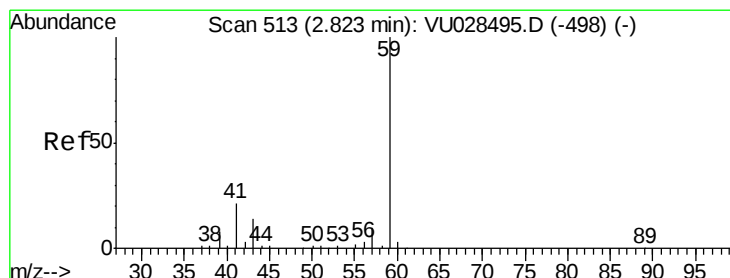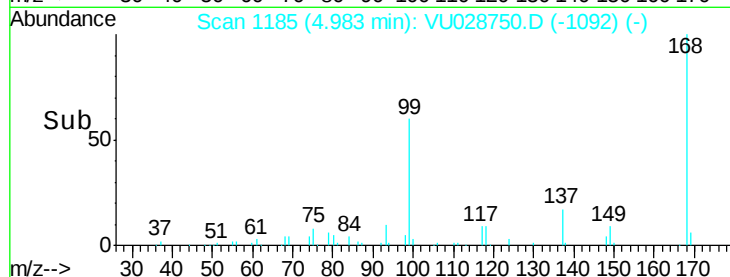

#11

Tert butyl alcohol

Concen: 179.850 ug/l

RT: 2.82 min Scan# 513

Delta R.T. -0.00 min

Lab File: VU028750.D


Acq: 18 Dec 2018 03:59

Tgt Ion: 59 Resp: 54720

Ion Ratio Lower Upper

59 100

57 9.5 8.0 12.0

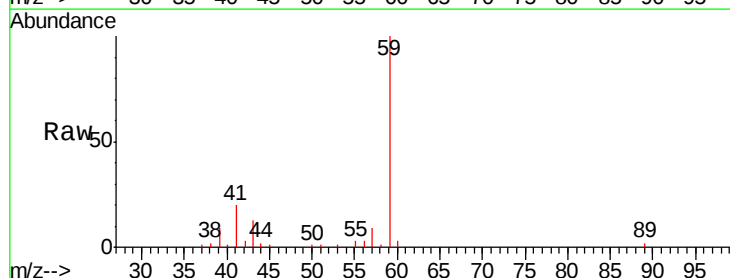

Abundance Ion 59.00 (58.70 to 59.70): VU028495.D (-498) (-)

Ion 57.00 (56.70 to 57.70): VU028495.D (-498) (-)

2.82

30000

25000

20000

15000


10000


5000

0

2.75 2.80 2.85 2.90

Time-->




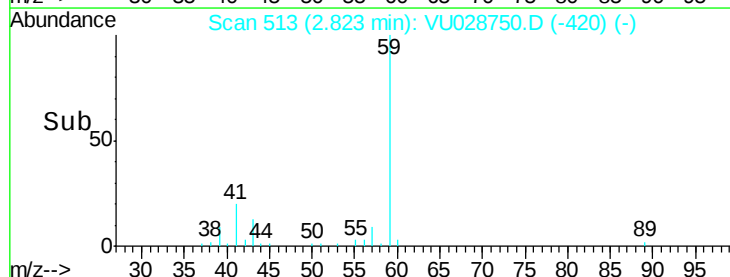


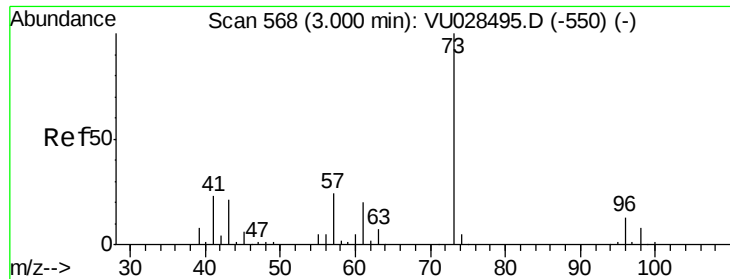

#19
Methyl tert-butyl Ether
Concen: 10.418 ug/l
RT: 3.00 min Scan# 568
Delta R.T. -0.00 min
Lab File: VU028750.D
Acq: 18 Dec 2018 03:59




Instrument :
MSVOA_U
ClientSampleId :
MW-2RDL


Tgt Ion: 73 Resp: 39348
Ion Ratio Lower Upper
73 100
57 24.1 19.4 29.2

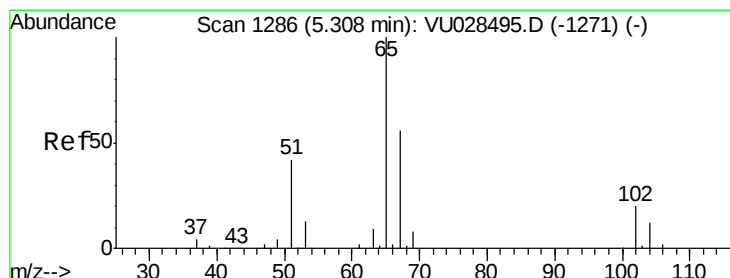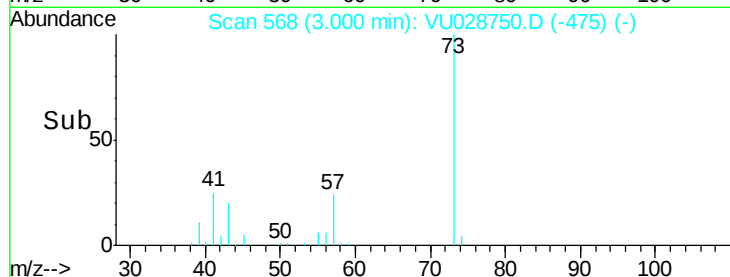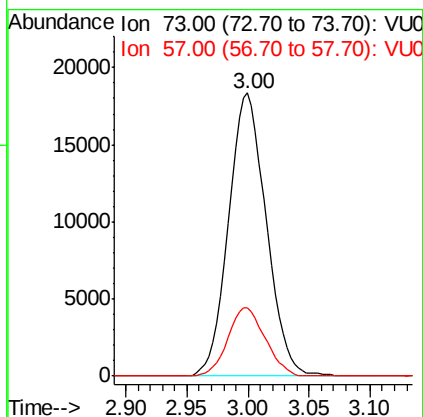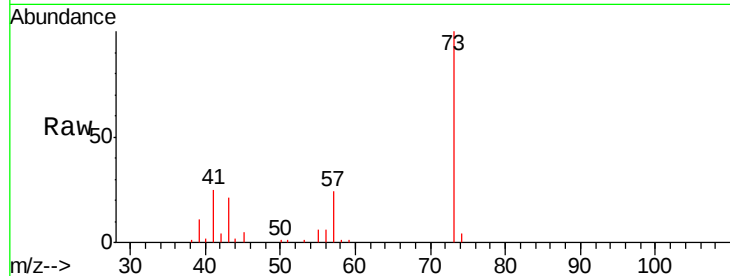

#33
1,2-Dichloroethane-d4
Concen: 51.669 ug/l
RT: 5.31 min Scan# 1286
Delta R.T. -0.00 min
Lab File: VU028750.D
Acq: 18 Dec 2018 03:59

Tgt Ion: 65 Resp: 70560
Ion Ratio Lower Upper
65 100
67 55.3 0.0 110.6

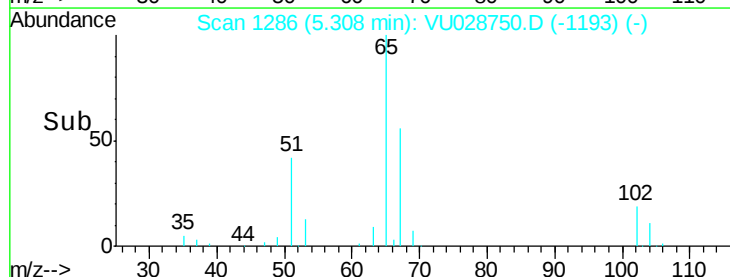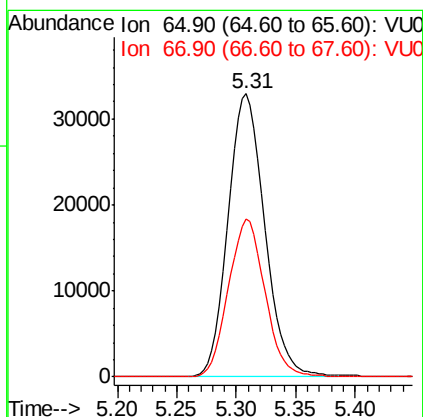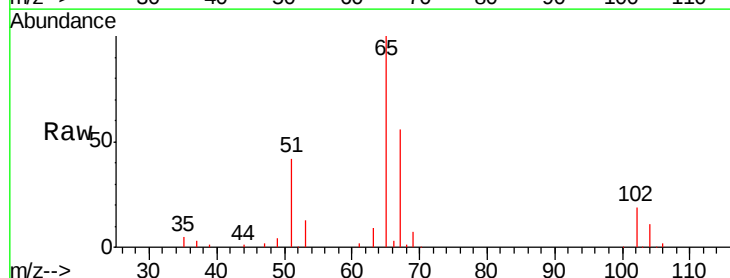


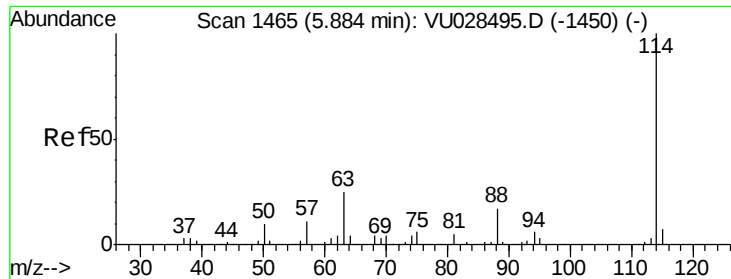




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.88 min Scan# 1465
 Delta R.T. -0.00 min
 Lab File: VU028750.D
 Acq: 18 Dec 2018 03:59

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-2RDL

Tgt Ion:114 Resp: 158493
 Ion Ratio Lower Upper
 114 100
 63 24.6 0.0 49.2
 88 17.0 0.0 33.4

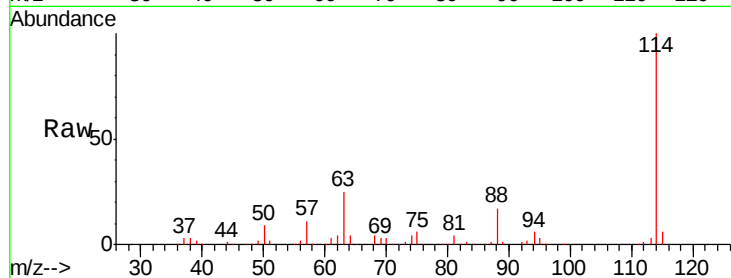


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VU0
 Ion 87.90 (87.60 to 88.60): VU0

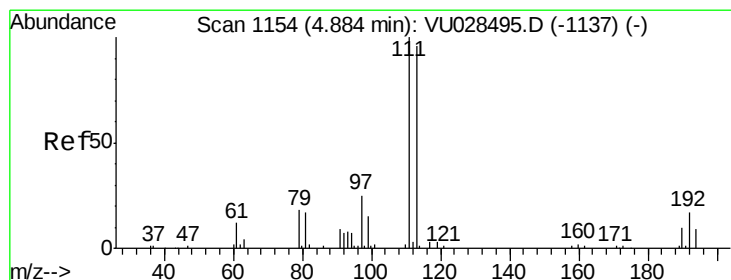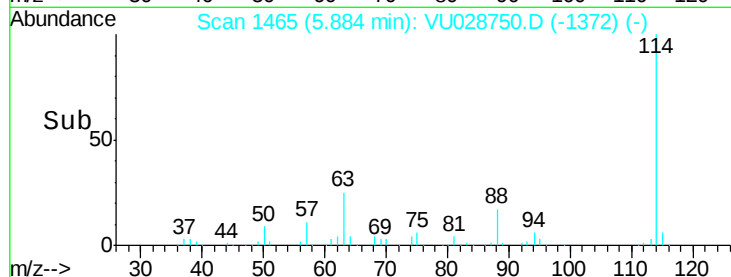
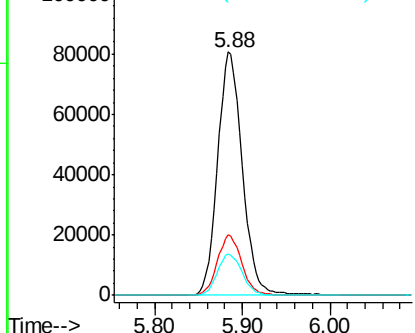



#35
 Dibromofluoromethane
 Concen: 53.936 ug/l
 RT: 4.88 min Scan# 1153
 Delta R.T. -0.00 min
 Lab File: VU028750.D
 Acq: 18 Dec 2018 03:59

Tgt Ion:113 Resp: 53796
 Ion Ratio Lower Upper
 113 100
 111 102.9 83.4 125.0
 192 19.0 14.8 22.2

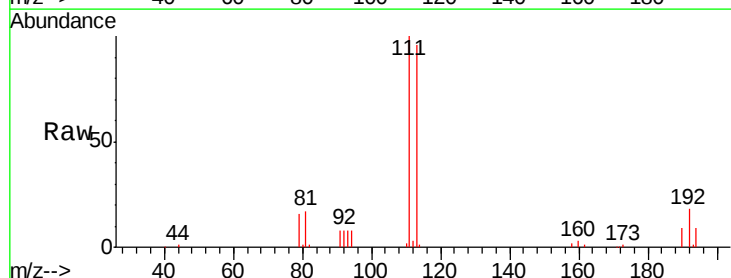

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

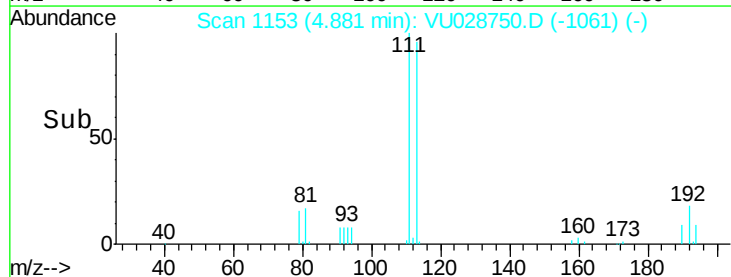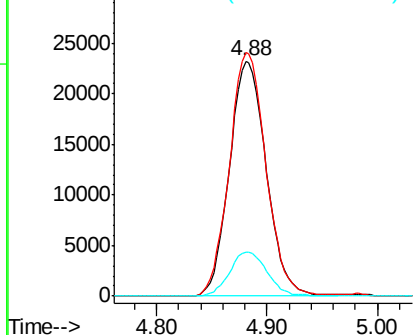

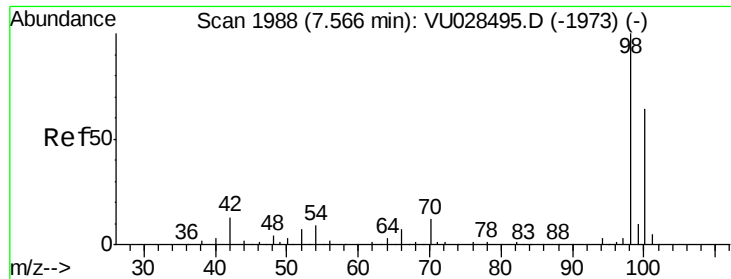

#50

Toluene-d8

Concen: 50.735 ug/l

RT: 7.57 min Scan# 1988

Delta R.T. -0.00 min

Lab File: VU028750.D

Acq: 18 Dec 2018 03:59

Instrument :

MSVOA_U

ClientSampleId :


MW-2RDL

Tgt Ion: 98 Resp: 200177

Ion Ratio Lower Upper

98 100

100 64.0 51.0 76.6

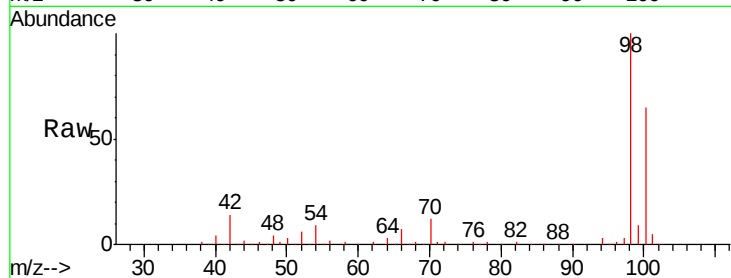

Abundance Ion 98.00 (97.70 to 98.70): VU028495.D (-1973) (-)

Ion 100.00 (99.70 to 100.70): VU028495.D (-1973) (-)



7.57

100000

50000

0

Time-->

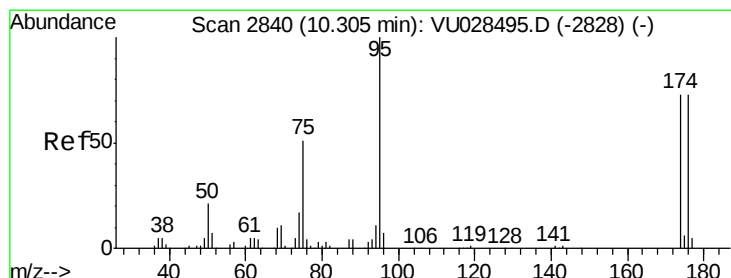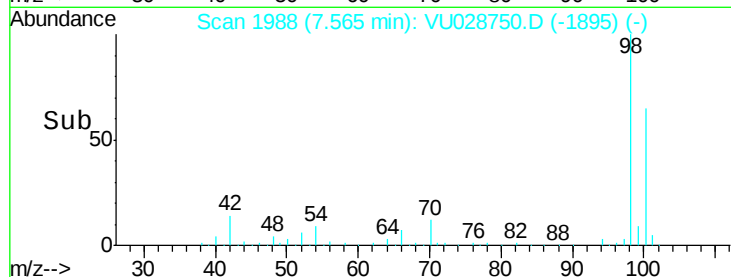

#62

4-Bromofluorobenzene

Concen: 44.946 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.00 min

Lab File: VU028750.D

Acq: 18 Dec 2018 03:59


Tgt Ion: 95 Resp: 66282

Ion Ratio Lower Upper

95 100

174 75.5 0.0 150.4

176 73.5 0.0 145.2

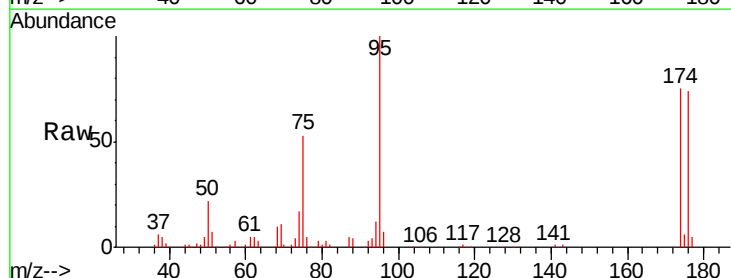

Abundance Ion 94.90 (94.60 to 95.60): VU028495.D (-2828) (-)

Ion 173.80 (173.50 to 174.50): VU028495.D (-2828) (-)

Ion 175.80 (175.50 to 176.50): VU028495.D (-2828) (-)

10.30

50000

40000


30000


20000

10000

0

Time-->

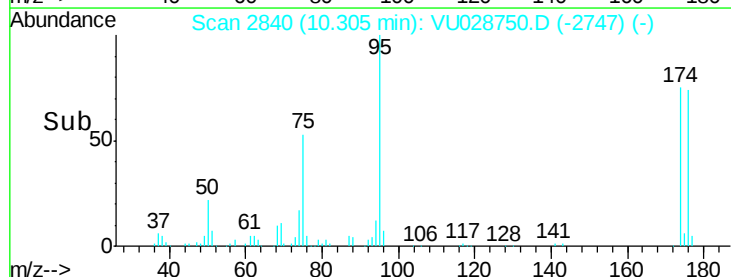


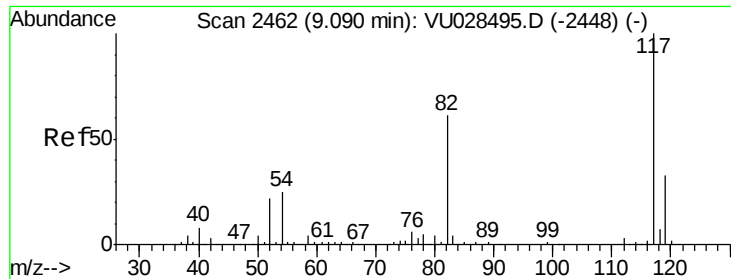




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2462
Delta R.T. -0.00 min
Lab File: VU028750.D
Acq: 18 Dec 2018 03:59

Instrument :
MSVOA_U
ClientSampleId :
MW-2RDL

Tgt Ion:117 Resp: 140243
Ion Ratio Lower Upper
117 100
82 60.5 48.9 73.3
119 32.0 26.2 39.4

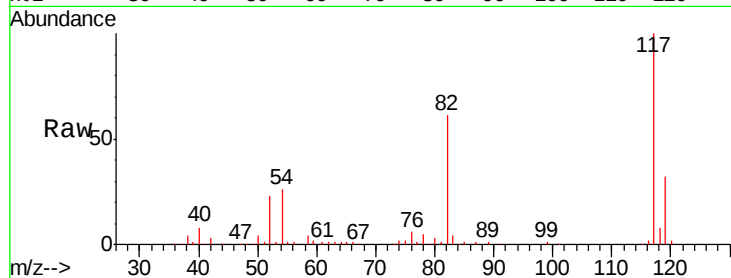


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VU0
Ion 118.90 (118.60 to 119.60): V

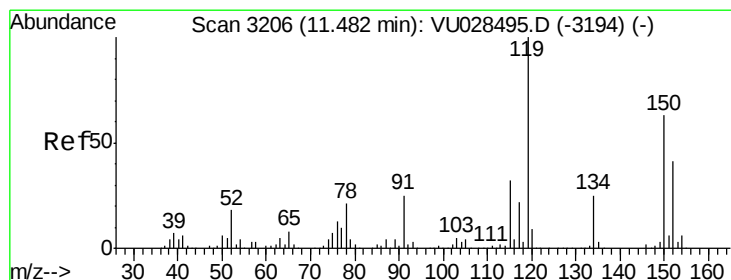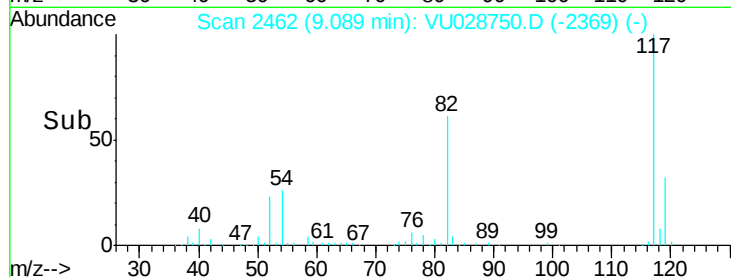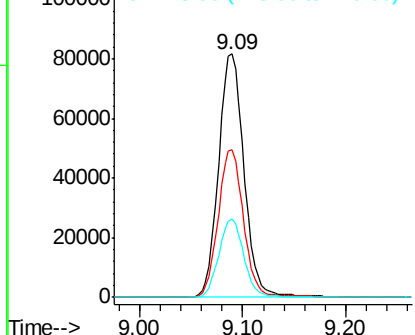

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3206
Delta R.T. -0.00 min
Lab File: VU028750.D
Acq: 18 Dec 2018 03:59

Tgt Ion:152 Resp: 55887
Ion Ratio Lower Upper
152 100
115 59.9 42.7 128.1
150 157.6 0.0 346.0

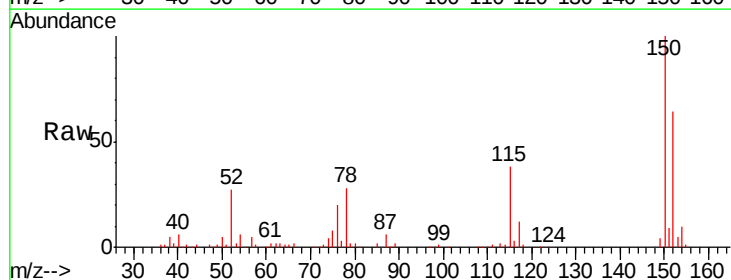

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

