


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121718\
Data File : VU028735.D
Acq On : 17 Dec 2018 21:33
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Title : SW846 8260
Last Update : Fri Dec 07 00:39:42 2018

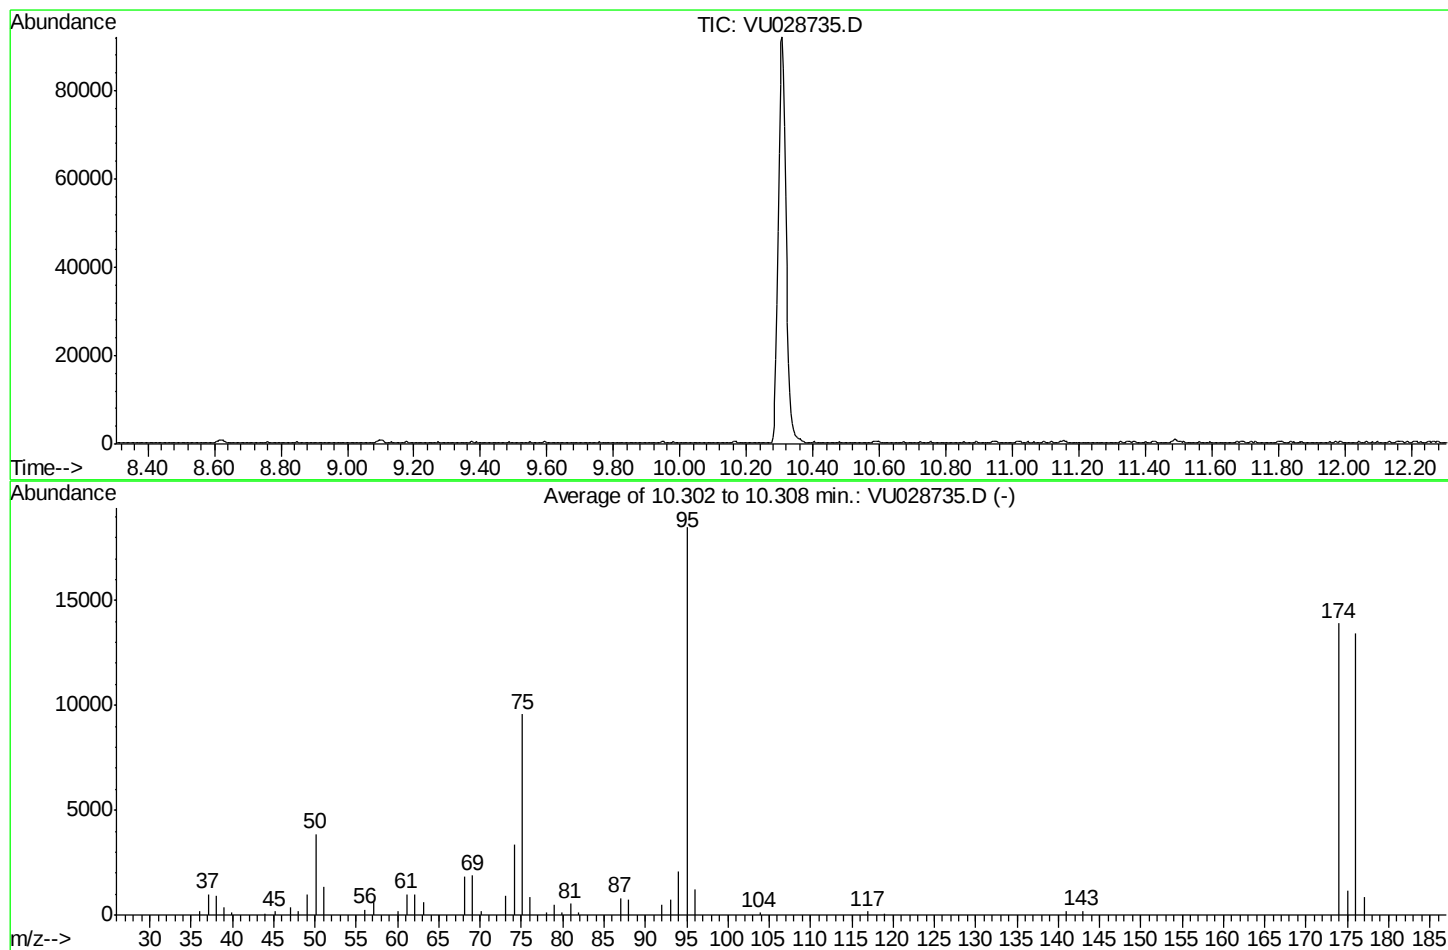

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	3849	PASS
75	95	30	60	51.8	9574	PASS
95	95	100	100	100.0	18490	PASS
96	95	5	9	6.8	1251	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.2	13902	PASS
175	174	5	9	8.2	1143	PASS
176	174	95	101	96.8	13459	PASS
177	176	5	9	6.5	874	PASS