




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046466.D
Acq On : 17 Dec 2021 13:02
Operator : SY/MD
Sample : M5101-14ME
Misc : 6.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL38

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/22/2021
Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 13:56:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 17 03:50:47 2021
Response via : Initial Calibration

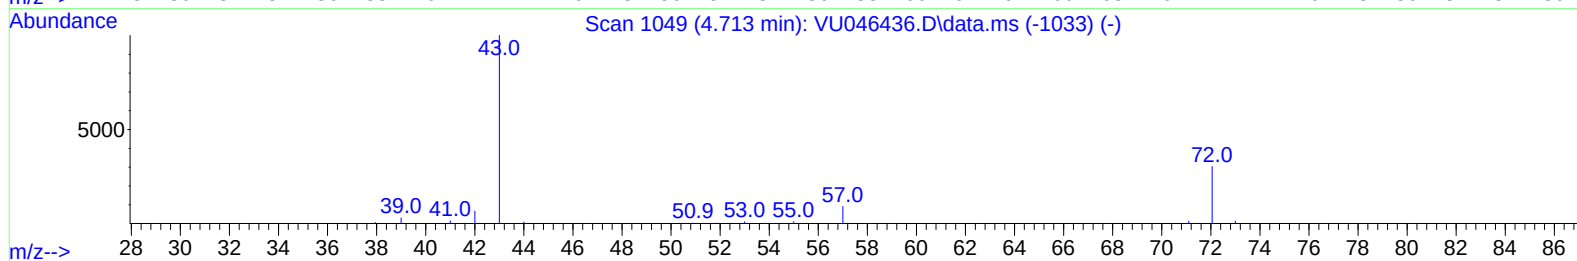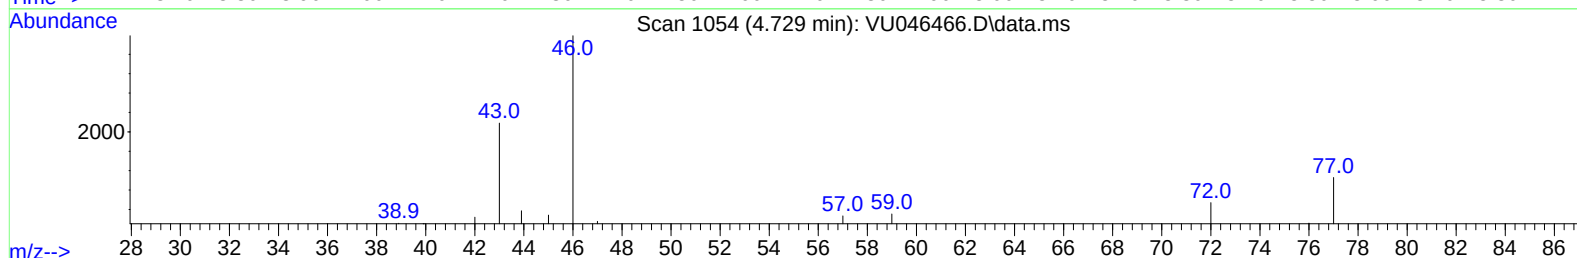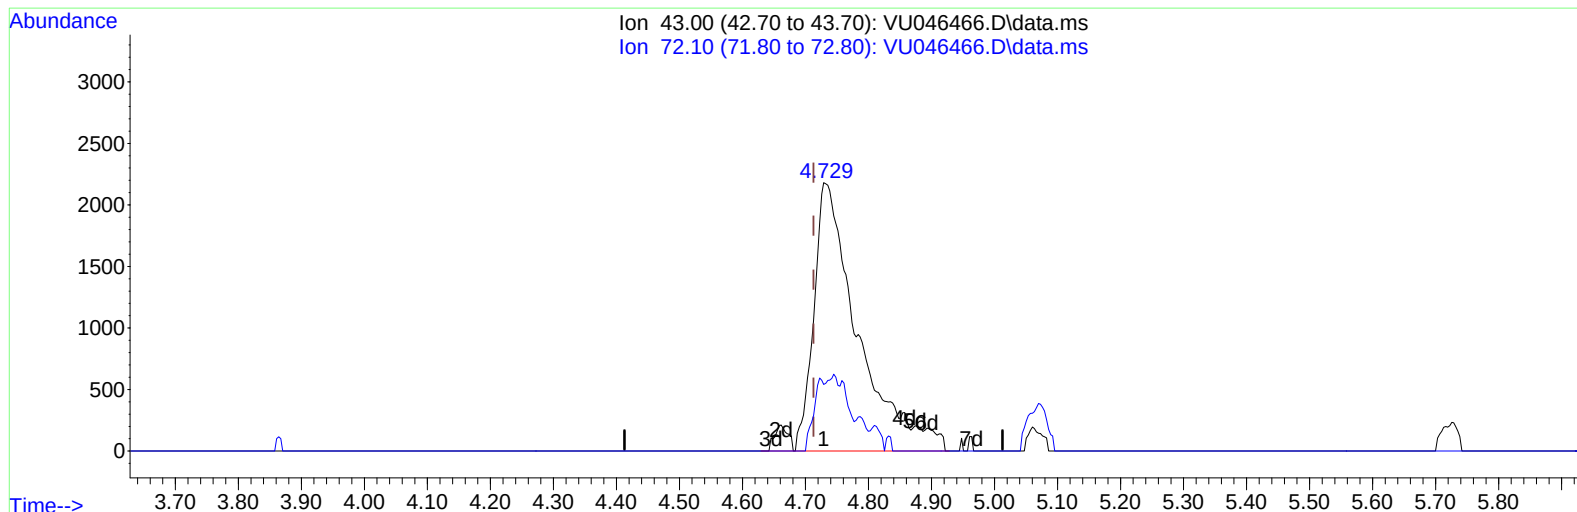

TIC: VU046466.D\data.ms

(22) 2-Butanone (T)

4.729min (+ 0.016) 7.88 ug/L m

response 10877

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.10	6.22#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046466.D
 Acq On : 17 Dec 2021 13:02
 Operator : SY/MD
 Sample : M5101-14ME
 Misc : 6.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL38

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 13:56:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 17 03:50:47 2021
 Response via : Initial Calibration

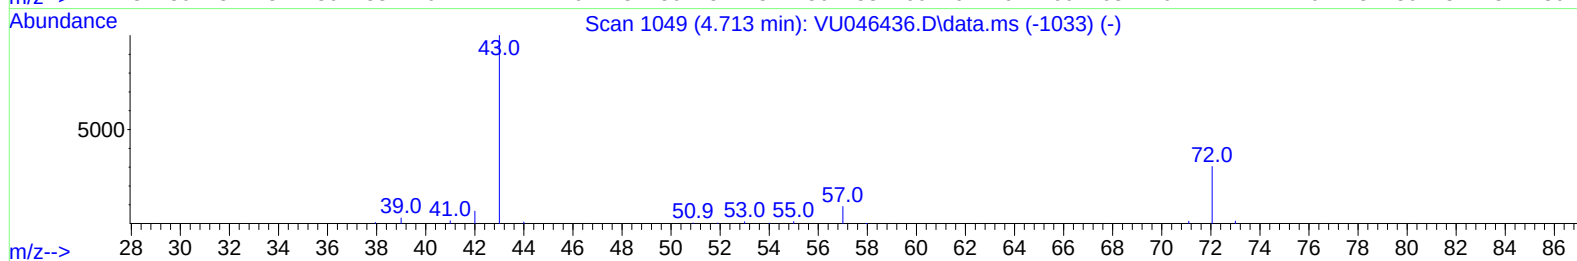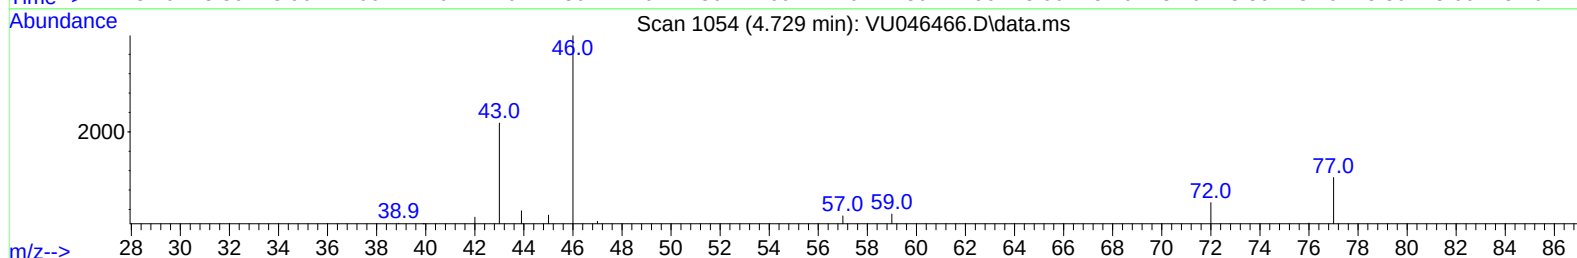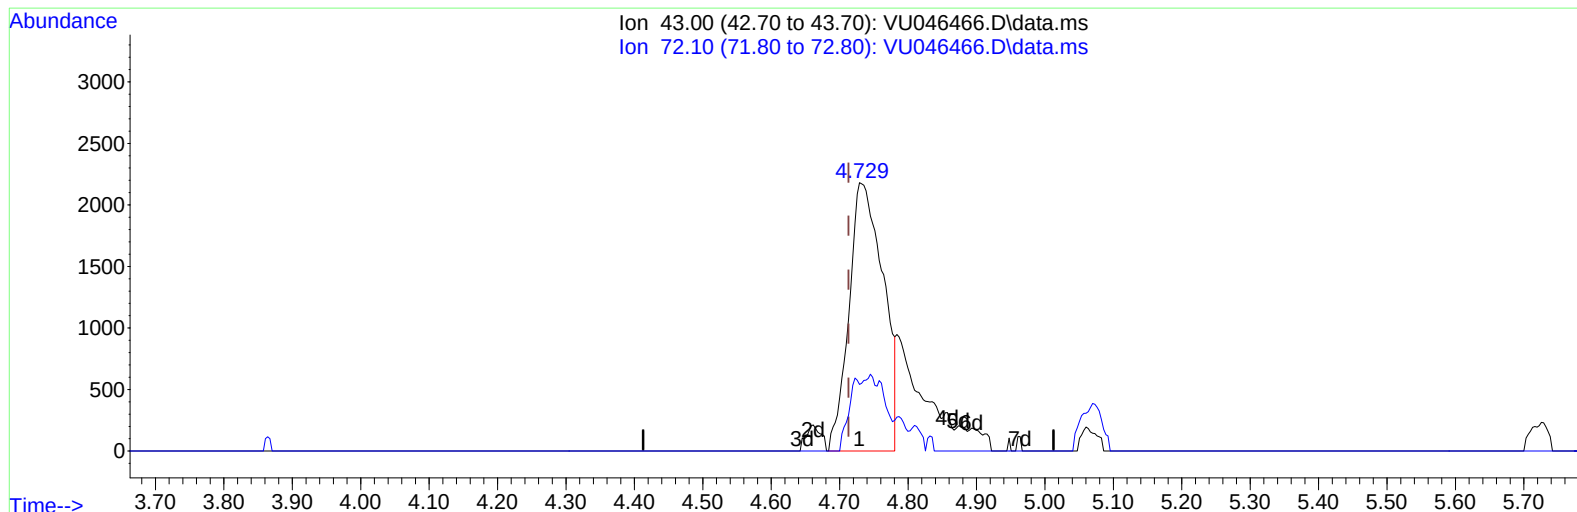

TIC: VU046466.D\data.ms

(22) 2-Butanone (T)

4.729min (+ 0.016) 5.47 ug/L

response 7556

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.10	8.96#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046466.D
 Acq On : 17 Dec 2021 13:02
 Operator : SY/MD
 Sample : M5101-14
 Misc : 6.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL38

Manual IntegrationsAPPROVED

Quant Time: Dec 17 13:56:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 17 03:50:47 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	155026	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	161411	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	79384	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	49564	38.812	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.620%		
7) Chloroethane-d5	1.916	69	35173	35.873	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	71.740%		
11) 1,1-Dichloroethene-d2	2.552	63	92274	40.251	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.500%		
21) 2-Butanone-d5	4.655	46	75940	74.805	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	74.800%		
24) Chloroform-d	5.063	84	94359	44.247	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.500%		
26) 1,2-Dichloroethane-d4	5.703	65	65328	45.646	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.300%		
32) Benzene-d6	5.726	84	186974	40.415	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.840%		
36) 1,2-Dichloropropane-d6	6.694	67	59004	41.153	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	82.300%		
41) Toluene-d8	7.899	98	167215	39.697	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.400%#		
43) trans-1,3-Dichloroprop...	8.185	79	28936	41.807	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.620%		
47) 2-Hexanone-d5	8.684	63	60348	88.772	ug/L	0.05
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.770%		
56) 1,1,2,2-Tetrachloroeth...	10.774	84	85981	39.543	ug/L	0.02
Spiked Amount 50.000	Range 65 - 120		Recovery =	79.080%		
66) 1,2-Dichlorobenzene-d4	12.201	152	64742	42.348	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.700%		
Target Compounds						
12) 1,1-Dichloroethene	2.562	96	47659	44.462	ug/L	96
19) 1,1-Dichloroethane	3.864	63	122333	59.312	ug/L	99
22) 2-Butanone	4.729	43	10877m	7.875	ug/L	
34) Trichloroethene	6.542	95	341490	265.339	ug/L	98
42) Toluene	7.970	91	61234	11.681	ug/L	99
46) Tetrachloroethene	8.555	164	884580	935.289	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046466.D
Acq On : 17 Dec 2021 13:02
Operator : SY/MD
Sample : M5101-14
Misc : 6.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL38

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/22/2021
Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 13:56:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 17 03:50:47 2021
Response via : Initial Calibration

