




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046478.D
 Acq On : 17 Dec 2021 17:34
 Operator : SY/MD
 Sample : M5102-01ME
 Misc : 6.47g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL34ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 23:30:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 17 03:50:47 2021
 Response via : Initial Calibration

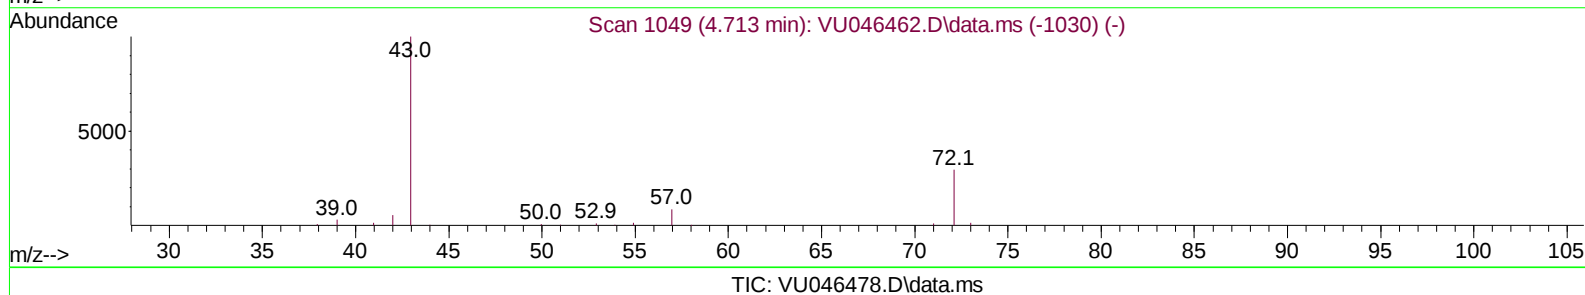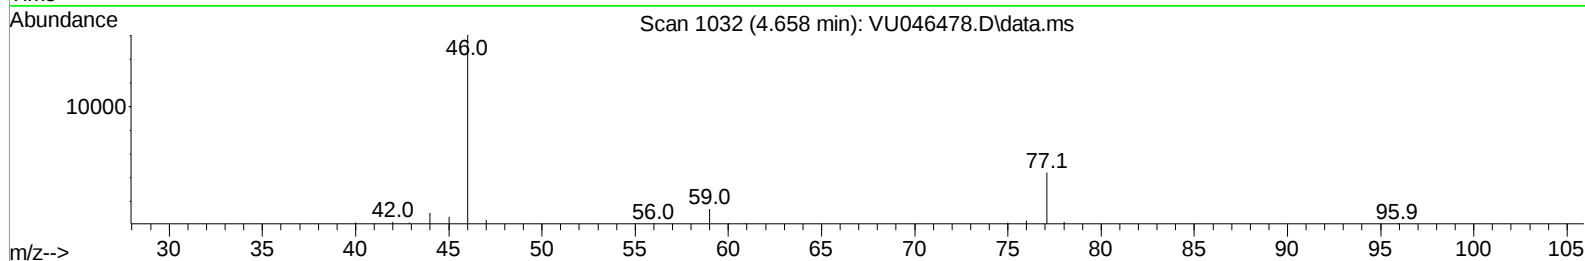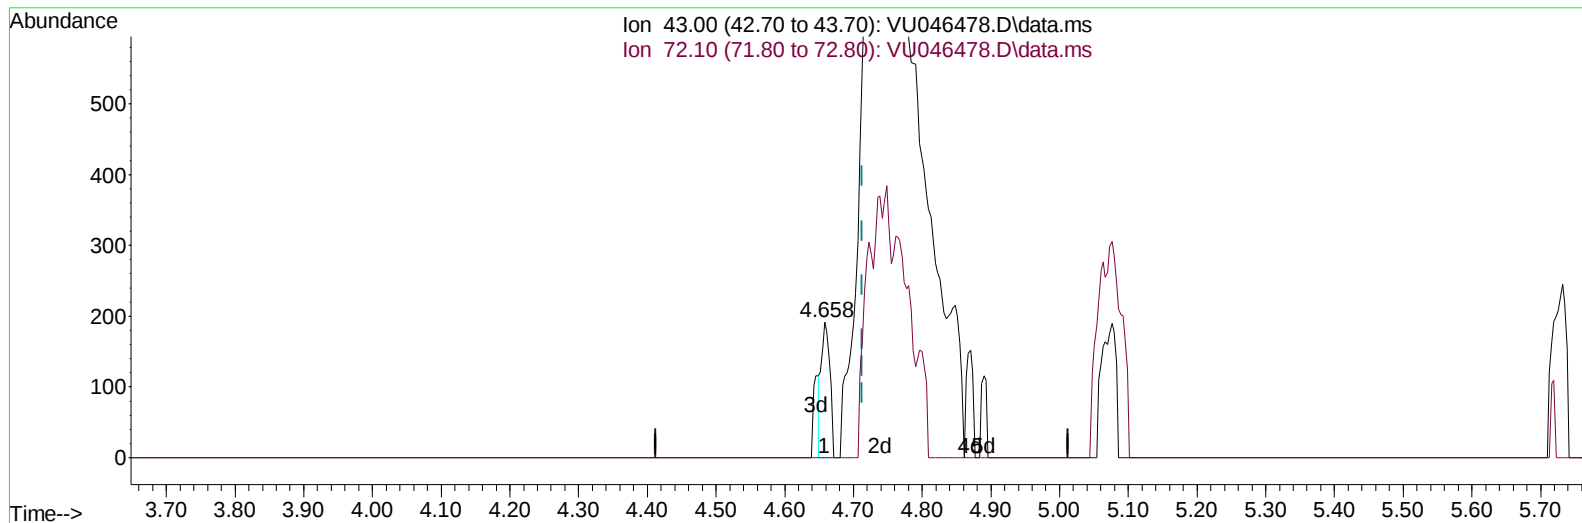

(22) 2-Butanone (T)

4.658min (-0.055) 0.13 ug/L

response 171

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.10	188.30#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046478.D
Acq On : 17 Dec 2021 17:34
Operator : SY/MD
Sample : M5102-01ME
Misc : 6.47g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL34ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/22/2021
Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 23:30:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 17 03:50:47 2021
Response via : Initial Calibration

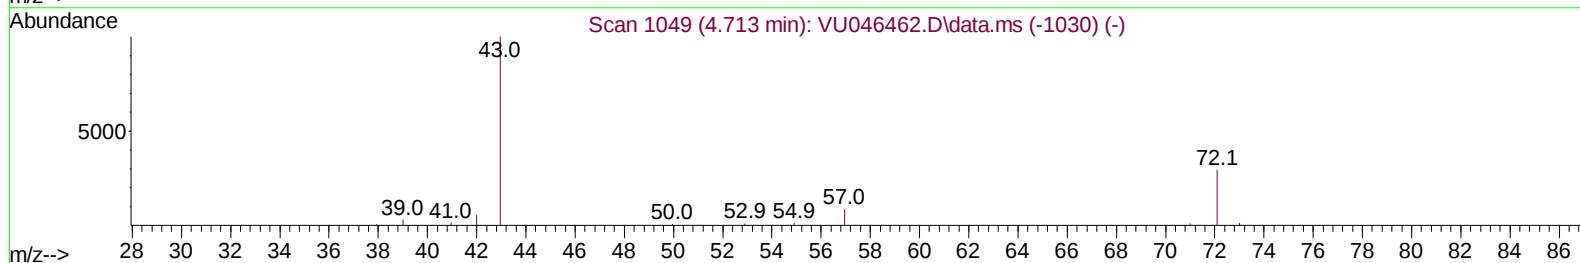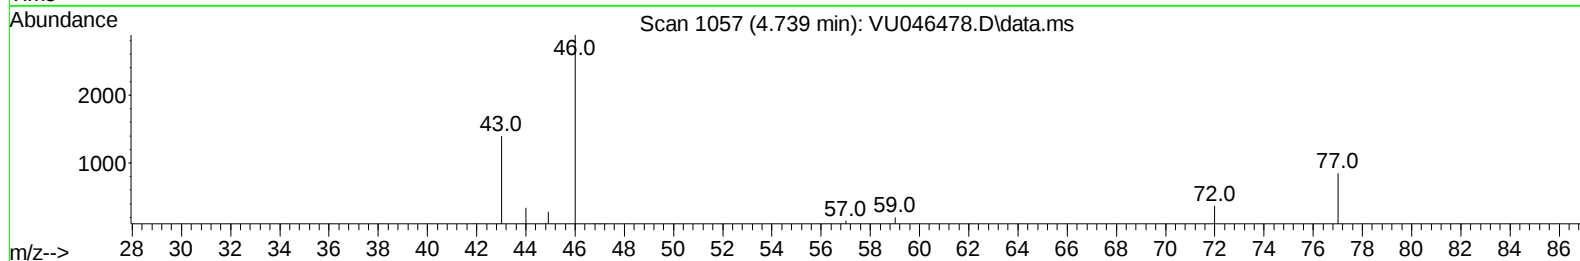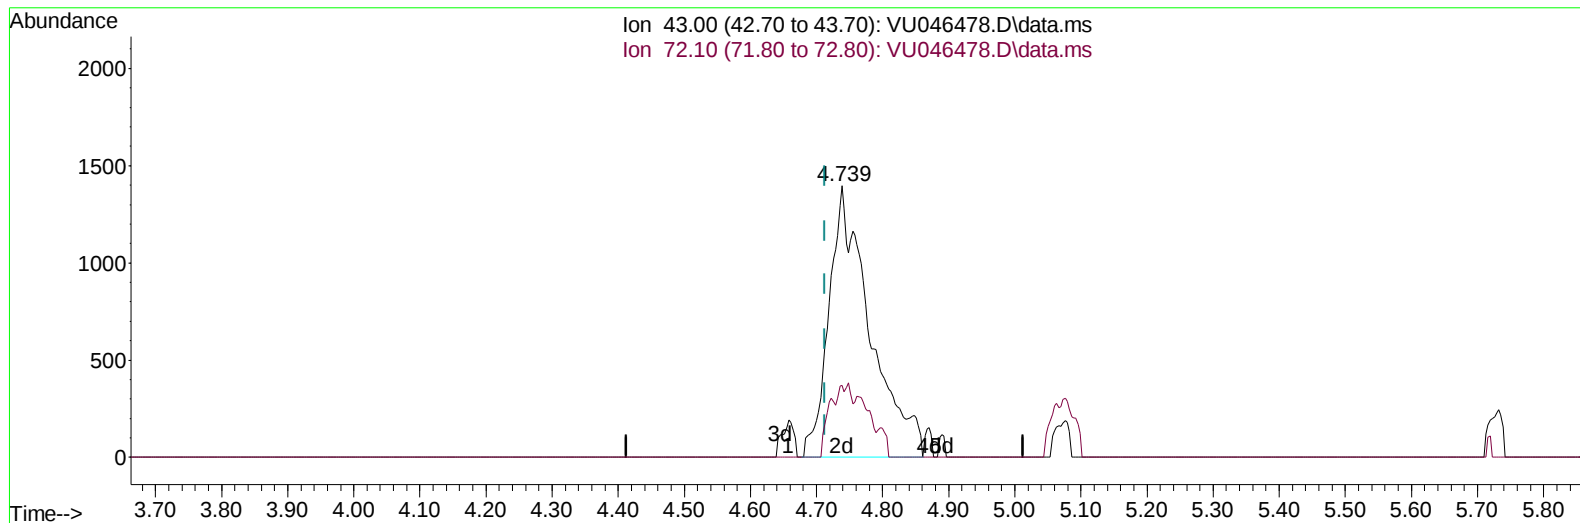

TIC: VU046478.D\data.ms

(22) 2-Butanone (T)

4.739min (+ 0.026) 4.44 ug/L m

response 6013

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.10	5.36#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046478.D
 Acq On : 17 Dec 2021 17:34
 Operator : SY/MD
 Sample : M5102-01ME
 Misc : 6.47g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL34ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/22/2021
 Supervised By :Mahesh Dadoda 12/22/2021

Quant Time: Dec 17 23:30:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 17 03:50:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	152042	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	157991	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	77997	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	43791	34.964	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	69.920%	
7) Chloroethane-d5	1.916	69	31364	32.616	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	65.240%#	
11) 1,1-Dichloroethene-d2	2.546	63	57081	25.388	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	50.780%#	
21) 2-Butanone-d5	4.658	46	69016	69.319	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	69.320%	
24) Chloroform-d	5.063	84	87105	41.647	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.300%	
26) 1,2-Dichloroethane-d4	5.703	65	59944	42.706	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	85.420%	
32) Benzene-d6	5.726	84	169267	37.380	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	74.760%	
36) 1,2-Dichloropropane-d6	6.693	67	54074	38.531	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	77.060%	
41) Toluene-d8	7.899	98	148601	36.042	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	72.080%#	
43) trans-1,3-Dichloroprop...	8.185	79	26983	39.829	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	79.660%	
47) 2-Hexanone-d5	8.681	63	52860	79.441	ug/L	0.04
Spiked Amount 100.000	Range 45	- 130	Recovery	=	79.440%	
56) 1,1,2,2-Tetrachloroeth...	10.774	84	81628	38.353	ug/L	0.02
Spiked Amount 50.000	Range 65	- 120	Recovery	=	76.700%	
66) 1,2-Dichlorobenzene-d4	12.201	152	59461	39.586	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	79.180%#	
Target Compounds						
22) 2-Butanone	4.739	43	6013m	4.439	ug/L	
30) 1,1,1-Trichloroethane	5.311	97	8056	4.154	ug/L	97
46) Tetrachloroethene	8.552	164	4463	4.821	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046478.D
Acq On : 17 Dec 2021 17:34
Operator : SY/MD
Sample : M5102-01ME
Misc : 6.47g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL34ME

Manual IntegrationsAPPROVED

Quant Time: Dec 17 23:30:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 17 03:50:47 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/22/2021
Supervised By :Mahesh Dadoda 12/22/2021

