

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046464.D
 Acq On : 17 Dec 2021 12:17
 Operator : SY/MD
 Sample : VU1217WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	109	rVB	62494	79551	14.54%	1.876%
2	1.919	171	180	200	rBV	46220	68279	12.48%	1.610%
3	2.295	294	297	299	rBV	149	119	0.02%	0.003%
4	2.350	310	314	317	rBV	261	227	0.04%	0.005%
5	2.424	334	337	339	rBV	188	131	0.02%	0.003%
6	2.571	371	383	414	rVV	111009	186339	34.05%	4.395%
7	2.678	414	416	419	rVB	277	168	0.03%	0.004%
8	2.748	435	438	441	rBV	152	150	0.03%	0.004%
9	2.797	448	453	457	rBV2	295	362	0.07%	0.009%
10	2.867	473	475	481	rVB	147	173	0.03%	0.004%
11	3.054	525	533	544	rVB2	1729	3061	0.56%	0.072%
12	3.195	567	577	582	rBV3	737	1478	0.27%	0.035%
13	3.411	641	644	648	rBV	183	178	0.03%	0.004%
14	3.449	653	656	659	rBB	149	125	0.02%	0.003%
15	3.793	759	763	767	rBV	179	212	0.04%	0.005%
16	3.938	805	808	811	rBB	142	121	0.02%	0.003%
17	4.636	1011	1025	1054	rVV	48010	128709	23.52%	3.036%
18	4.838	1086	1088	1095	rVB2	248	253	0.05%	0.006%
19	4.874	1096	1099	1101	rBV2	228	168	0.03%	0.004%
20	4.925	1108	1115	1117	rBB	144	167	0.03%	0.004%
21	4.948	1120	1122	1125	rBV	126	110	0.02%	0.003%
22	5.067	1144	1159	1183	rBV	100901	219229	40.07%	5.171%
23	5.163	1188	1189	1193	rVB2	509	273	0.05%	0.006%
24	5.298	1229	1231	1233	rBV	218	114	0.02%	0.003%
25	5.311	1233	1235	1239	rVB	242	169	0.03%	0.004%
26	5.729	1344	1365	1390	rBV2	200629	547172	100.00%	12.905%
27	6.253	1514	1528	1553	rBV	174432	329276	60.18%	7.766%
28	6.356	1558	1560	1563	rVB	297	184	0.03%	0.004%
29	6.533	1610	1615	1618	rBB	438	349	0.06%	0.008%
30	6.549	1618	1620	1624	rBB	141	121	0.02%	0.003%
31	6.694	1651	1665	1684	rBV	126936	243560	44.51%	5.744%
32	7.047	1771	1775	1776	rBV	230	160	0.03%	0.004%
33	7.179	1813	1816	1820	rBV	194	225	0.04%	0.005%
34	7.240	1830	1835	1838	rBB	175	193	0.04%	0.005%
35	7.292	1848	1851	1853	rBV	132	118	0.02%	0.003%
36	7.568	1925	1937	1956	rBV	68323	117855	21.54%	2.780%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046464.D
 Acq On : 17 Dec 2021 12:17
 Operator : SY/MD
 Sample : VU1217WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.690	1970	1975	1977	rBB	324	260	0.05%	0.006%
38	7.838	2018	2021	2026	rBB	133	137	0.03%	0.003%
39	7.899	2027	2040	2056	rBV	247534	423716	77.44%	9.993%
40	7.973	2059	2063	2073	rVB	3533	4531	0.83%	0.107%
41	8.182	2112	2128	2149	rBV	48497	80491	14.71%	1.898%
42	8.282	2157	2159	2162	rVB	260	141	0.03%	0.003%
43	8.314	2165	2169	2170	rBV	223	151	0.03%	0.004%
44	8.346	2174	2179	2181	rBV	141	147	0.03%	0.003%
45	8.475	2214	2219	2221	rBV	256	263	0.05%	0.006%
46	8.491	2221	2224	2228	rVV2	236	211	0.04%	0.005%
47	8.568	2245	2248	2252	rVB2	284	200	0.04%	0.005%
48	8.636	2257	2269	2294	rBV	162665	273116	49.91%	6.441%
49	8.764	2306	2309	2312	rVB2	183	133	0.02%	0.003%
50	8.912	2350	2355	2362	rBV3	628	962	0.18%	0.023%
51	9.050	2396	2398	2401	rVB	169	113	0.02%	0.003%
52	9.073	2402	2405	2408	rBB	154	123	0.02%	0.003%
53	9.118	2416	2419	2422	rBB	163	129	0.02%	0.003%
54	9.137	2423	2425	2429	rBV	120	131	0.02%	0.003%
55	9.275	2466	2468	2472	rBV	149	148	0.03%	0.003%
56	9.369	2492	2497	2500	rBB	162	194	0.04%	0.005%
57	9.420	2501	2513	2535	rBV	260723	424572	77.59%	10.014%
58	9.510	2539	2541	2544	rVB	366	187	0.03%	0.004%
59	9.568	2555	2559	2561	rBV	218	181	0.03%	0.004%
60	9.597	2565	2568	2570	rVB	166	113	0.02%	0.003%
61	9.619	2571	2575	2578	rBB	150	149	0.03%	0.004%
62	9.658	2583	2587	2589	rBB	132	115	0.02%	0.003%
63	9.674	2589	2592	2594	rBV	149	124	0.02%	0.003%
64	9.690	2594	2597	2599	rVV	171	118	0.02%	0.003%
65	9.700	2599	2600	2604	rVB2	289	179	0.03%	0.004%
66	9.732	2607	2610	2612	rBV	132	117	0.02%	0.003%
67	9.883	2653	2657	2661	rBB	173	196	0.04%	0.005%
68	10.005	2689	2695	2701	rBV	174	318	0.06%	0.008%
69	10.317	2787	2792	2794	rBB	164	156	0.03%	0.004%
70	10.336	2795	2798	2802	rBV	154	182	0.03%	0.004%
71	10.555	2864	2866	2873	rVB	165	213	0.04%	0.005%
72	10.668	2897	2901	2903	rBV2	848	618	0.11%	0.015%
73	10.758	2917	2929	2944	rBV	181784	289201	52.85%	6.821%
74	10.838	2949	2954	2957	rBV	167	210	0.04%	0.005%
75	10.906	2971	2975	2980	rVB2	252	259	0.05%	0.006%
76	11.111	3032	3039	3044	rBV	185	345	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046464.D
 Acq On : 17 Dec 2021 12:17
 Operator : SY/MD
 Sample : VU1217WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.314	3099	3102	3106	rVB	163	158	0.03%	0.004%
78	11.336	3106	3109	3111	rBV	164	135	0.02%	0.003%
79	11.378	3119	3122	3124	rBV	131	115	0.02%	0.003%
80	11.455	3141	3146	3147	rBV2	482	381	0.07%	0.009%
81	11.568	3179	3181	3183	rBV	172	121	0.02%	0.003%
82	11.642	3201	3204	3205	rBV	164	113	0.02%	0.003%
83	11.812	3245	3257	3275	rVV	261786	414588	75.77%	9.778%
84	11.976	3303	3308	3311	rBV	477	330	0.06%	0.008%
85	12.195	3363	3376	3392	rVV	243929	386522	70.64%	9.116%
86	12.774	3549	3556	3562	rVV2	675	906	0.17%	0.021%
87	13.854	3889	3892	3899	rVB2	337	230	0.04%	0.005%
88	14.098	3960	3968	3973	rVB2	395	630	0.12%	0.015%
89	14.169	3986	3990	3993	rBV	143	116	0.02%	0.003%
90	14.336	4039	4042	4046	rVB2	313	231	0.04%	0.005%
91	14.587	4111	4120	4126	rBV3	762	1091	0.20%	0.026%
92	15.503	4403	4405	4409	rVB	256	157	0.03%	0.004%
93	15.603	4433	4436	4437	rBV2	210	122	0.02%	0.003%
94	15.629	4440	4444	4449	rVV	223	249	0.05%	0.006%
95	15.886	4517	4524	4527	rBV2	223	282	0.05%	0.007%
96	16.523	4719	4722	4725	rBV	342	301	0.06%	0.007%
97	16.783	4800	4803	4807	rVB2	457	338	0.06%	0.008%
98	16.809	4807	4811	4814	rBV2	381	364	0.07%	0.009%
99	17.005	4870	4872	4874	rBV	346	190	0.03%	0.004%
100	17.593	5052	5055	5057	rBV2	623	347	0.06%	0.008%




Sum of corrected areas: 4239946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046464.D
Acq On : 17 Dec 2021 12:17
Operator : SY/MD
Sample : VU1217WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

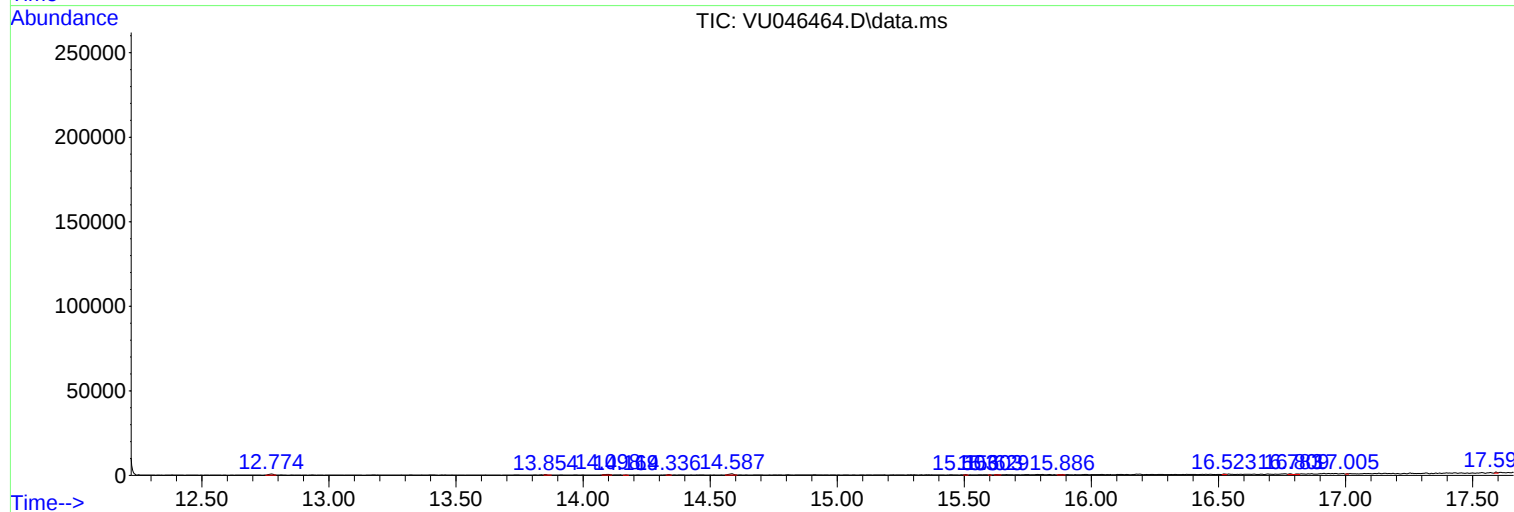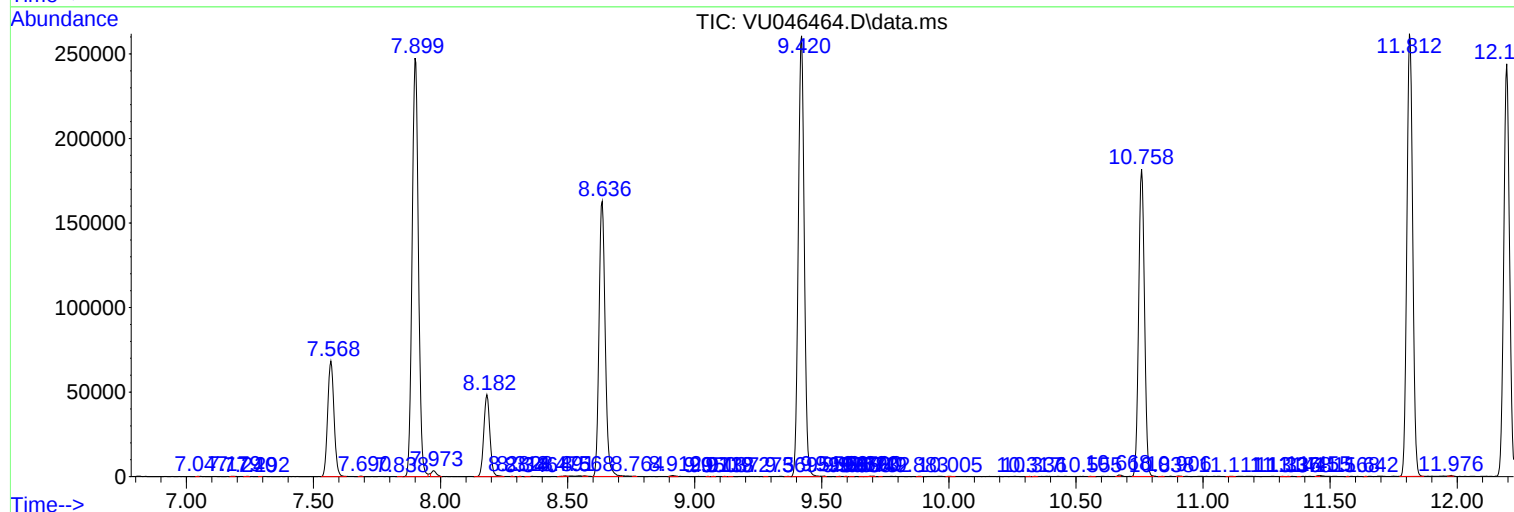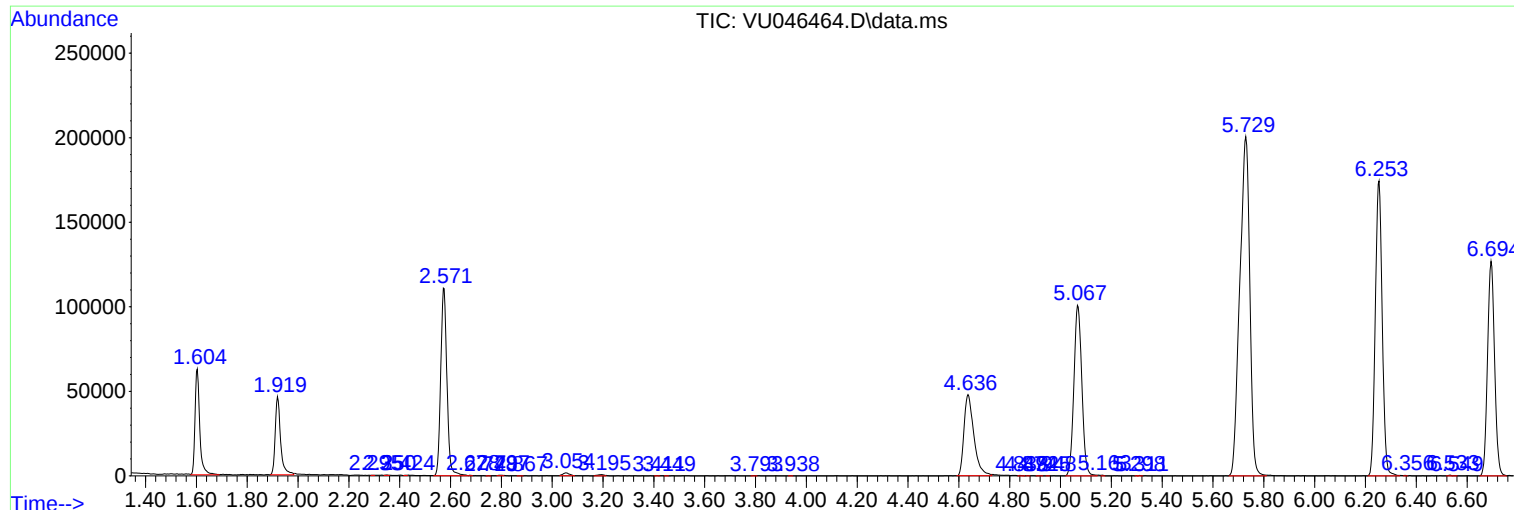

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046464.D
Acq On : 17 Dec 2021 12:17
Operator : SY/MD
Sample : VU1217WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046464.D
Acq On : 17 Dec 2021 12:17
Operator : SY/MD
Sample : VU1217WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc