

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046470.D
 Acq On : 17 Dec 2021 14:33
 Operator : SY/MD
 Sample : M5103-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	102	rBV2	77371	100365	0.70%	0.329%
2	1.919	172	180	201	rBV	46046	67096	0.47%	0.220%
3	2.575	372	384	418	rVB2	116291	202383	1.40%	0.664%
4	2.703	419	424	427	rVB	269	277	0.00%	0.001%
5	2.732	430	433	437	rBV	138	161	0.00%	0.001%
6	2.800	450	454	459	rBB	145	205	0.00%	0.001%
7	2.944	496	499	502	rBB	140	116	0.00%	0.000%
8	3.195	564	577	587	rBB2	2328	5075	0.04%	0.017%
9	3.240	588	591	594	rBV	156	146	0.00%	0.000%
10	3.359	615	628	643	rBV	22132	42727	0.30%	0.140%
11	3.864	779	785	787	rBV	1035	1021	0.01%	0.003%
12	4.552	997	999	1003	rBB	127	112	0.00%	0.000%
13	4.671	1011	1036	1082	rBV	867209	2055167	14.26%	6.744%
14	4.851	1090	1092	1095	rVB2	460	260	0.00%	0.001%
15	4.944	1119	1121	1125	rBB	305	216	0.00%	0.001%
16	5.066	1143	1159	1178	rBV	100524	219551	1.52%	0.720%
17	5.224	1206	1208	1211	rBB2	230	131	0.00%	0.000%
18	5.263	1217	1220	1223	rVV2	214	146	0.00%	0.000%
19	5.279	1223	1225	1226	rVV	201	110	0.00%	0.000%
20	5.324	1226	1239	1252	rVV2	5036	10641	0.07%	0.035%
21	5.729	1344	1365	1393	rBV2	199802	548386	3.80%	1.799%
22	6.253	1513	1528	1553	rBV2	173839	330398	2.29%	1.084%
23	6.369	1561	1564	1567	rVV	274	241	0.00%	0.001%
24	6.549	1602	1620	1653	rBV	7660006	14415232	100.00%	47.301%
25	6.693	1655	1665	1684	rVB	129073	254381	1.76%	0.835%
26	6.922	1733	1736	1742	rBB	257	226	0.00%	0.001%
27	7.063	1777	1780	1783	rBB	138	116	0.00%	0.000%
28	7.185	1814	1818	1823	rVB2	447	429	0.00%	0.001%
29	7.497	1911	1915	1918	rBB	129	112	0.00%	0.000%
30	7.568	1925	1937	1958	rBV	69064	119721	0.83%	0.393%
31	7.697	1974	1977	1979	rVB	424	253	0.00%	0.001%
32	7.899	2027	2040	2056	rBV	246039	423238	2.94%	1.389%
33	7.973	2057	2063	2073	rVV	4537	7060	0.05%	0.023%
34	8.018	2075	2077	2080	rBB	254	126	0.00%	0.000%
35	8.105	2100	2104	2107	rBB	126	112	0.00%	0.000%
36	8.182	2116	2128	2149	rBV	48827	82216	0.57%	0.270%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046470.D
 Acq On : 17 Dec 2021 14:33
 Operator : SY/MD
 Sample : M5103-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.259	2149	2152	2156	rVB2	277	203	0.00%	0.001%
38	8.295	2161	2163	2166	rBV	140	117	0.00%	0.000%
39	8.359	2182	2183	2188	rBB	242	134	0.00%	0.000%
40	8.398	2193	2195	2198	rVV2	324	160	0.00%	0.001%
41	8.423	2200	2203	2207	rBB	161	154	0.00%	0.001%
42	8.475	2207	2219	2229	rBV	27028	47347	0.33%	0.155%
43	8.558	2229	2245	2260	rVV	5750212	9601478	66.61%	31.505%
44	8.632	2260	2268	2297	rVV	171405	304089	2.11%	0.998%
45	8.742	2297	2302	2310	rVV3	442	629	0.00%	0.002%
46	8.774	2310	2312	2316	rVV2	174	149	0.00%	0.000%
47	8.825	2323	2328	2329	rBV	145	125	0.00%	0.000%
48	8.841	2329	2333	2340	rVB2	318	391	0.00%	0.001%
49	8.989	2377	2379	2381	rBV	230	113	0.00%	0.000%
50	9.176	2434	2437	2440	rBB	128	113	0.00%	0.000%
51	9.214	2445	2449	2452	rVV	120	122	0.00%	0.000%
52	9.256	2459	2462	2464	rBV	118	108	0.00%	0.000%
53	9.365	2493	2496	2500	rBV	153	179	0.00%	0.001%
54	9.417	2500	2512	2530	rBV	254595	424188	2.94%	1.392%
55	9.510	2539	2541	2544	rBV2	280	192	0.00%	0.001%
56	9.700	2593	2600	2606	rBB3	694	827	0.01%	0.003%
57	9.761	2607	2619	2629	rBB2	6875	11344	0.08%	0.037%
58	9.844	2641	2645	2647	rBV	145	150	0.00%	0.000%
59	9.883	2654	2657	2660	rBB	148	123	0.00%	0.000%
60	9.902	2660	2663	2666	rBB	140	116	0.00%	0.000%
61	9.922	2666	2669	2672	rBV	143	152	0.00%	0.000%
62	10.082	2715	2719	2721	rBB	125	111	0.00%	0.000%
63	10.211	2756	2759	2763	rBB	172	162	0.00%	0.001%
64	10.233	2764	2766	2769	rBB	175	111	0.00%	0.000%
65	10.324	2792	2794	2799	rBV	146	167	0.00%	0.001%
66	10.349	2799	2802	2805	rVB	157	126	0.00%	0.000%
67	10.375	2807	2810	2813	rBB	149	121	0.00%	0.000%
68	10.394	2813	2816	2821	rBB	144	171	0.00%	0.001%
69	10.484	2842	2844	2848	rVB	268	176	0.00%	0.001%
70	10.571	2868	2871	2874	rBV	153	154	0.00%	0.001%
71	10.671	2895	2902	2903	rBV2	870	821	0.01%	0.003%
72	10.758	2917	2929	2945	rBV	178658	283637	1.97%	0.931%
73	10.893	2959	2971	2984	rBV	30035	49424	0.34%	0.162%
74	11.095	3030	3034	3036	rBV	150	157	0.00%	0.001%
75	11.131	3043	3045	3047	rBV	166	115	0.00%	0.000%
76	11.327	3098	3106	3114	rBV	175	455	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046470.D
 Acq On : 17 Dec 2021 14:33
 Operator : SY/MD
 Sample : M5103-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.459	3141	3147	3151	rBV	337	407	0.00%	0.001%
78	11.812	3245	3257	3276	rVB	278887	434969	3.02%	1.427%
79	11.973	3303	3307	3310	rBV	394	269	0.00%	0.001%
80	12.063	3330	3335	3342	rBV3	758	794	0.01%	0.003%
81	12.127	3350	3355	3357	rBV	206	234	0.00%	0.001%
82	12.195	3364	3376	3395	rVV	252041	394639	2.74%	1.295%
83	12.542	3481	3484	3487	rVB	194	158	0.00%	0.001%
84	12.581	3487	3496	3500	rBV	235	423	0.00%	0.001%
85	12.774	3544	3556	3566	rBV2	11654	17266	0.12%	0.057%
86	13.233	3691	3699	3706	rBV3	3875	5324	0.04%	0.017%
87	13.417	3753	3756	3760	rVB	138	111	0.00%	0.000%
88	13.638	3820	3825	3829	rBV	178	175	0.00%	0.001%
89	13.741	3852	3857	3861	rVB	131	143	0.00%	0.000%
90	14.095	3964	3967	3972	rBV2	212	194	0.00%	0.001%
91	14.581	4109	4118	4128	rVB2	1262	2154	0.01%	0.007%
92	15.208	4308	4313	4316	rVB	256	239	0.00%	0.001%
93	15.240	4320	4323	4326	rBV	208	141	0.00%	0.000%
94	15.468	4391	4394	4398	rVV2	187	125	0.00%	0.000%
95	15.725	4469	4474	4479	rBV2	219	253	0.00%	0.001%
96	15.783	4490	4492	4495	rBV2	180	126	0.00%	0.000%
97	15.880	4514	4522	4524	rBV2	226	290	0.00%	0.001%
98	16.410	4685	4687	4689	rBV2	231	125	0.00%	0.000%
99	16.503	4713	4716	4718	rBV2	291	214	0.00%	0.001%
100	17.179	4924	4926	4929	rBV3	419	241	0.00%	0.001%




Sum of corrected areas: 30475778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046470.D
Acq On : 17 Dec 2021 14:33
Operator : SY/MD
Sample : M5103-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

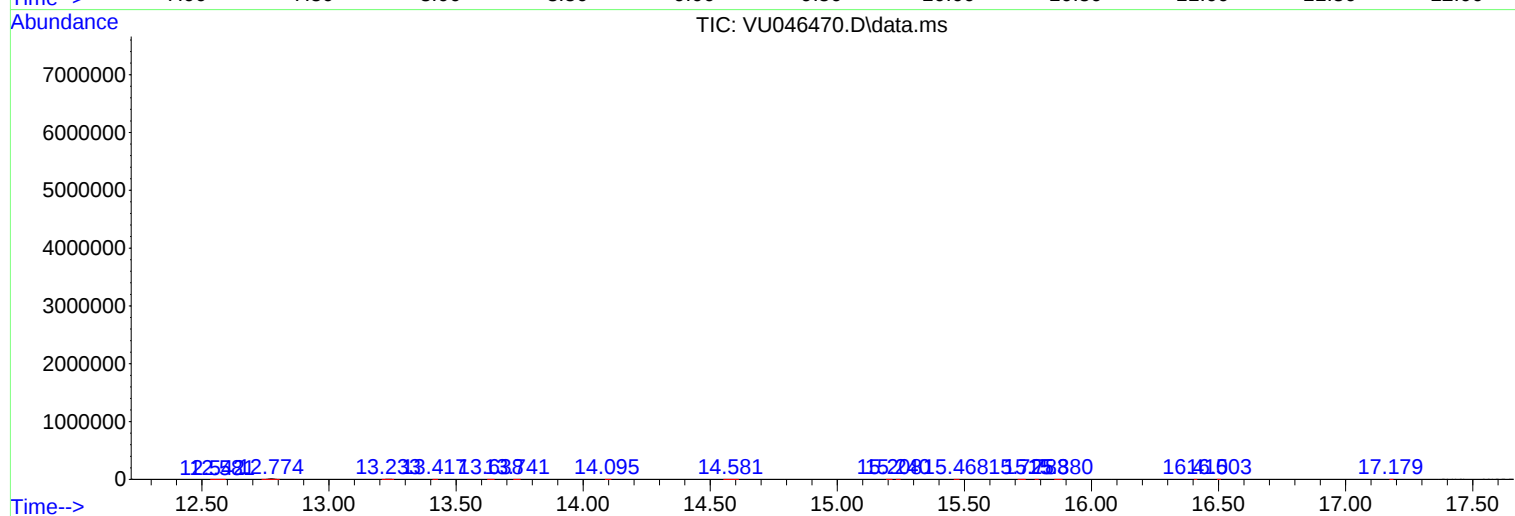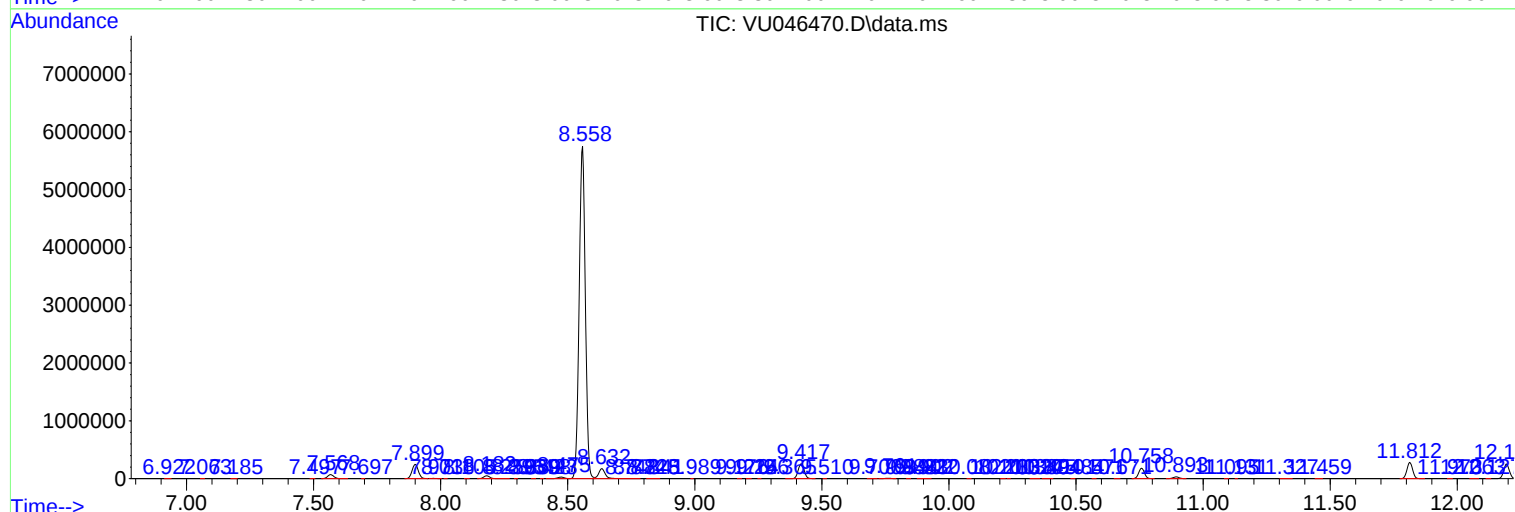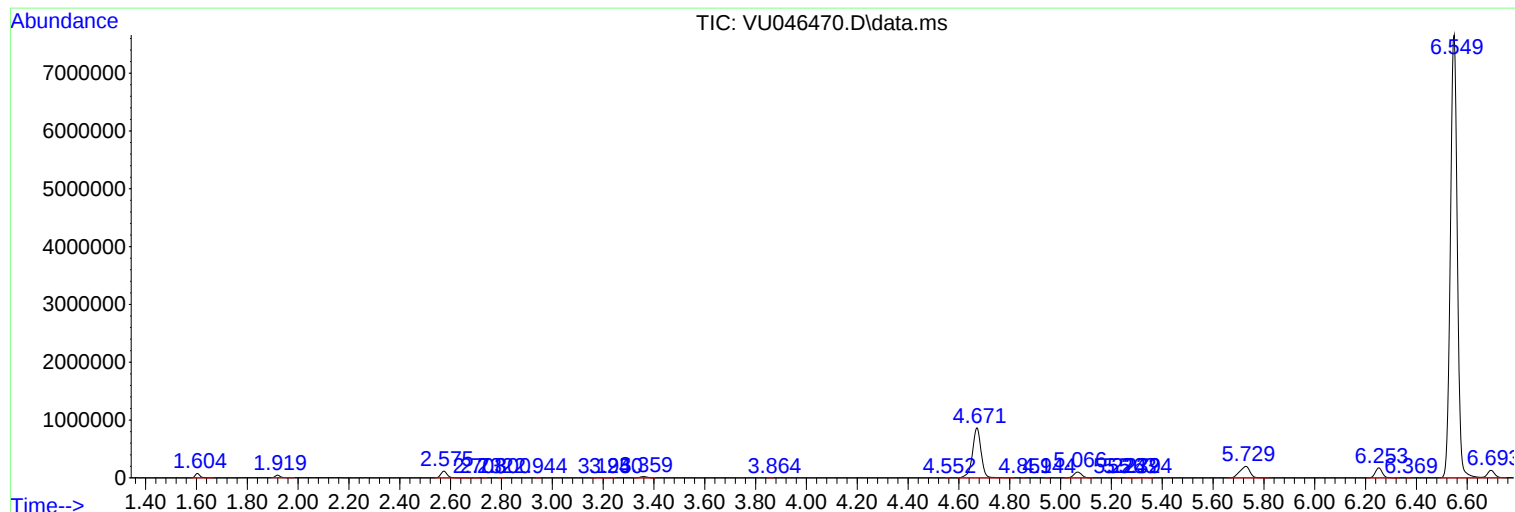

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046470.D
Acq On : 17 Dec 2021 14:33
Operator : SY/MD
Sample : M5103-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046470.D
Acq On : 17 Dec 2021 14:33
Operator : SY/MD
Sample : M5103-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc