

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046472.D
 Acq On : 17 Dec 2021 15:18
 Operator : SY/MD
 Sample : M5037-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

Signal : TIC: VU046472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	100	rBV	57692	72886	13.71%	1.695%
2	1.919	171	180	209	rBV	44595	65039	12.23%	1.513%
3	2.366	316	319	323	rBV2	173	169	0.03%	0.004%
4	2.395	323	328	330	rBV3	224	233	0.04%	0.005%
5	2.430	335	339	344	rVV3	246	263	0.05%	0.006%
6	2.571	371	383	397	rBV	107219	176728	33.24%	4.111%
7	2.649	401	407	429	rVB2	8706	22543	4.24%	0.524%
8	2.748	436	438	443	rVB2	204	130	0.02%	0.003%
9	2.845	465	468	471	rBV	137	139	0.03%	0.003%
10	2.915	486	490	491	rBV2	268	214	0.04%	0.005%
11	2.983	509	511	515	rVB	196	153	0.03%	0.004%
12	3.054	525	533	544	rVB3	2228	4241	0.80%	0.099%
13	3.102	544	548	550	rBV	170	153	0.03%	0.004%
14	3.192	567	576	577	rBV2	732	969	0.18%	0.023%
15	3.282	599	604	607	rBB	175	184	0.03%	0.004%
16	3.391	634	638	641	rBB	141	142	0.03%	0.003%
17	3.430	647	650	654	rBB	145	146	0.03%	0.003%
18	3.948	809	811	816	rBB	163	150	0.03%	0.003%
19	4.456	967	969	974	rBB	174	163	0.03%	0.004%
20	4.636	1011	1025	1047	rBV	47144	132297	24.89%	3.077%
21	4.793	1071	1074	1079	rVB2	256	225	0.04%	0.005%
22	4.851	1089	1092	1094	rBV2	236	165	0.03%	0.004%
23	4.996	1132	1137	1141	rBV	159	212	0.04%	0.005%
24	5.067	1143	1159	1177	rBV	97813	212828	40.03%	4.950%
25	5.301	1226	1232	1235	rBB2	349	363	0.07%	0.008%
26	5.359	1248	1250	1253	rBB	237	134	0.03%	0.003%
27	5.729	1343	1365	1393	rBV2	195741	531633	100.00%	12.366%
28	5.825	1393	1395	1400	rVB	255	125	0.02%	0.003%
29	6.189	1504	1508	1511	rBB	152	157	0.03%	0.004%
30	6.253	1512	1528	1553	rBV	171913	324557	61.05%	7.549%
31	6.353	1558	1559	1563	rVV	269	211	0.04%	0.005%
32	6.375	1563	1566	1569	rVB	237	152	0.03%	0.004%
33	6.546	1609	1619	1630	rBB2	7579	13544	2.55%	0.315%
34	6.594	1631	1634	1638	rBB	334	236	0.04%	0.005%
35	6.693	1652	1665	1688	rBB	122768	237099	44.60%	5.515%
36	6.883	1719	1724	1726	rBV	148	172	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046472.D
 Acq On : 17 Dec 2021 15:18
 Operator : SY/MD
 Sample : M5037-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.025	1766	1768	1773	rBB	148	151	0.03%	0.004%
38	7.054	1774	1777	1779	rBB	272	170	0.03%	0.004%
39	7.185	1816	1818	1821	rVV	273	130	0.02%	0.003%
40	7.568	1925	1937	1955	rBV	65948	113154	21.28%	2.632%
41	7.899	2026	2040	2054	rBV	239556	409460	77.02%	9.524%
42	7.970	2056	2062	2074	rVB	6516	10697	2.01%	0.249%
43	8.182	2116	2128	2144	rBV	46529	77973	14.67%	1.814%
44	8.243	2144	2147	2151	rVV	385	394	0.07%	0.009%
45	8.472	2205	2218	2229	rBV2	7771	13732	2.58%	0.319%
46	8.555	2235	2244	2254	rVB2	9769	15880	2.99%	0.369%
47	8.636	2257	2269	2296	rBV	164869	274436	51.62%	6.384%
48	8.761	2305	2308	2311	rBV	165	157	0.03%	0.004%
49	8.787	2311	2316	2330	rVB3	1265	1719	0.32%	0.040%
50	8.864	2336	2340	2343	rBB	176	136	0.03%	0.003%
51	8.883	2344	2346	2354	rBV	137	230	0.04%	0.005%
52	9.028	2387	2391	2393	rBV	136	145	0.03%	0.003%
53	9.266	2461	2465	2469	rBB	164	185	0.03%	0.004%
54	9.349	2487	2491	2493	rBB	155	129	0.02%	0.003%
55	9.365	2493	2496	2500	rBV	158	186	0.03%	0.004%
56	9.420	2500	2513	2529	rBV	256766	421502	79.28%	9.804%
57	9.574	2555	2561	2563	rBV2	363	385	0.07%	0.009%
58	9.697	2591	2599	2607	rVB3	1097	1657	0.31%	0.039%
59	9.732	2608	2610	2615	rBV	162	169	0.03%	0.004%
60	9.848	2643	2646	2648	rBV	146	130	0.02%	0.003%
61	9.915	2665	2667	2670	rBV	172	145	0.03%	0.003%
62	9.967	2679	2683	2687	rBB	159	181	0.03%	0.004%
63	9.992	2687	2691	2694	rBV	174	203	0.04%	0.005%
64	10.060	2707	2712	2714	rBV	138	141	0.03%	0.003%
65	10.098	2721	2724	2728	rBV3	366	315	0.06%	0.007%
66	10.320	2789	2793	2796	rBV	173	181	0.03%	0.004%
67	10.462	2835	2837	2843	rVB	147	177	0.03%	0.004%
68	10.526	2854	2857	2859	rBV	172	134	0.03%	0.003%
69	10.578	2867	2873	2881	rBV3	1476	1926	0.36%	0.045%
70	10.674	2897	2903	2909	rBV4	878	1052	0.20%	0.024%
71	10.758	2916	2929	2949	rBV	180281	285876	53.77%	6.650%
72	10.896	2960	2972	2982	rBV	10538	16877	3.17%	0.393%
73	10.957	2987	2991	2992	rBV	196	161	0.03%	0.004%
74	11.018	3007	3010	3013	rBB	161	132	0.02%	0.003%
75	11.111	3035	3039	3042	rBV	165	186	0.03%	0.004%
76	11.233	3075	3077	3080	rBV	149	126	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046472.D
 Acq On : 17 Dec 2021 15:18
 Operator : SY/MD
 Sample : M5037-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.471	3144	3151	3158	rVB6	914	1328	0.25%	0.031%
78	11.690	3213	3219	3220	rBV2	438	405	0.08%	0.009%
79	11.758	3237	3240	3244	rBB	175	161	0.03%	0.004%
80	11.812	3245	3257	3273	rBV	272338	425794	80.09%	9.904%
81	11.938	3294	3296	3301	rBV	176	198	0.04%	0.005%
82	11.973	3304	3307	3312	rVB2	632	529	0.10%	0.012%
83	12.060	3326	3334	3346	rBV3	7368	12360	2.32%	0.287%
84	12.195	3363	3376	3391	rVV	247267	389985	73.36%	9.071%
85	12.250	3391	3393	3402	rVB	221	175	0.03%	0.004%
86	12.529	3472	3480	3491	rVB4	5367	6970	1.31%	0.162%
87	12.774	3546	3556	3566	rBV2	4265	6356	1.20%	0.148%
88	12.886	3587	3591	3600	rVB3	1055	1010	0.19%	0.023%
89	13.516	3780	3787	3794	rVB2	373	623	0.12%	0.014%
90	13.921	3908	3913	3914	rBV2	287	207	0.04%	0.005%
91	14.095	3963	3967	3970	rBV2	222	157	0.03%	0.004%
92	14.577	4108	4117	4126	rVB2	1011	1750	0.33%	0.041%
93	14.986	4241	4244	4248	rBV2	244	202	0.04%	0.005%
94	15.391	4367	4370	4373	rVB	261	146	0.03%	0.003%
95	15.446	4385	4387	4393	rVB2	193	165	0.03%	0.004%
96	15.474	4393	4396	4398	rBV2	267	186	0.03%	0.004%
97	15.552	4415	4420	4422	rBV2	213	213	0.04%	0.005%
98	15.587	4427	4431	4434	rBV	175	166	0.03%	0.004%
99	15.622	4439	4442	4444	rBV	178	134	0.03%	0.003%
100	15.783	4487	4492	4499	rBV2	302	438	0.08%	0.010%




Sum of corrected areas: 4299133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046472.D
Acq On : 17 Dec 2021 15:18
Operator : SY/MD
Sample : M5037-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

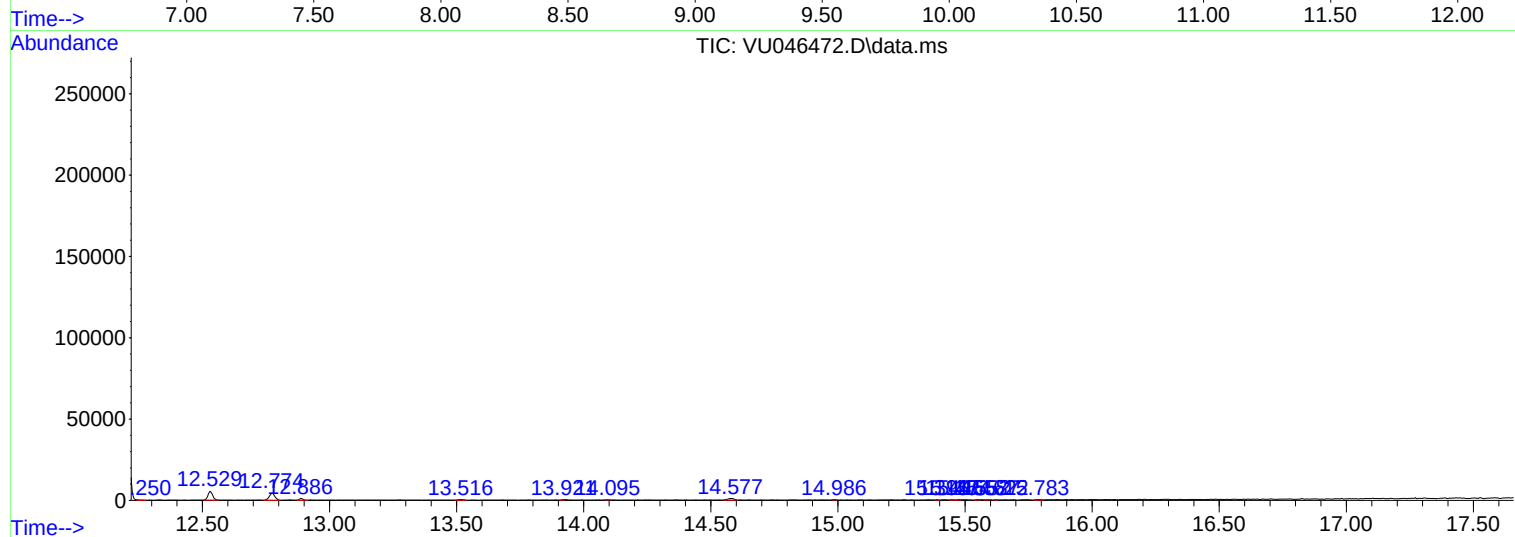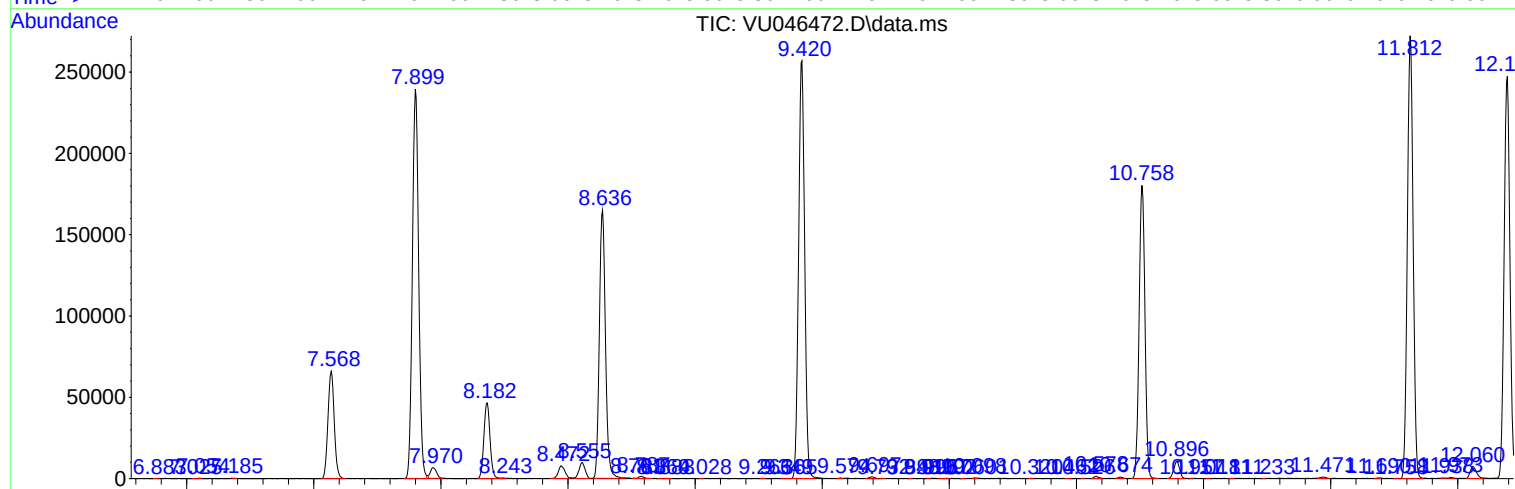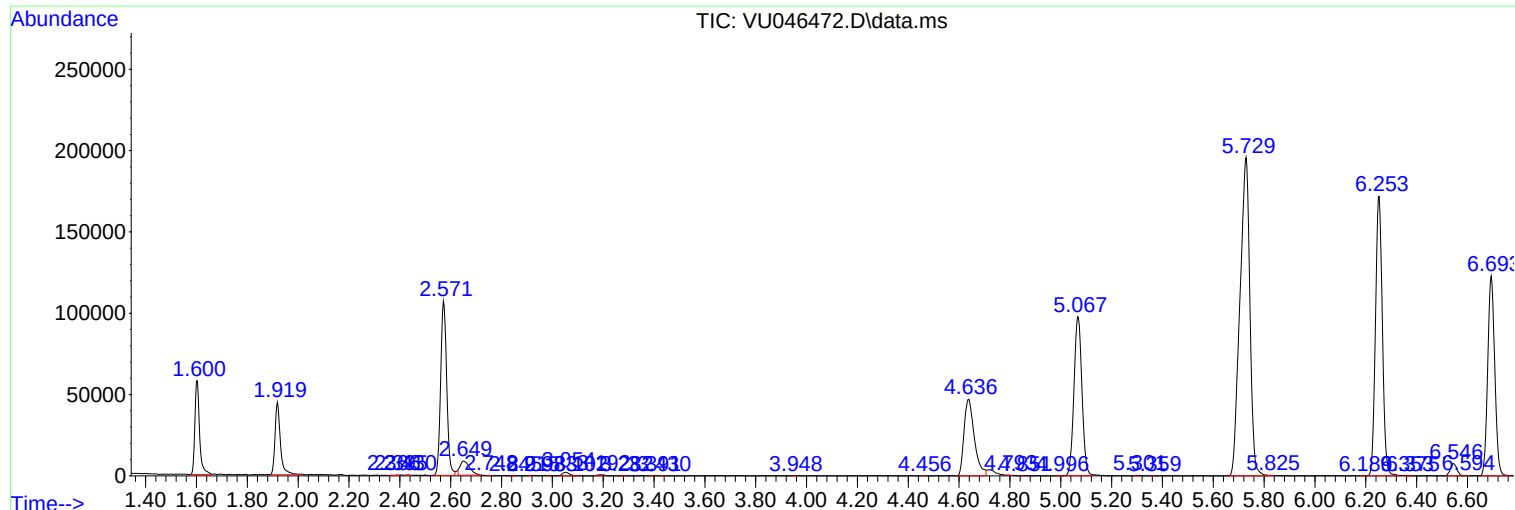

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046472.D
Acq On : 17 Dec 2021 15:18
Operator : SY/MD
Sample : M5037-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
Data File : VU046472.D
Acq On : 17 Dec 2021 15:18
Operator : SY/MD
Sample : M5037-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc