


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121721\
 Data File : VU046461.D
 Acq On : 17 Dec 2021 10:47
 Operator : SY/MD
 Sample : BFB034
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB034

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 20 00:25:10 2021

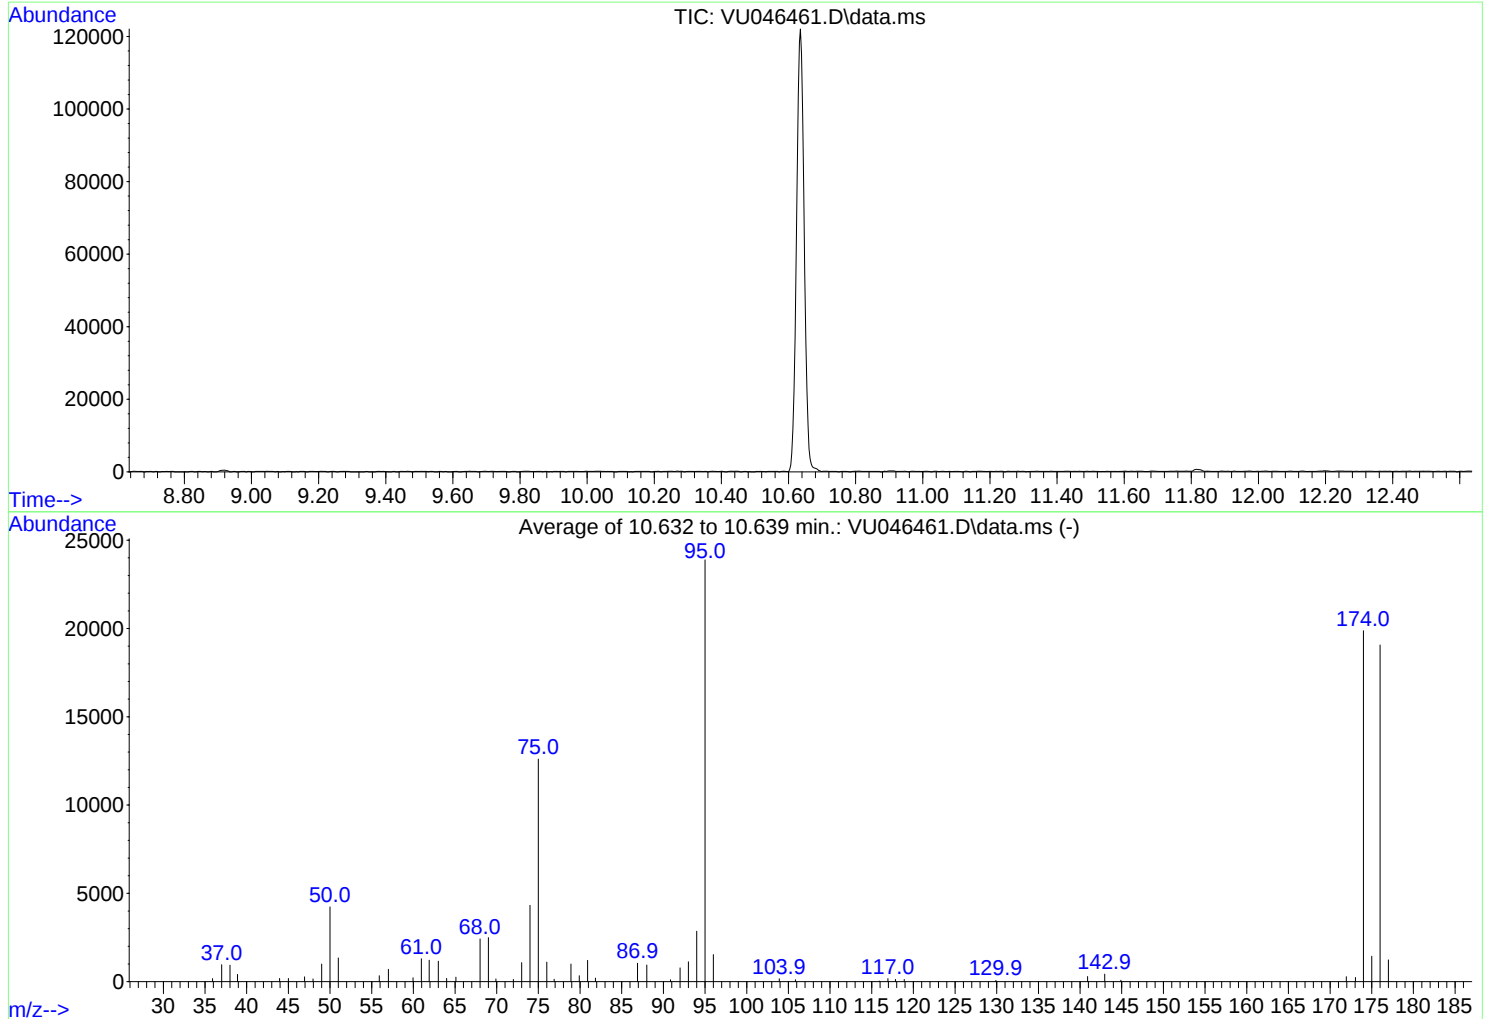

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	4232	PASS
75	95	30	80	52.8	12607	PASS
95	95	100	100	100.0	23888	PASS
96	95	5	9	6.4	1534	PASS
173	174	0.00	2	1.2	237	PASS
174	95	50	120	83.2	19872	PASS
175	174	5	9	7.2	1438	PASS
176	174	95	101	96.0	19069	PASS
177	176	5	9	6.5	1231	PASS

m/z	Abundance
44.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	148.0
37.00	960.0
38.00	979.0
38.90	383.0
43.90	319.0
45.00	216.0
47.00	308.0
47.90	158.0
49.00	1079.0
50.00	4278.0
51.00	1324.0
55.90	378.0
57.00	735.0
59.90	212.0
60.90	1252.0
61.90	1191.0
63.00	1276.0
64.00	207.0
65.10	248.0
68.00	2492.0
69.00	2530.0
69.90	168.0
72.00	126.0
73.00	1016.0
74.00	4335.0
75.00	12460.0
76.00	1155.0
76.90	149.0
78.90	1024.0
79.90	326.0
80.90	1194.0
81.90	203.0
86.90	1096.0
88.00	927.0
90.80	111.0
92.00	777.0
93.00	1132.0
94.00	2807.0
95.00	24248.0
96.00	1499.0
103.90	182.0
105.80	109.0
117.00	159.0
117.90	113.0
118.90	134.0
140.90	291.0
143.00	447.0
144.90	128.0
171.90	275.0
173.00	265.0
174.00	19264.0
175.00	1505.0
176.00	18840.0
177.00	1217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	175.0
37.00	962.0
38.00	983.0
38.90	438.0
44.00	296.0
45.00	184.0
47.00	291.0
48.00	166.0
49.00	1046.0
50.00	4399.0
51.00	1394.0
55.90	343.0
57.00	723.0
59.90	224.0
61.00	1310.0
61.90	1253.0
63.00	1201.0
64.00	188.0
65.10	265.0
68.00	2475.0
69.00	2526.0
69.90	154.0
72.00	140.0
73.00	1087.0
74.00	4456.0
75.00	13032.0
76.00	1128.0
76.90	138.0
78.90	1037.0
79.90	355.0
80.90	1272.0
81.80	205.0
86.90	1072.0
88.00	969.0
90.80	112.0
92.00	823.0
93.00	1114.0
94.00	2913.0
95.00	24552.0
96.00	1601.0
103.90	167.0
105.80	113.0
117.00	165.0
117.90	135.0
118.90	126.0
129.90	115.0
140.90	322.0
142.90	438.0
144.90	105.0
171.90	289.0
173.00	235.0
174.00	20416.0
175.00	1495.0
176.00	19632.0
177.00	1264.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	189.0
37.00	948.0
38.00	847.0
38.90	410.0
44.00	226.0
45.00	130.0
46.90	229.0
48.00	150.0
49.00	874.0
50.00	4018.0
51.00	1298.0
55.90	274.0
57.00	624.0
60.00	225.0
61.00	1322.0
61.90	1188.0
63.00	1012.0
64.00	161.0
65.10	250.0
68.00	2297.0
69.00	2408.0
69.90	138.0
72.00	110.0
73.00	1126.0
74.00	4177.0
75.00	12329.0
76.00	1028.0
76.90	108.0
78.90	933.0
79.90	331.0
80.90	1161.0
81.80	197.0
86.90	959.0
88.00	934.0
90.90	111.0
92.00	748.0
93.00	1115.0
94.00	2837.0
95.00	22864.0
96.00	1502.0
103.90	133.0
105.90	109.0
115.90	112.0
116.90	184.0
117.80	139.0
118.90	131.0
129.90	113.0
140.90	268.0
142.90	398.0
172.00	275.0
173.10	210.0
174.00	19936.0
175.00	1315.0
176.00	18736.0
177.00	1211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034