

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
 Data File : VU056971.D
 Acq On : 17 Dec 2023 16:27
 Operator : MD/SY
 Sample : 05842-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C19

Quant Time: Dec 18 01:18:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 18 01:16:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	263822	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	267891	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	101855	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	66483	2.940	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	58.800%
7) Chloroethane-d5	1.904	69	65443	3.867	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.400%
11) 1,1-Dichloroethene-d2	2.560	65	30614	3.164	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.200%
20) 2-Butanone-d5	4.615	46	217030	48.597	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.200%
24) Chloroform-d	5.055	84	175113	4.089	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%
26) 1,2-Dichloroethane-d4	5.695	65	86400	4.264	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.721	84	307788	3.704	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.000%
36) 1,2-Dichloropropane-d6	6.685	67	99084	3.810	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.200%
41) Toluene-d8	7.894	98	231931	3.123	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	62.400%#
43) trans-1,3-Dichloroprop...	8.177	79	32349	3.207	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	64.200%
46) 2-Hexanone-d5	8.627	63	165910	43.615	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.240%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	83386	4.431	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	85360	4.263	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.200%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.573	96	7796	0.364	ug/L #	1
25) Chloroform	5.078	83	34568	0.790	ug/L	96
38) Bromodichloromethane	7.107	83	5650	0.184	ug/L	98
47) Tetrachloroethene	8.547	164	209423	11.587	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
Data File : VU056971.D
Acq On : 17 Dec 2023 16:27
Operator : MD/SY
Sample : 05842-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C19

Quant Time: Dec 18 01:18:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 18 01:16:15 2023
Response via : Initial Calibration

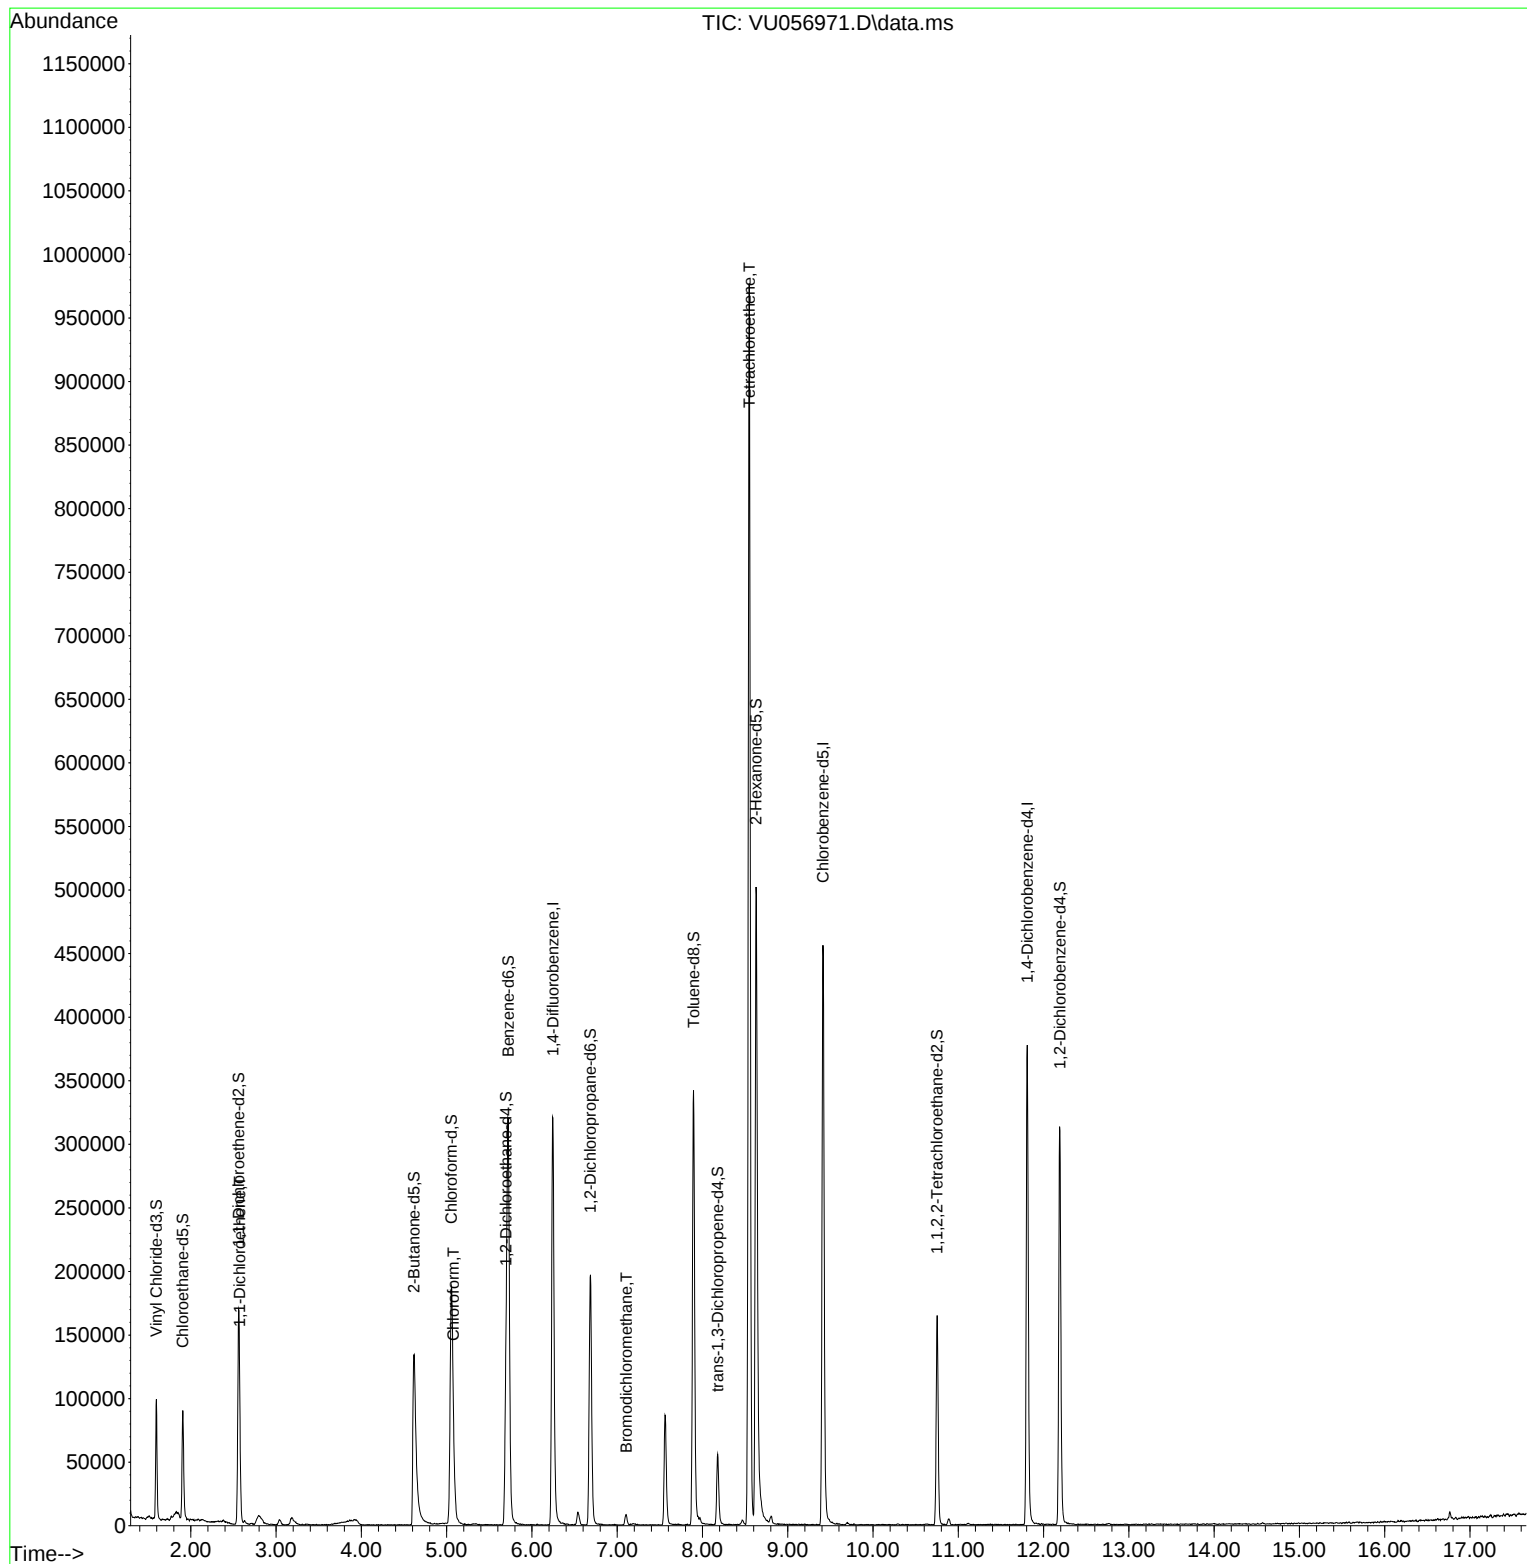

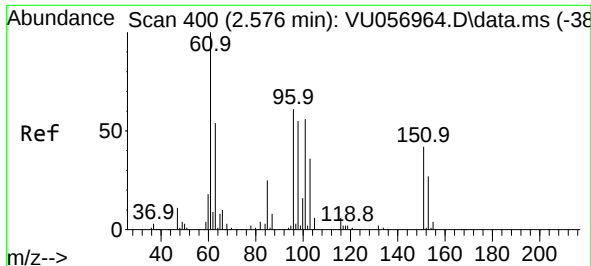

#12

1,1-Dichloroethene

Concen: 0.364 ug/L

RT: 2.573 min Scan# 399

Delta R.T. -0.003 min

Lab File: VU056971.D

Acq: 17 Dec 2023 16:27

Instrument :

MSVOA_U

ClientSampleId :

F7C19





Tgt Ion: 96 Resp: 7796

Ion Ratio Lower Upper

96 100

61 229.5 119.0 221.0#

63 719.5 88.7 164.7#

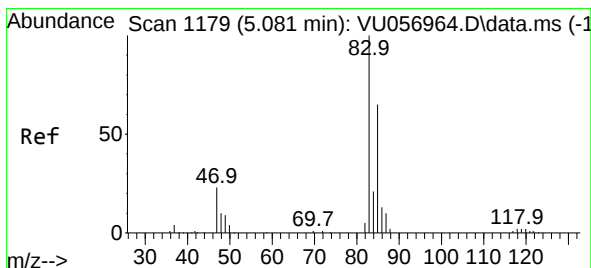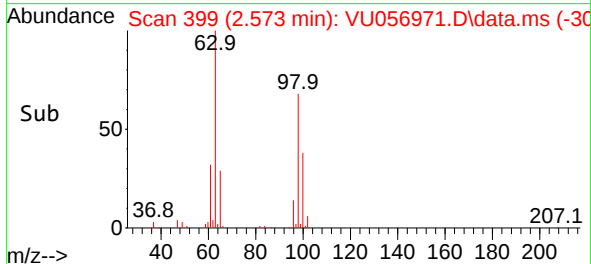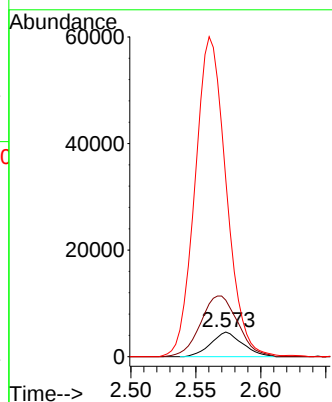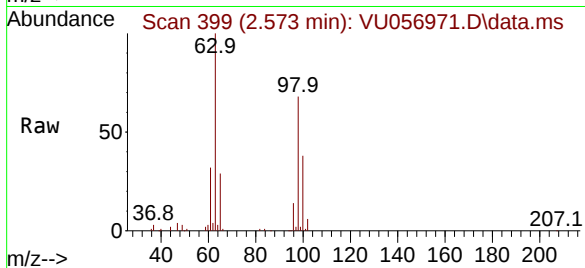

#25

Chloroform

Concen: 0.790 ug/L

RT: 5.078 min Scan# 1178

Delta R.T. -0.003 min

Lab File: VU056971.D




Acq: 17 Dec 2023 16:27


Tgt Ion: 83 Resp: 34568

Ion Ratio Lower Upper

83 100

85 68.2 45.8 85.0


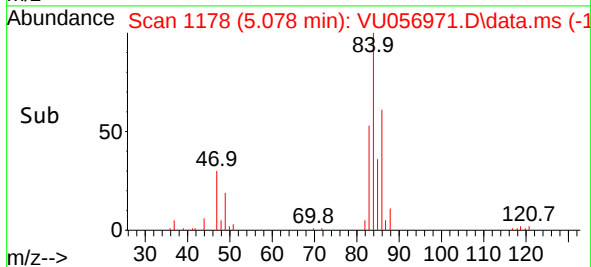
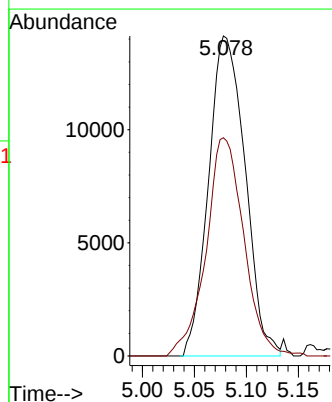
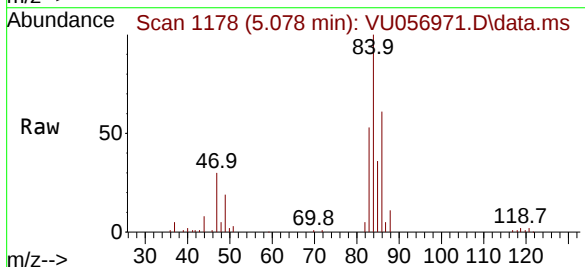


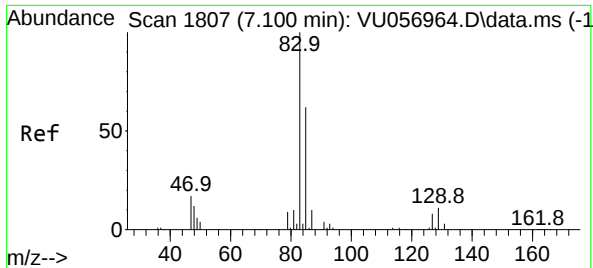

#38
Bromodichloromethane
Concen: 0.184 ug/L
RT: 7.107 min Scan# 11
Delta R.T. 0.007 min
Lab File: VU056971.D
Acq: 17 Dec 2023 16:27

Instrument :
MSVOA_U
ClientSampleId :
F7C19

Tgt Ion: 83 Resp: 5650
Ion Ratio Lower Upper
83 100
85 62.6 45.0 83.6
127 7.2 7.0 10.4

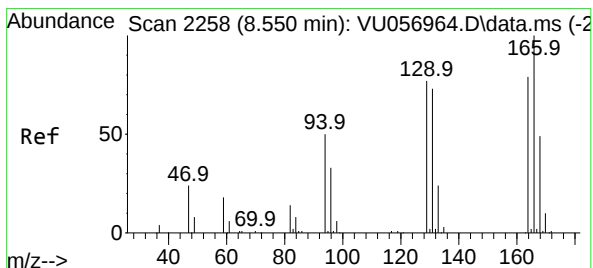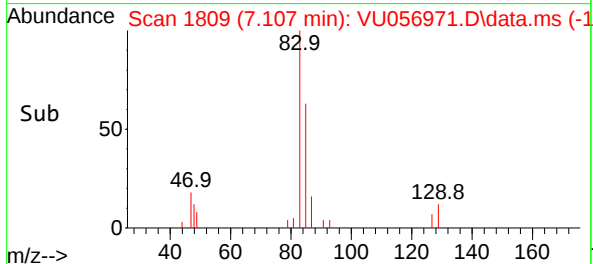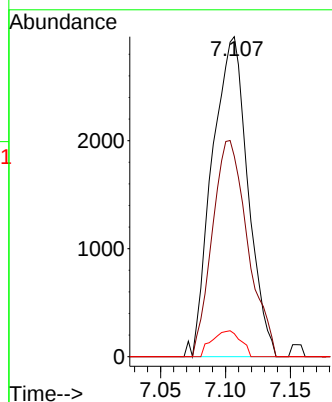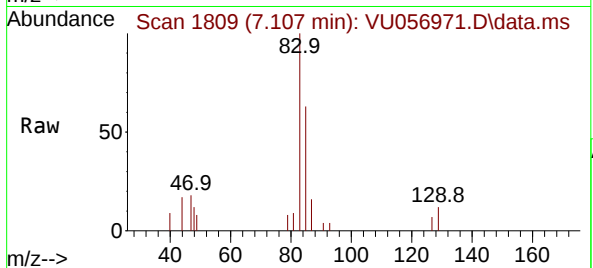

#47
Tetrachloroethene
Concen: 11.587 ug/L
RT: 8.547 min Scan# 2257
Delta R.T. -0.003 min
Lab File: VU056971.D
Acq: 17 Dec 2023 16:27

Tgt Ion: 164 Resp: 209423
Ion Ratio Lower Upper
164 100
129 105.6 73.4 136.4
131 101.9 71.5 132.9
166 127.5 92.7 172.1

