

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
 Data File : VU056975.D
 Acq On : 17 Dec 2023 18:04
 Operator : MD/SY
 Sample : 05842-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C23

Quant Time: Dec 18 01:19:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Dec 18 01:16:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	254156	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	250273	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	105311	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	64522	2.962	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	59.200%
7) Chloroethane-d5	1.907	69	63560	3.899	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.000%
11) 1,1-Dichloroethene-d2	2.560	65	29482	3.163	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.200%
20) 2-Butanone-d5	4.618	46	209049	48.590	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.180%
24) Chloroform-d	5.055	84	165865	4.021	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.400%
26) 1,2-Dichloroethane-d4	5.695	65	85420	4.376	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
32) Benzene-d6	5.721	84	301012	3.878	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.600%
36) 1,2-Dichloropropane-d6	6.685	67	103258	4.250	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.000%
41) Toluene-d8	7.894	98	212267	3.059	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	61.200%#
43) trans-1,3-Dichloroprop...	8.177	79	30670	3.255	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	65.000%
46) 2-Hexanone-d5	8.627	63	148466	41.777	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.560%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	81040	4.610	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	86223	4.165	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.400%
Target Compounds					Qvalue	
13) Acetone	2.624	43	68471	26.115	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
Data File : VU056975.D
Acq On : 17 Dec 2023 18:04
Operator : MD/SY
Sample : 05842-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C23

Quant Time: Dec 18 01:19:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Dec 18 01:16:15 2023
Response via : Initial Calibration

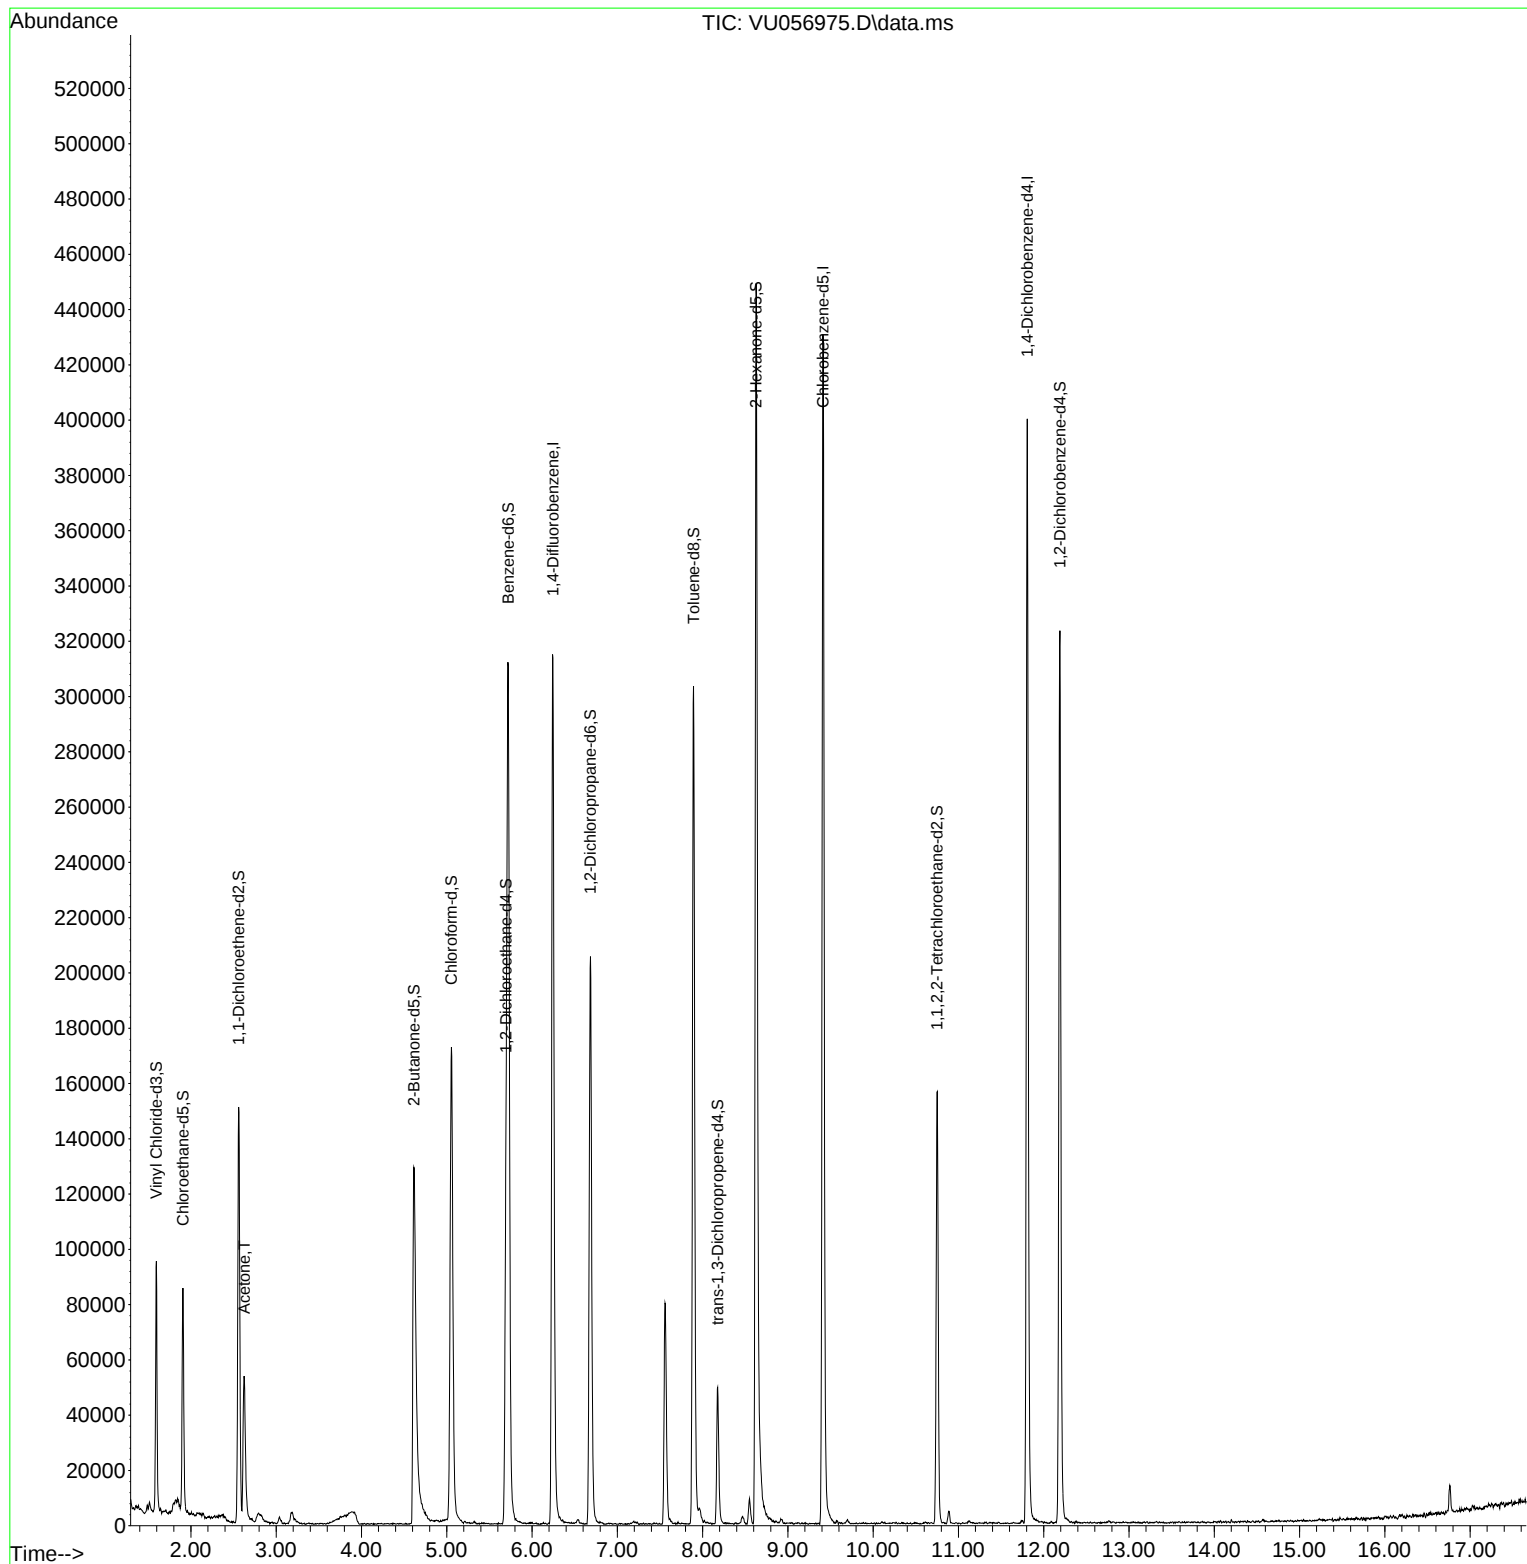

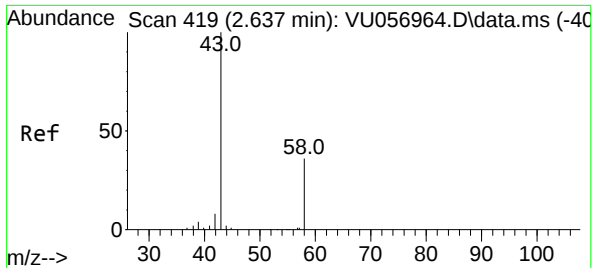

#13
 Acetone
 Concen: 26.115 ug/L
 RT: 2.624 min Scan# 41
 Delta R.T. -0.013 min
 Lab File: VU056975.D
 Acq: 17 Dec 2023 18:04

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C23

Tgt Ion: 43 Resp: 68471
 Ion Ratio Lower Upper
 43 100
 58 34.3 0.0 72.6

