

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
 Data File : VU056976.D
 Acq On : 17 Dec 2023 18:29
 Operator : MD/SY
 Sample : 05842-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C24

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	111	rVB	90736	107656	12.68%	1.410%
2	1.808	148	161	164	rBV10	4887	9157	1.08%	0.120%
3	1.904	183	191	208	rVB	79689	112620	13.26%	1.475%
4	2.560	383	395	410	rBV2	157174	267676	31.53%	3.506%
5	2.788	454	466	472	rBV3	4493	10021	1.18%	0.131%
6	3.181	575	588	602	rBV3	8338	21434	2.52%	0.281%
7	4.615	1024	1034	1072	rBV	133746	352565	41.53%	4.618%
8	5.058	1156	1172	1209	rVB2	177704	466577	54.96%	6.111%
9	5.721	1358	1378	1398	rBV2	303723	807266	95.08%	10.573%
10	6.242	1527	1540	1574	rBV	325838	638948	75.26%	8.369%
11	6.685	1665	1678	1703	rBV	206223	409397	48.22%	5.362%
12	7.100	1797	1807	1817	rBV2	5019	8756	1.03%	0.115%
13	7.563	1936	1951	1974	rBV	85605	157386	18.54%	2.061%
14	7.894	2038	2054	2075	rBV	325460	578934	68.19%	7.583%
15	8.177	2132	2142	2155	rBV2	52066	90224	10.63%	1.182%
16	8.550	2245	2258	2272	rBV	313566	534514	62.96%	7.001%
17	8.627	2272	2282	2319	rVV	445189	849013	100.00%	11.120%
18	9.412	2509	2526	2544	rBV	423556	735413	86.62%	9.632%
19	10.749	2927	2942	2958	rBV2	150559	248899	29.32%	3.260%
20	11.807	3259	3271	3290	rBV	406757	676324	79.66%	8.858%
21	12.187	3377	3389	3416	rBV	322239	552288	65.05%	7.234%




Sum of corrected areas: 7635068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
Data File : VU056976.D
Acq On : 17 Dec 2023 18:29
Operator : MD/SY
Sample : 05842-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

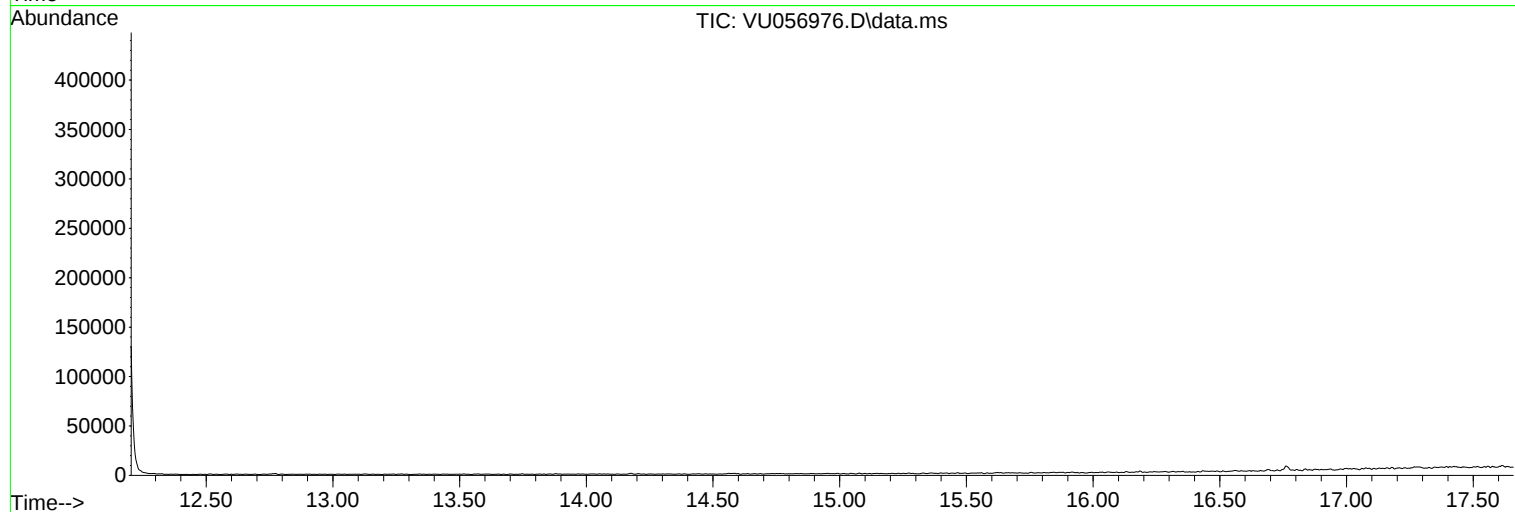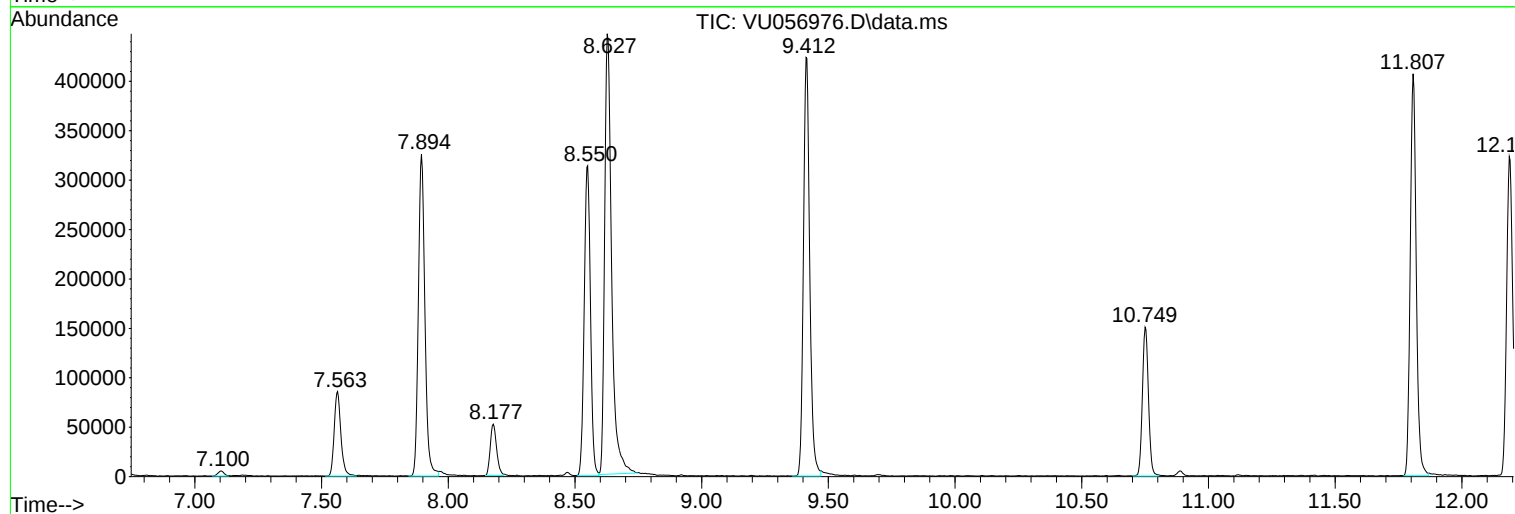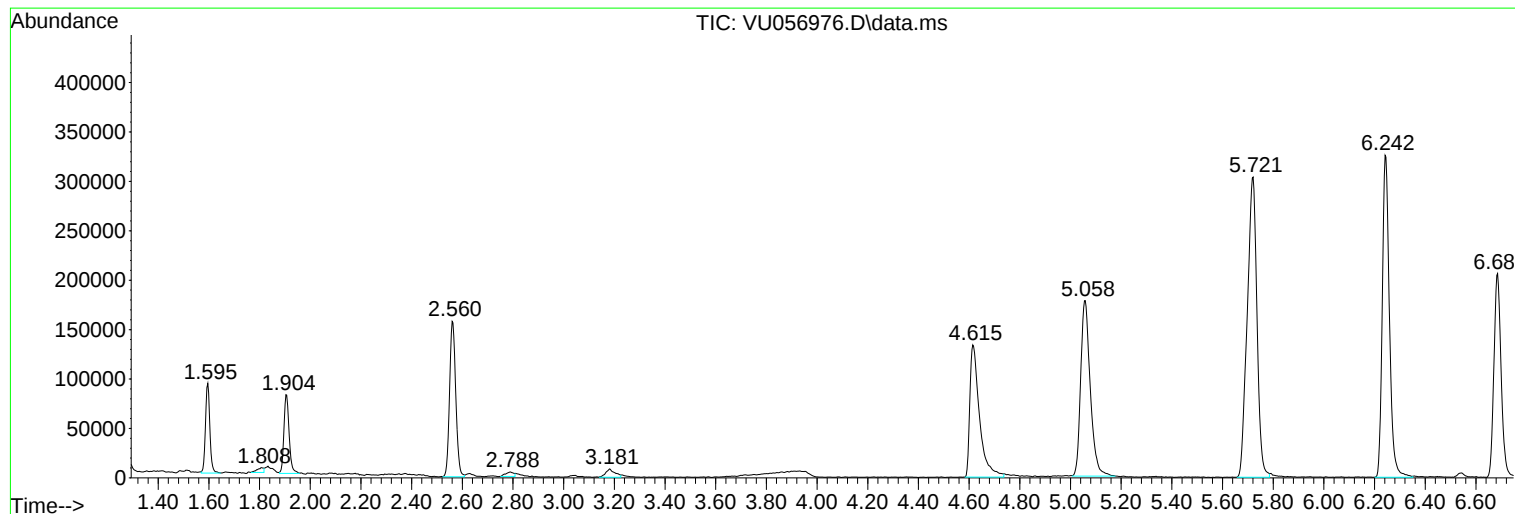

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
Data File : VU056976.D
Acq On : 17 Dec 2023 18:29
Operator : MD/SY
Sample : 05842-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
Data File : VU056976.D
Acq On : 17 Dec 2023 18:29
Operator : MD/SY
Sample : 05842-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc