


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121723\
Data File : VU056963.D
Acq On : 17 Dec 2023 09:55
Operator : MD/SY
Sample : BFB095
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB095

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 19 02:36:03 2023

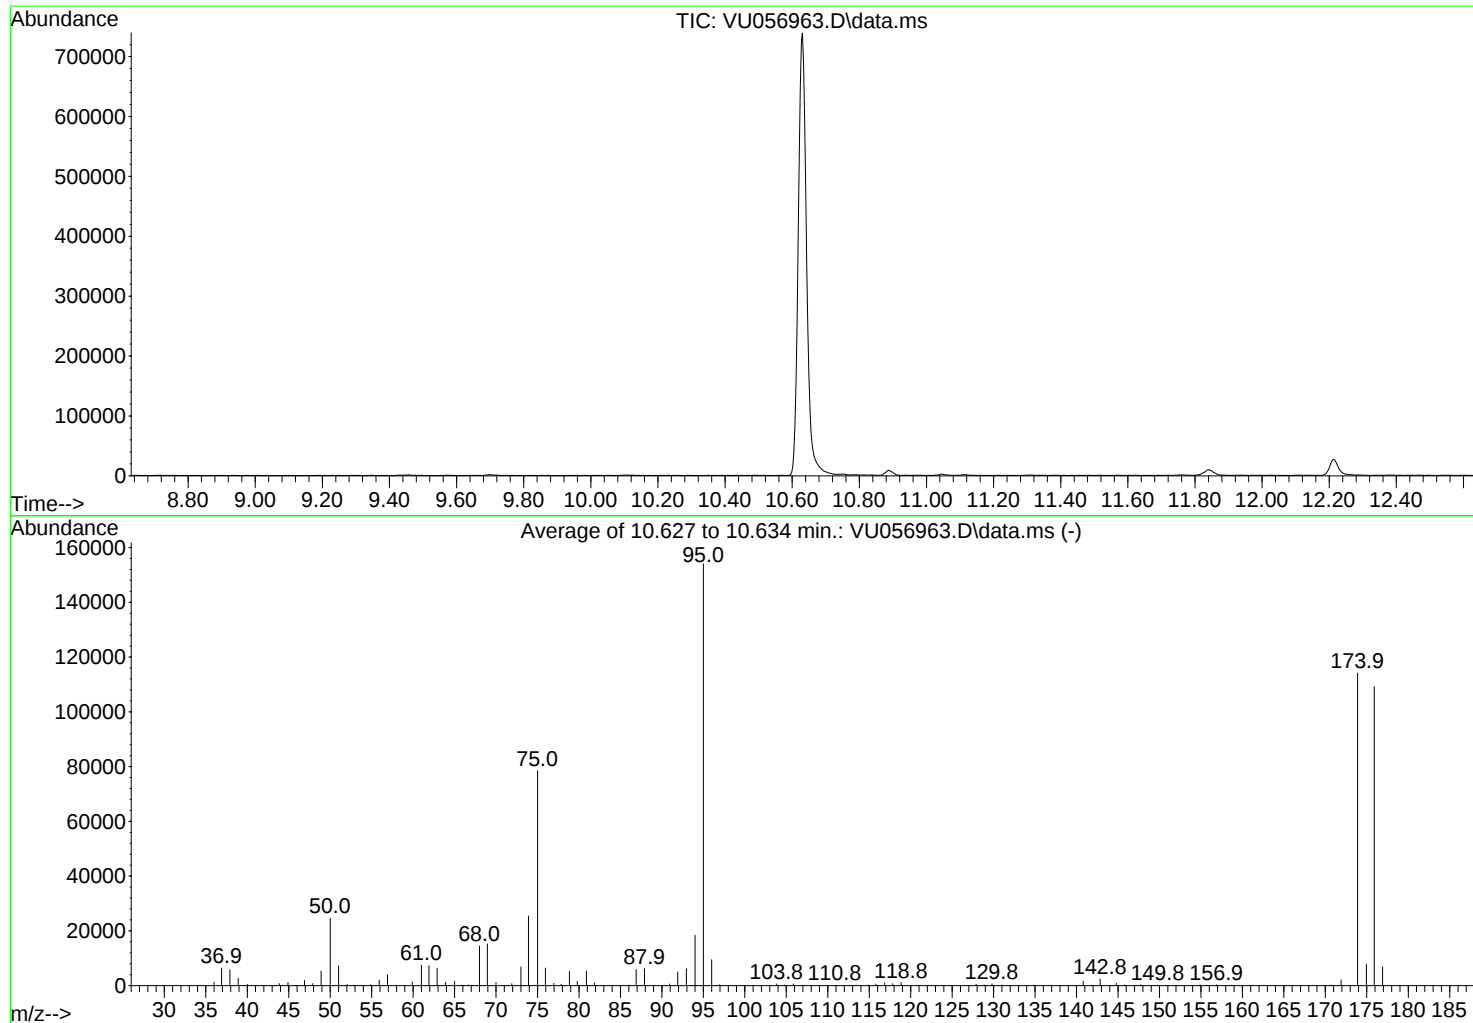

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	24587	PASS
75	95	30	80	51.0	78509	PASS
95	95	100	100	100.0	154048	PASS
96	95	5	9	6.2	9497	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.1	114131	PASS
175	174	5	9	6.8	7770	PASS
176	174	95	101	95.8	109285	PASS
177	176	5	9	6.3	6920	PASS

m/z	Abundance
39.70	274.0
43.80	412.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
36.00	1180.0
36.90	6567.0
37.90	6385.0
38.90	2842.0
40.00	456.0
40.90	160.0
43.10	144.0
43.90	1230.0
44.90	1124.0
45.80	171.0
46.90	1730.0
47.90	830.0
48.90	5287.0
50.00	25048.0
51.00	7231.0
52.00	465.0
52.80	212.0
53.80	155.0
54.90	496.0
55.90	2055.0
56.90	4131.0
57.90	242.0
59.90	1154.0
61.00	7508.0
61.90	7781.0
62.90	6615.0
63.90	1221.0
65.00	1430.0
65.80	148.0
66.70	317.0
67.10	222.0
68.00	14877.0
68.90	15164.0
70.00	1226.0
70.90	106.0
71.90	765.0
73.00	7236.0
73.90	25920.0
75.00	79072.0
76.00	6766.0
76.90	904.0
77.80	564.0
78.90	5318.0
79.80	1780.0
80.90	5375.0
81.80	1130.0
82.70	147.0
86.00	213.0
86.90	6007.0
87.90	6394.0
90.90	522.0
91.90	4847.0
93.00	5999.0
94.00	18736.0
95.00	156800.0
96.00	10116.0
96.90	354.0
103.80	659.0
104.80	244.0
105.80	662.0
106.70	178.0
110.90	133.0
112.00	113.0
112.60	103.0
115.00	294.0
115.80	631.0
116.90	1097.0
117.80	745.0
118.90	1190.0
127.90	417.0
128.90	265.0
129.80	688.0
131.00	197.0
134.90	245.0
136.90	273.0
139.80	156.0
140.80	1676.0
141.80	112.0
142.90	2566.0
144.80	1028.0
145.80	230.0
147.70	322.0
149.80	178.0
154.90	258.0
155.70	132.0
156.90	364.0
158.70	170.0
160.90	177.0
170.70	369.0
171.90	2067.0
173.90	112816.0
174.90	7464.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

175.90109040.0

176.907137.0

177.80222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
36.00	1273.0
36.90	6690.0
37.90	5834.0
38.90	2746.0
40.00	459.0
40.90	148.0
43.00	124.0
43.90	1237.0
44.90	1228.0
45.80	154.0
46.90	1919.0
47.90	785.0
48.90	5518.0
50.00	25200.0
51.00	7353.0
52.00	487.0
52.90	249.0
53.80	191.0
54.90	420.0
55.90	2110.0
56.90	4199.0
58.00	253.0
59.90	1373.0
61.00	7785.0
61.90	7516.0
62.90	6577.0
63.90	1286.0
65.00	1633.0
65.90	157.0
66.70	308.0
68.00	15029.0
69.00	15836.0
70.00	1131.0
71.00	111.0
71.80	667.0
73.00	7048.0
73.90	26192.0
75.00	80608.0
75.90	6577.0
76.90	849.0
77.90	483.0
78.80	5350.0
79.80	1637.0
80.90	5459.0
81.90	1071.0
82.70	121.0
86.00	212.0
86.90	6158.0
87.90	6379.0
90.90	568.0
91.90	5156.0
92.90	6285.0
94.00	19000.0
95.00	158080.0
96.00	9745.0
96.90	376.0
103.90	617.0
104.80	272.0
105.90	616.0
106.90	205.0
109.70	103.0
110.90	146.0
112.00	104.0
112.70	157.0
115.00	326.0
115.80	579.0
116.80	991.0
117.80	766.0
118.90	1198.0
127.90	488.0
128.80	232.0
129.80	674.0
131.00	228.0
134.80	272.0
136.60	178.0
137.00	259.0
139.70	128.0
140.80	1710.0
141.90	124.0
142.80	2529.0
144.80	949.0
145.80	244.0
146.80	106.0
147.80	356.0
149.80	194.0
154.90	280.0
155.70	190.0
156.90	320.0
157.90	112.0
158.70	182.0
160.80	146.0
170.70	283.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

171.90	2202.0
173.90	117712.0
175.00	7967.0
175.90	112536.0
176.90	7119.0
177.90	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
36.00	1250.0
36.90	6125.0
37.90	5083.0
38.90	2418.0
40.00	514.0
40.90	100.0
43.90	1086.0
44.90	1135.0
46.20	163.0
46.90	1894.0
47.90	728.0
48.90	5222.0
50.00	23512.0
51.00	6901.0
52.10	483.0
52.90	273.0
53.90	190.0
54.90	323.0
55.90	2009.0
56.90	3807.0
58.00	191.0
59.90	1438.0
61.00	7024.0
61.90	6674.0
62.90	5865.0
63.90	1206.0
65.00	1708.0
66.10	154.0
67.00	255.0
68.00	13672.0
69.00	14711.0
70.00	979.0
72.00	647.0
73.00	6169.0
73.90	24080.0
75.00	75848.0
75.90	5967.0
77.00	789.0
77.90	481.0
78.80	4971.0
79.80	1255.0
80.90	5139.0
81.90	1056.0
82.80	103.0
86.00	233.0
86.90	5618.0
87.90	5769.0
90.90	603.0
91.90	5063.0
92.90	6374.0
94.00	17656.0
95.00	147264.0
96.00	8630.0
96.90	310.0
103.90	602.0
104.80	261.0
105.90	573.0
107.00	254.0
109.70	173.0
110.70	146.0
112.00	116.0
112.90	228.0
114.90	251.0
115.80	516.0
116.80	907.0
117.90	621.0
118.80	1027.0
127.90	563.0
128.80	178.0
129.80	637.0
131.00	203.0
134.80	272.0
136.50	132.0
137.00	212.0
139.70	137.0
140.80	1473.0
141.90	131.0
142.90	2296.0
144.80	740.0
145.80	230.0
147.70	373.0
149.80	155.0
153.90	113.0
154.90	345.0
155.70	173.0
156.90	263.0
157.90	120.0
158.70	159.0
160.80	107.0
170.90	205.0
171.90	2090.0
173.90	111864.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

175.00	7880.0
175.90	106280.0
176.90	6505.0
178.00	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095