

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121724\
 Data File : VU062410.D
 Acq On : 18 Dec 2024 01:28
 Operator : MD/SY
 Sample : P5309-04
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF3

Quant Time: Dec 18 06:34:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 18 01:12:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	94666	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	89763	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	43459	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	24565	3.847	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.000%
7) Chloroethane-d5	1.907	69	20957	4.614	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	2.560	65	12646	4.163	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.200%
20) 2-Butanone-d5	4.627	46	60092	49.105	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.220%
24) Chloroform-d	5.052	84	63013	4.560	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	5.695	65	34863	5.130	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
32) Benzene-d6	5.717	84	110680	4.281	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.682	67	32564	4.402	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.000%
41) Toluene-d8	7.891	98	103360	4.232	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.600%
43) trans-1,3-Dichloroprop...	8.177	79	13868	4.259	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.627	63	46347	47.182	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.360%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	28196	4.899	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.000%
66) 1,2-Dichlorobenzene-d4	12.183	152	41192	5.144	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%
Target Compounds						
13) Acetone	2.650	43	4138	4.966	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121724\
Data File : VU062410.D
Acq On : 18 Dec 2024 01:28
Operator : MD/SY
Sample : P5309-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF3

Quant Time: Dec 18 06:34:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 18 01:12:26 2024
Response via : Initial Calibration

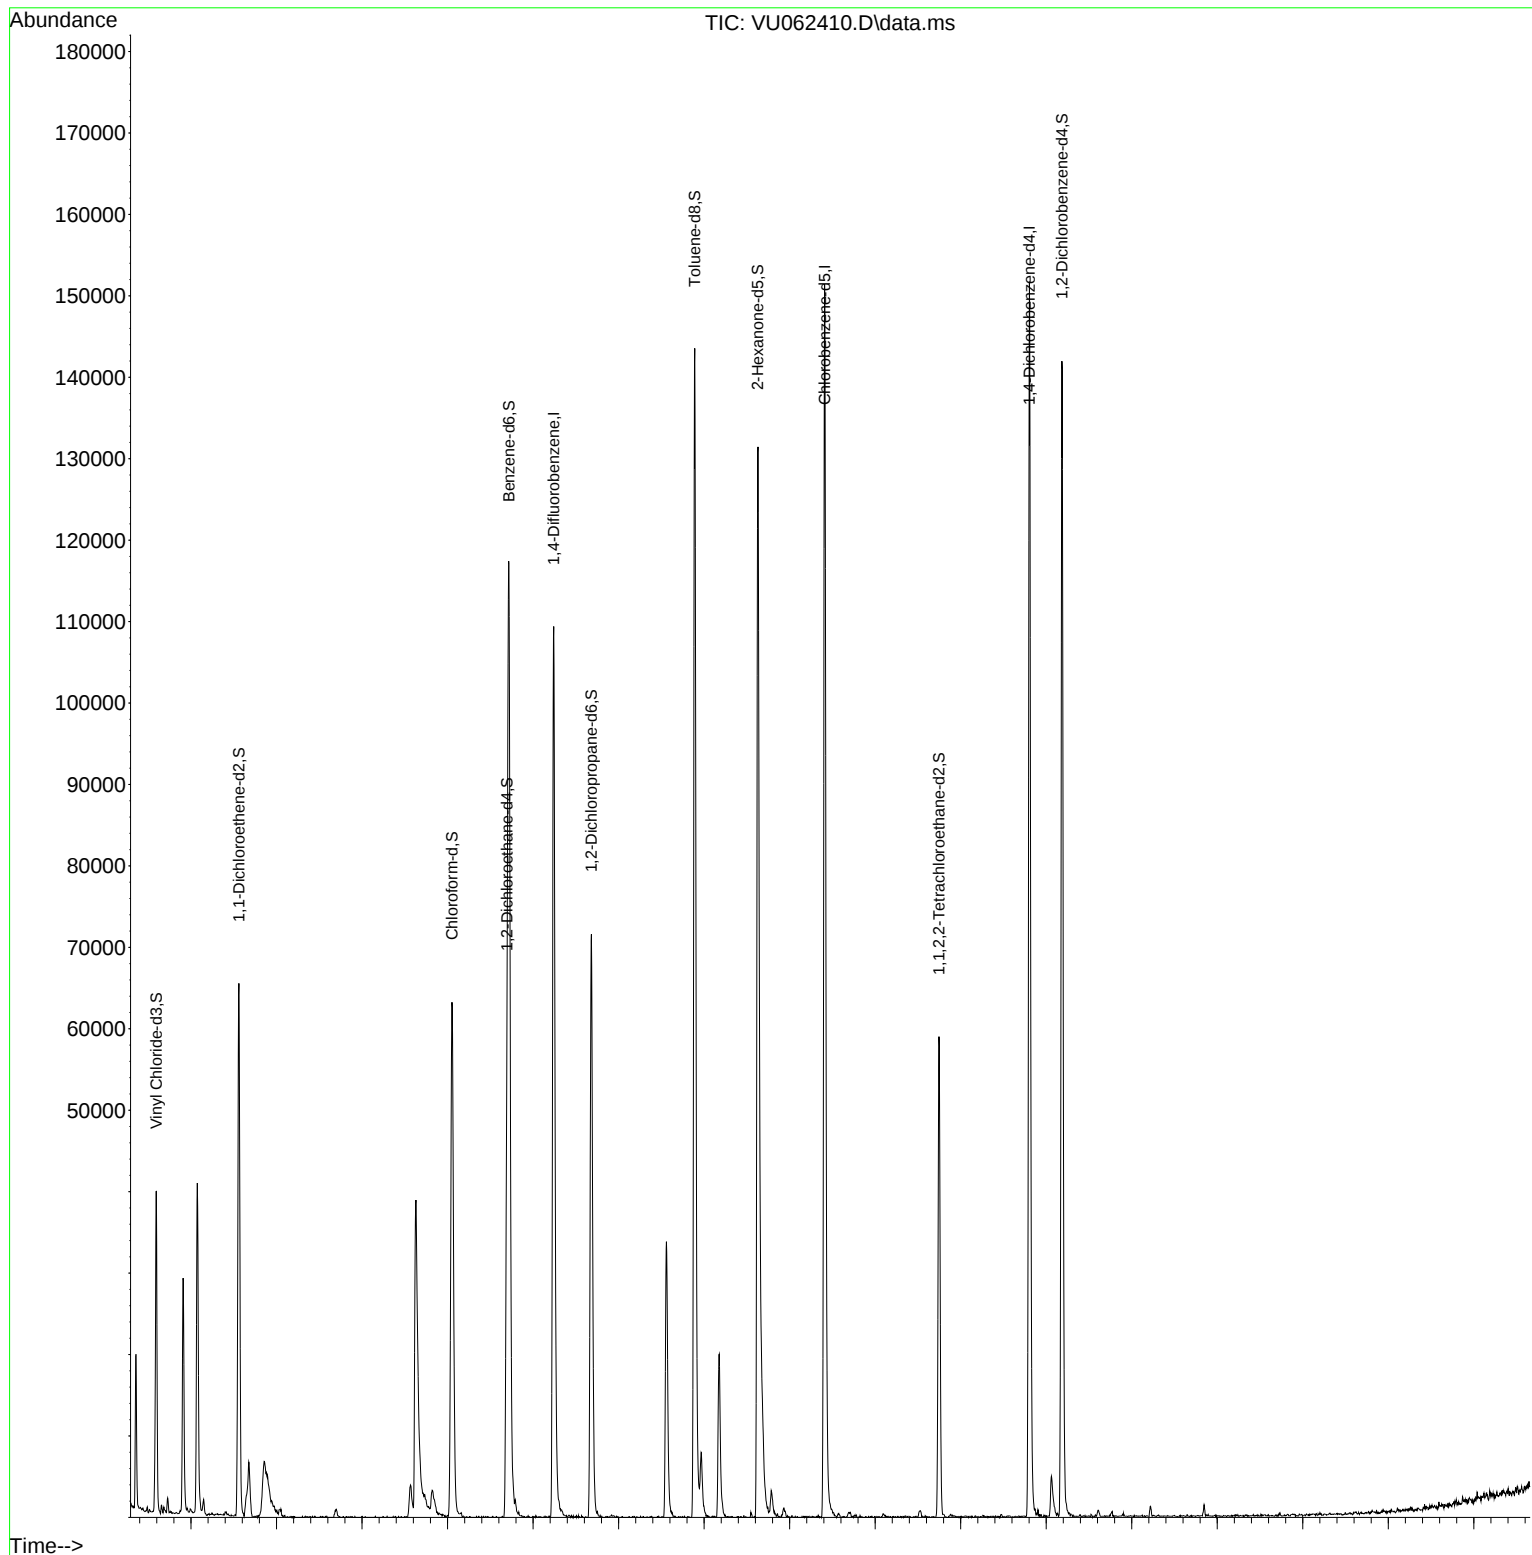

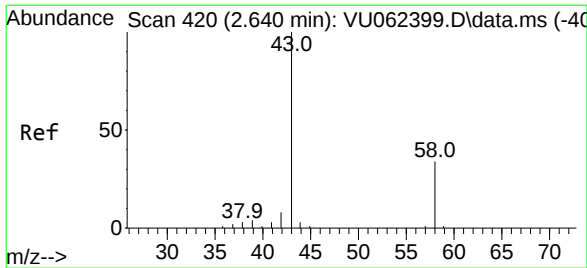

#13
 Acetone
 Concen: 4.966 ug/L
 RT: 2.650 min Scan# 42
 Delta R.T. 0.010 min
 Lab File: VU062410.D
 Acq: 18 Dec 2024 01:28

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF3

Tgt Ion: 43 Resp: 4138
 Ion Ratio Lower Upper
 43 100
 58 32.3 0.0 64.0

