

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121724\
 Data File : VU062413.D
 Acq On : 18 Dec 2024 02:42
 Operator : MD/SY
 Sample : P5309-08
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CG3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	85	94	108	rVB	43447	55173	2.65%	1.102%
2	1.907	184	192	208	rBV	32022	43214	2.07%	0.863%
3	2.074	235	244	258	rBV	40266	56052	2.69%	1.119%
4	2.560	384	395	414	rVB	71586	116527	5.59%	2.326%
5	2.862	470	489	501	rBV6	6065	21559	1.03%	0.430%
6	4.631	1030	1039	1077	rBV	41994	122729	5.89%	2.450%
7	5.052	1155	1170	1196	rBV	67362	152341	7.31%	3.041%
8	5.714	1358	1376	1405	rBV2	125951	337996	16.22%	6.748%
9	6.242	1528	1540	1562	rBV	119574	232047	11.13%	4.633%
10	6.531	1615	1630	1666	rBV	1089492	2083945	100.00%	41.605%
11	6.679	1666	1676	1700	rVB	78710	159056	7.63%	3.175%
12	7.560	1938	1950	1973	rBV2	37877	68660	3.29%	1.371%
13	7.891	2040	2053	2069	rBV	160291	284288	13.64%	5.676%
14	8.174	2130	2141	2160	rBV2	22304	40096	1.92%	0.801%
15	8.627	2272	2282	2320	rBV3	146218	321749	15.44%	6.424%
16	9.409	2513	2525	2552	rBV	162589	286881	13.77%	5.727%
17	10.746	2930	2941	2959	rVB	63426	103176	4.95%	2.060%
18	11.804	3258	3270	3291	rBV	161783	266443	12.79%	5.319%
19	12.183	3373	3388	3411	rBV	150927	256921	12.33%	5.129%




Sum of corrected areas: 5008853

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121724\
Data File : VU062413.D
Acq On : 18 Dec 2024 02:42
Operator : MD/SY
Sample : P5309-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

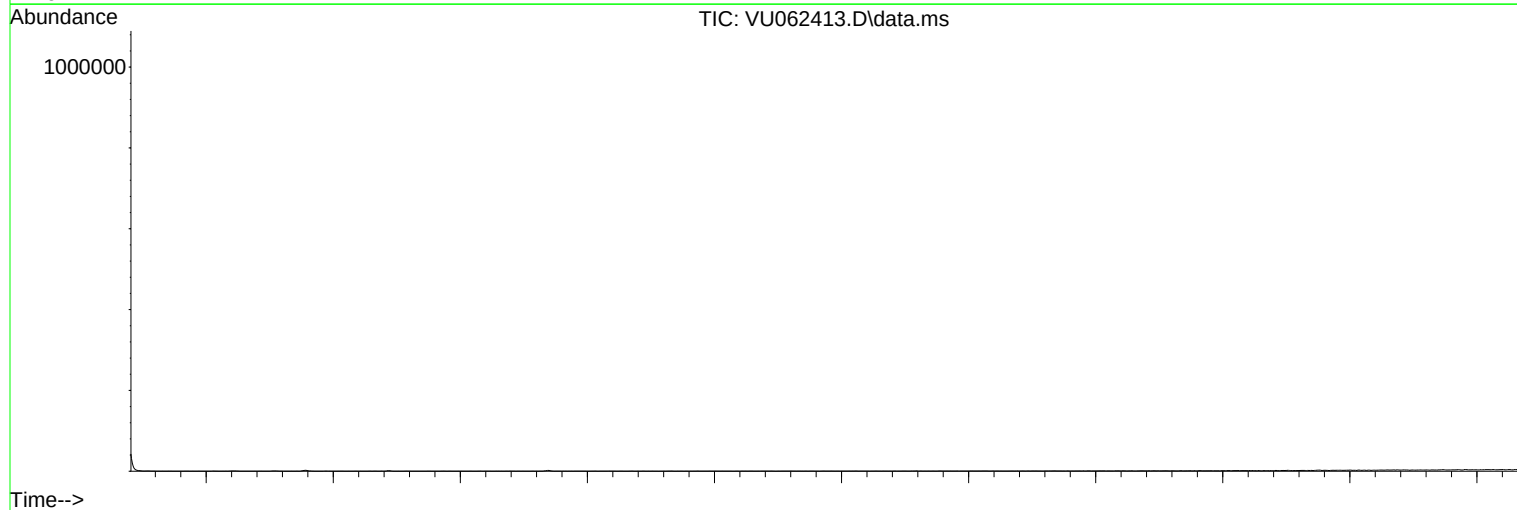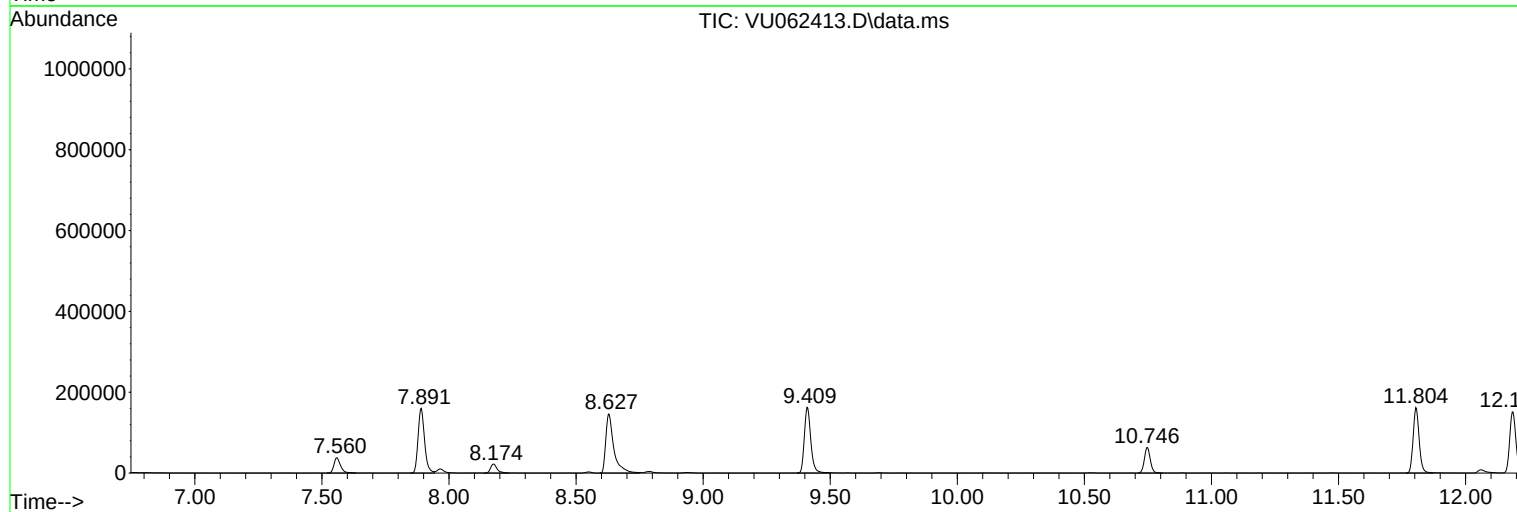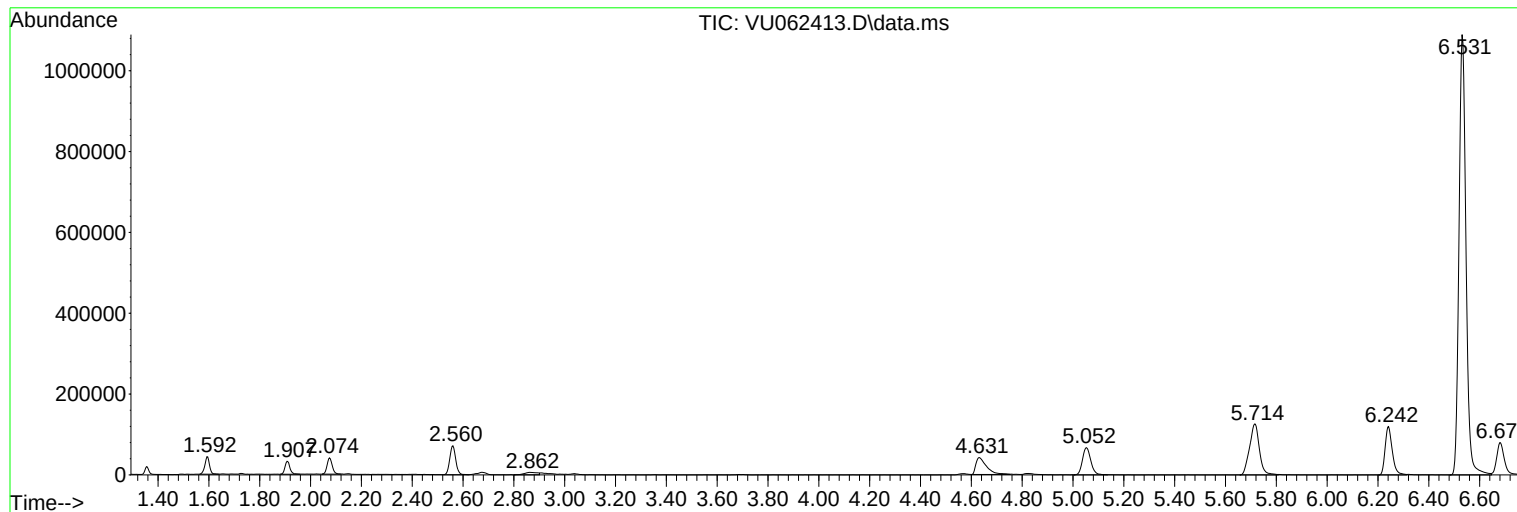

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121724\
Data File : VU062413.D
Acq On : 18 Dec 2024 02:42
Operator : MD/SY
Sample : P5309-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.074	1.21 ug/L	56052	1,4-Difluorobenzene	6.242

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3	Fluorodichloromethane	102	CHCl2F	000075-43-4	90
4	Cyclopentene, 1-chloro-	102	C5H7Cl	000930-29-0	5
5	Chlorine dioxide	67	ClO2	010049-04-4	5

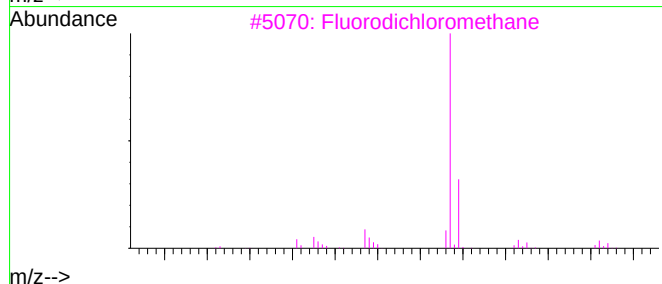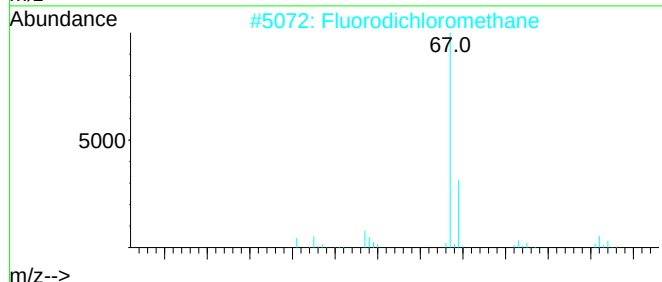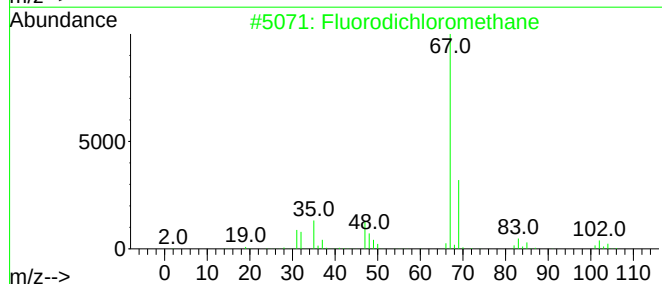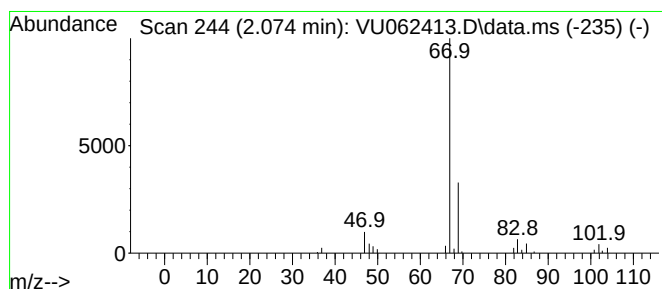

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121724\
Data File : VU062413.D
Acq On : 18 Dec 2024 02:42
Operator : MD/SY
Sample : P5309-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
Fluorodichlorom...	2.074	1.2	ug/L	56052	1	6.242	232047	5.0