


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121724\
Data File : VU062374.D
Acq On : 17 Dec 2024 08:13
Operator : MD/SY
Sample : BFB048
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB048

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 18 01:12:26 2024

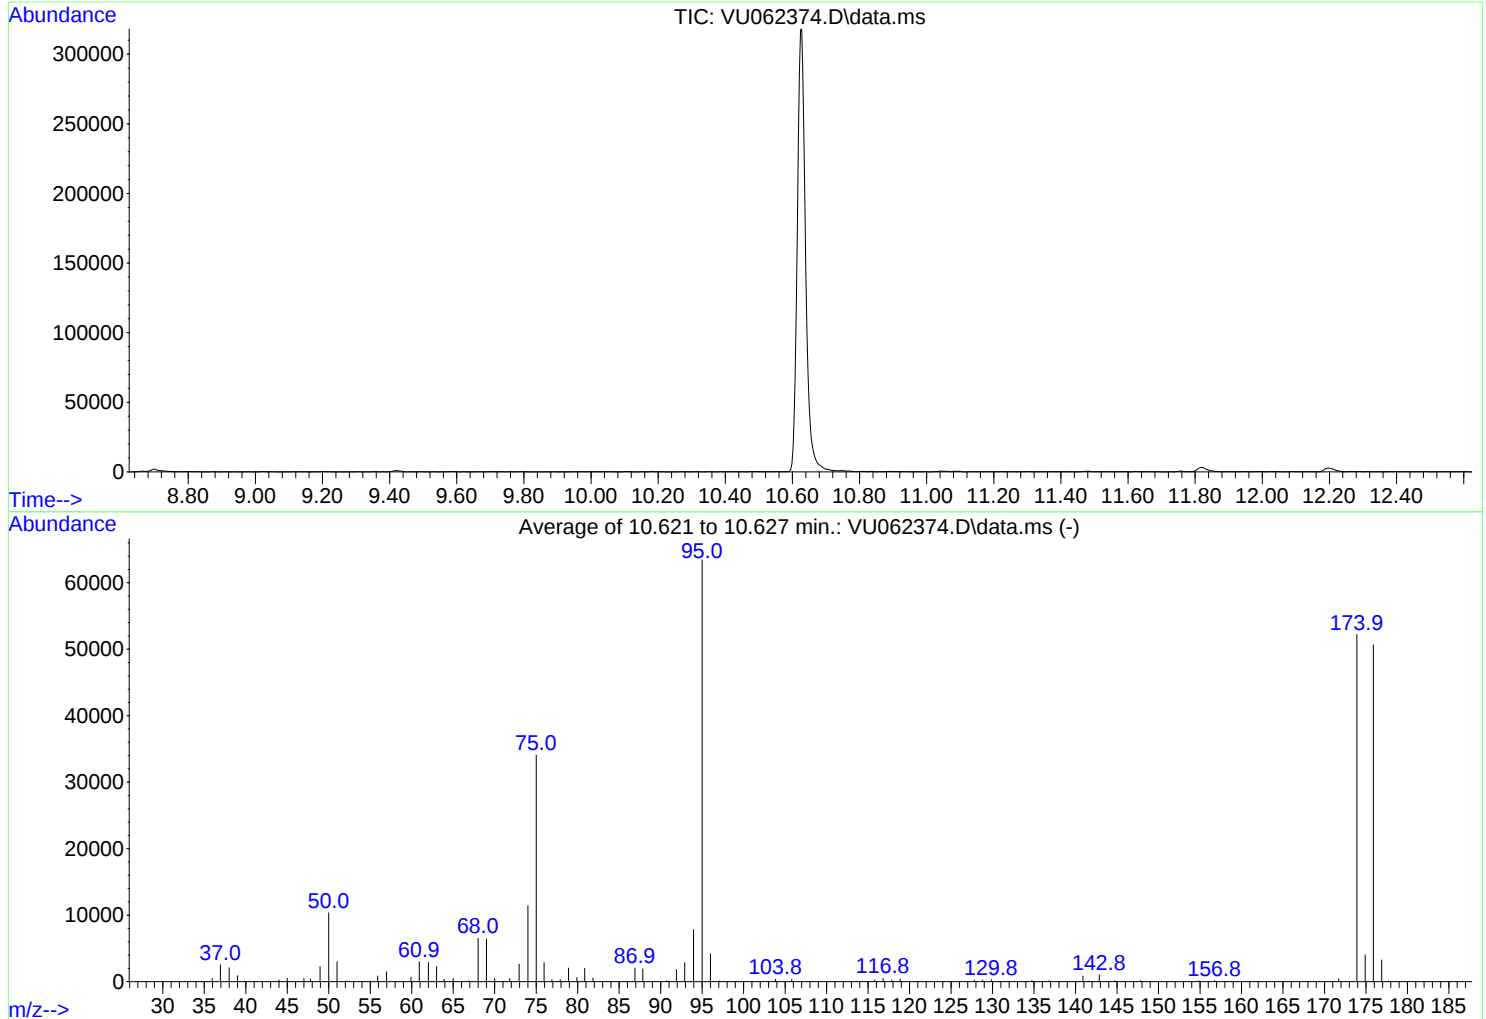

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	10363	PASS
75	95	30	80	53.7	34072	PASS
95	95	100	100	100.0	63445	PASS
96	95	5	9	6.6	4173	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.3	52211	PASS
175	174	5	9	7.7	4026	PASS
176	174	95	101	97.1	50677	PASS
177	176	5	9	6.4	3259	PASS

m/z	Abundance
44.00	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB048

m/z	Abundance
35.90	498.0
36.90	2455.0
38.00	2053.0
39.00	723.0
44.00	408.0
45.00	477.0
47.10	461.0
47.80	358.0
49.00	2162.0
50.00	9813.0
51.00	2807.0
52.10	125.0
55.00	125.0
55.90	841.0
57.00	1387.0
59.90	617.0
60.90	2896.0
62.00	2751.0
63.00	2092.0
63.90	401.0
65.00	470.0
66.90	153.0
68.00	6203.0
69.00	6057.0
70.00	501.0
71.80	468.0
73.00	2559.0
74.00	10669.0
75.00	32056.0
76.00	2776.0
76.90	257.0
77.90	287.0
78.90	1935.0
79.90	568.0
80.80	1835.0
81.80	559.0
86.90	1926.0
87.90	1964.0
90.70	236.0
91.90	1735.0
92.90	2670.0
93.90	7367.0
95.00	59952.0
96.00	3845.0
97.10	118.0
103.90	348.0
105.80	297.0
115.80	217.0
116.80	430.0
117.90	222.0
118.90	340.0
127.80	225.0
128.80	191.0
129.90	303.0
134.80	166.0
136.80	164.0
140.90	902.0
141.60	110.0
142.80	960.0
144.70	174.0
147.80	146.0
154.90	114.0
156.80	139.0
171.70	354.0
173.90	47776.0
174.90	3777.0
175.90	46744.0
176.90	2984.0
177.70	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB048

m/z	Abundance
35.90	473.0
37.00	2629.0
38.00	2130.0
39.00	910.0
39.90	127.0
44.00	407.0
45.00	492.0
47.00	474.0
47.80	412.0
48.90	2320.0
50.00	10654.0
51.00	3048.0
52.10	144.0
55.00	135.0
55.90	858.0
57.00	1502.0
59.90	685.0
60.90	3063.0
62.00	2959.0
63.00	2347.0
63.90	381.0
65.00	535.0
66.90	163.0
68.00	6765.0
69.00	6681.0
70.00	474.0
71.80	480.0
72.90	2683.0
74.00	11739.0
75.00	35000.0
76.00	2969.0
76.90	321.0
77.90	314.0
78.90	2122.0
79.90	641.0
80.80	2046.0
81.80	569.0
86.90	2115.0
87.80	1967.0
90.70	231.0
91.90	1859.0
92.90	2870.0
94.00	8055.0
95.00	65408.0
96.00	4278.0
97.00	144.0
103.80	376.0
105.80	354.0
114.80	110.0
115.80	262.0
116.80	515.0
117.80	253.0
118.90	372.0
127.80	233.0
128.80	239.0
129.90	346.0
134.70	215.0
136.80	147.0
140.90	868.0
141.60	108.0
142.80	1034.0
144.70	197.0
145.90	111.0
147.80	197.0
154.90	147.0
156.80	189.0
158.80	130.0
171.70	446.0
173.90	53800.0
174.90	4188.0
175.90	52488.0
176.90	3384.0
177.80	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB048

m/z	Abundance
36.00	427.0
37.00	2473.0
38.00	2106.0
39.00	1011.0
39.90	135.0
44.00	377.0
45.00	472.0
46.90	483.0
47.80	375.0
48.90	2348.0
50.00	10623.0
51.00	3077.0
52.00	109.0
55.00	134.0
55.90	813.0
56.90	1555.0
59.90	719.0
60.90	3057.0
62.00	2929.0
63.00	2414.0
63.90	317.0
65.00	539.0
66.90	170.0
68.00	6616.0
69.00	6485.0
70.00	404.0
71.80	417.0
73.00	2687.0
74.00	11809.0
75.00	35160.0
75.90	2889.0
76.90	354.0
77.90	312.0
78.90	2063.0
79.90	676.0
80.90	2136.0
81.90	497.0
86.90	2079.0
87.80	1828.0
90.90	244.0
91.90	1842.0
92.90	2963.0
94.00	8069.0
95.00	64976.0
96.00	4397.0
97.00	141.0
103.80	373.0
105.80	382.0
112.90	114.0
115.80	278.0
116.80	553.0
117.80	267.0
118.80	385.0
127.80	241.0
128.80	200.0
129.80	331.0
130.80	111.0
134.70	210.0
136.80	138.0
140.90	787.0
142.90	1034.0
144.80	170.0
145.80	141.0
147.90	190.0
154.90	181.0
156.70	219.0
158.70	127.0
171.70	536.0
173.90	55056.0
174.90	4114.0
175.90	52800.0
176.90	3409.0

Instrument :
MSVOA_U
ClientSampleId :
BFB048