


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121818\
Data File : VU028763.D
Acq On : 18 Dec 2018 10:54
Operator : MD/SY
Sample : BFB97
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB97

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
Title : VOC Analysis
Last Update : Wed Dec 19 00:38:48 2018

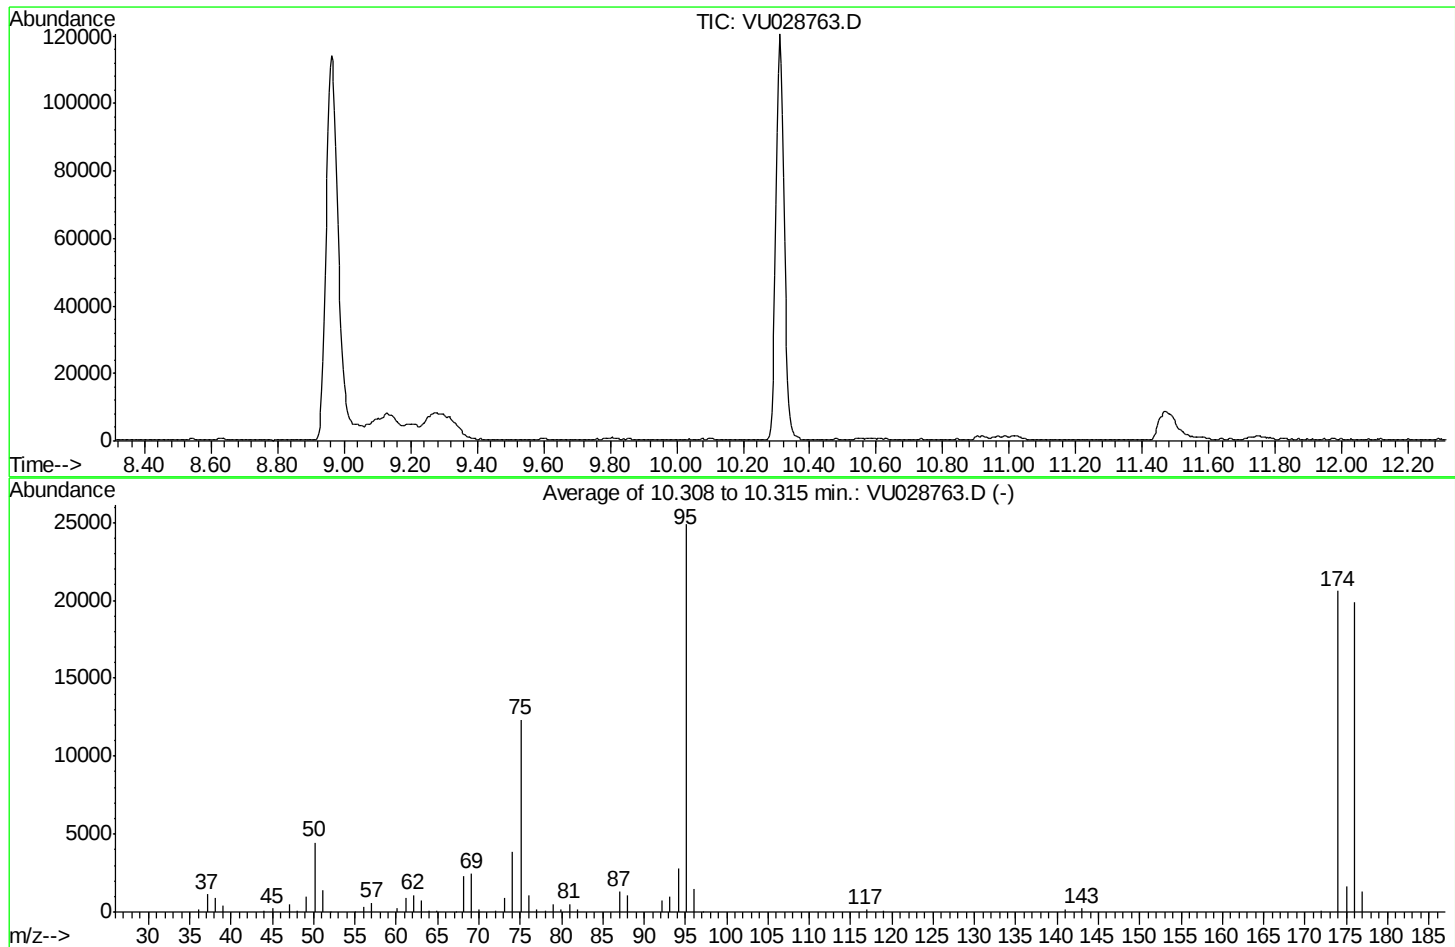

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	4451	PASS
75	95	30	80	49.7	12358	PASS
95	95	100	100	100.0	24880	PASS
96	95	5	9	6.1	1512	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.8	20589	PASS
175	174	5	9	8.0	1639	PASS
176	174	95	101	96.7	19901	PASS
177	176	5	9	6.6	1320	PASS

m/z	Abundance
44.00	345.0

Instrument :
MSVOA_U
ClientSampleId :
BFB97

m/z	Abundance
36.00	182.0
37.10	1136.0
38.10	836.0
39.00	387.0
44.00	418.0
45.00	244.0
47.00	355.0
47.90	103.0
49.10	946.0
50.10	4177.0
51.10	1298.0
56.00	273.0
57.10	555.0
60.10	200.0
61.10	875.0
62.10	1108.0
63.10	680.0
64.00	103.0
64.90	126.0
68.10	2172.0
69.10	2313.0
70.00	157.0
71.90	115.0
73.10	829.0
74.10	3763.0
75.10	11688.0
76.00	977.0
76.90	190.0
78.00	139.0
79.00	484.0
79.90	109.0
81.00	545.0
81.90	109.0
87.00	1193.0
88.00	1027.0
92.10	714.0
93.10	964.0
94.10	2749.0
95.10	23600.0
96.10	1395.0
117.00	134.0
140.90	134.0
143.00	248.0
174.00	19928.0
175.00	1495.0
176.00	19352.0
177.00	1307.0

Instrument :
MSVOA_U
ClientSampleId :
BFB97

m/z	Abundance
36.00	184.0
37.10	1180.0
38.10	894.0
39.00	418.0
44.00	433.0
45.00	232.0
47.00	479.0
48.00	102.0
49.10	1000.0
50.10	4527.0
51.10	1434.0
52.00	100.0
55.00	102.0
56.00	304.0
57.00	631.0
60.10	254.0
61.10	951.0
62.10	1147.0
63.10	740.0
64.00	114.0
64.90	108.0
67.20	116.0
68.10	2311.0
69.10	2464.0
70.00	183.0
72.10	118.0
73.10	917.0
74.10	3984.0
75.10	12677.0
76.00	1088.0
76.90	173.0
78.00	112.0
79.00	515.0
80.00	132.0
81.00	534.0
82.00	150.0
87.00	1328.0
88.00	1084.0
92.10	777.0
93.10	969.0
94.10	2882.0
95.10	25544.0
96.10	1547.0
97.10	100.0
116.90	135.0
119.00	105.0
140.90	153.0
143.00	246.0
172.00	113.0
174.00	21296.0
175.00	1682.0
176.00	20408.0
177.00	1363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB97

m/z	Abundance
36.00	188.0
37.10	1111.0
38.10	934.0
39.00	465.0
44.00	429.0
45.10	212.0
47.00	573.0
48.00	118.0
49.00	967.0
50.10	4650.0
51.10	1552.0
56.00	296.0
57.00	667.0
60.10	298.0
61.10	948.0
62.10	1049.0
63.10	767.0
64.00	124.0
68.10	2309.0
69.10	2572.0
70.00	176.0
72.10	136.0
73.10	970.0
74.10	3896.0
75.10	12710.0
76.10	1134.0
76.90	141.0
79.00	555.0
80.00	151.0
80.90	525.0
82.00	148.0
87.00	1316.0
88.00	1161.0
92.10	722.0
93.10	950.0
94.10	2840.0
95.10	25496.0
96.10	1594.0
116.90	126.0
118.90	123.0
140.90	168.0
143.00	214.0
172.00	110.0
174.00	20544.0
175.00	1742.0
176.00	19944.0
177.00	1291.0

Instrument :
MSVOA_U
ClientSampleId :
BFB97