


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121820\
Data File : VU041668.D
Acq On : 18 Dec 2020 10:13
Operator : SY/MD
Sample : L5129-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL8

Manual Integrations
APPROVED

MMDadoda
12/19/2020 12:46:08 PM

Quant Time: Dec 19 04:21:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 19 04:12:21 2020
Response via : Initial Calibration

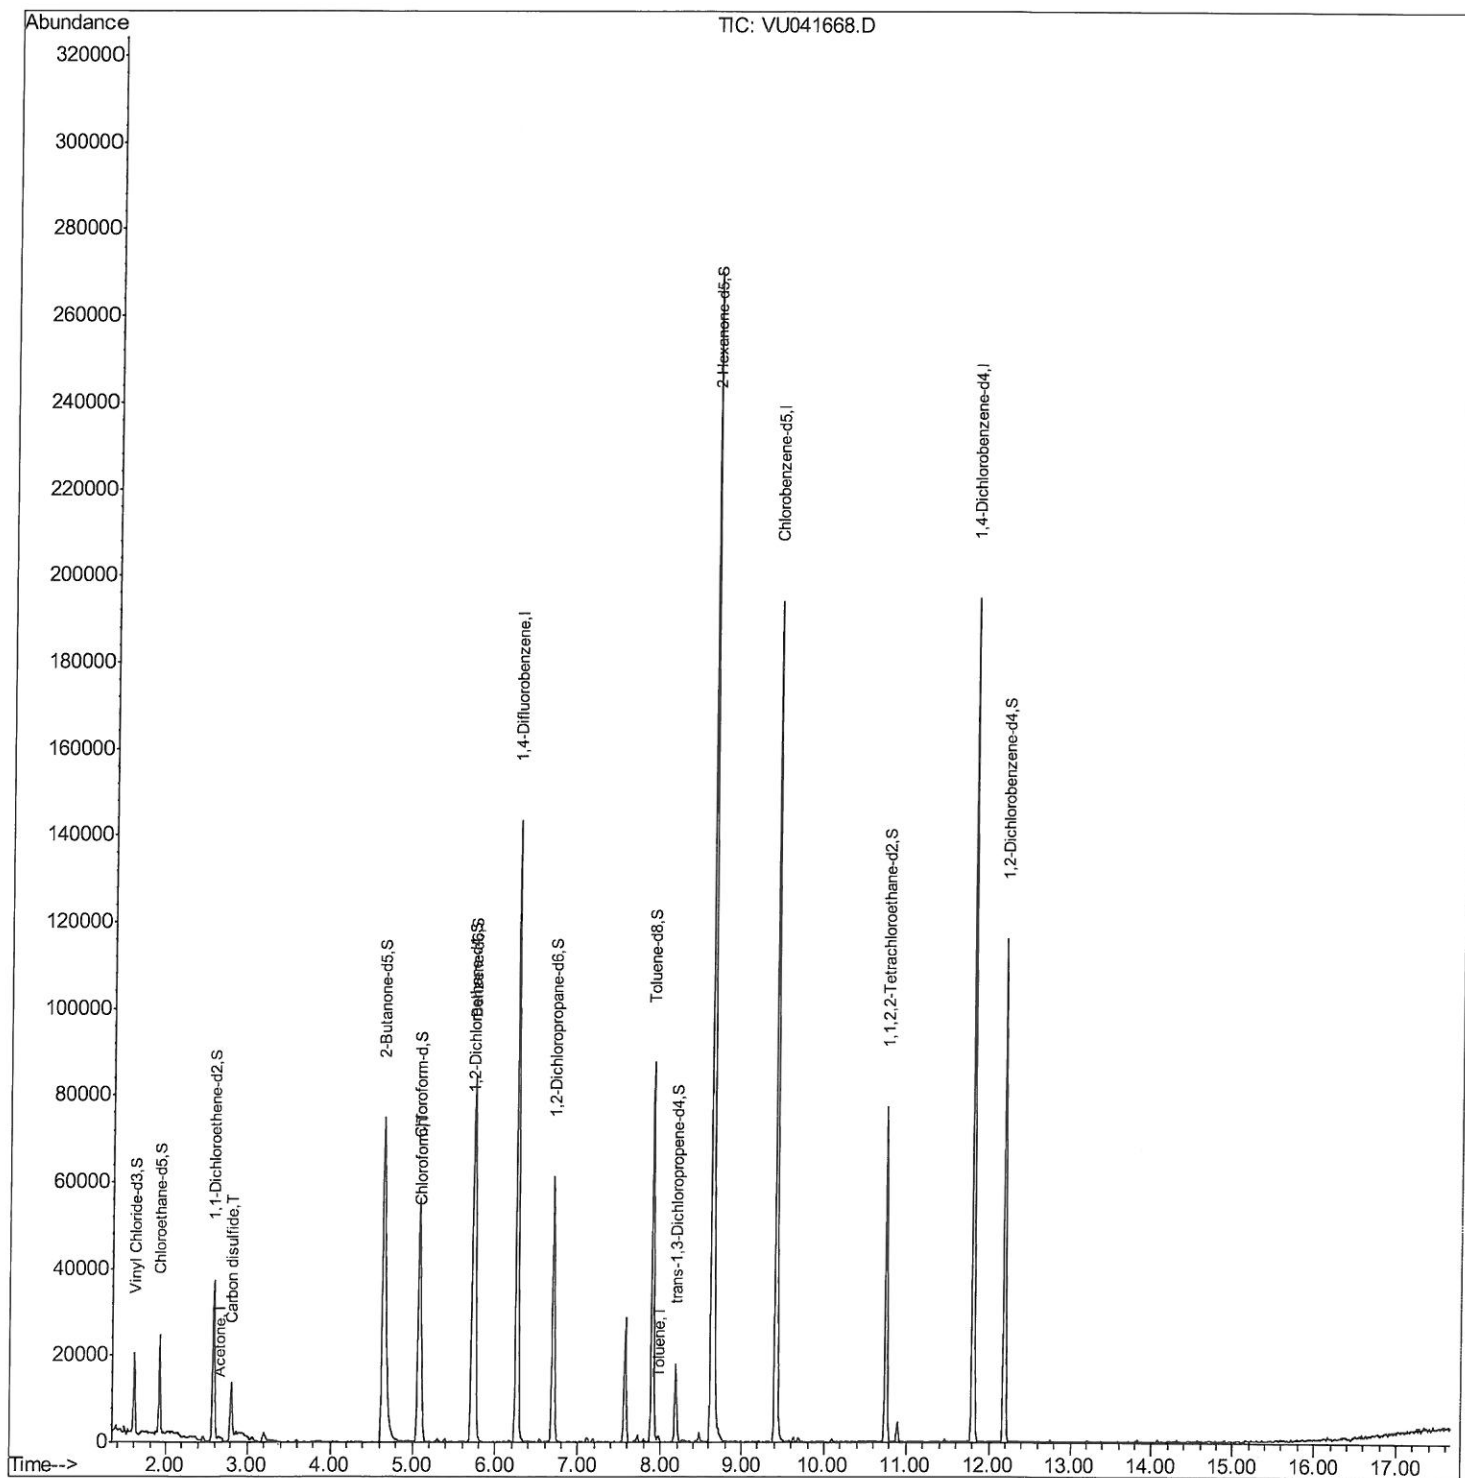

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121820\
Data File : VU041668.D
Acq On : 18 Dec 2020 10:13
Operator : SY/MD
Sample : L5129-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL8

Manual Integrations
APPROVED

MMDadoda
12/19/2020 12:46:08 PM

Quant Time: Dec 19 04:13:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 19 04:12:21 2020
Response via : Initial Calibration

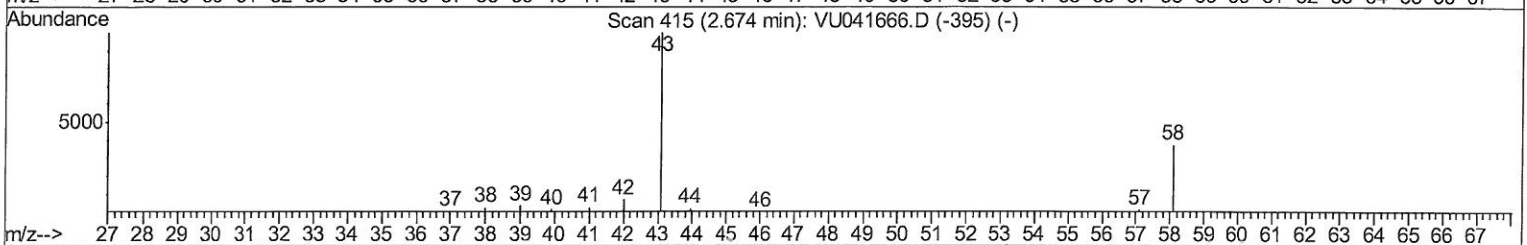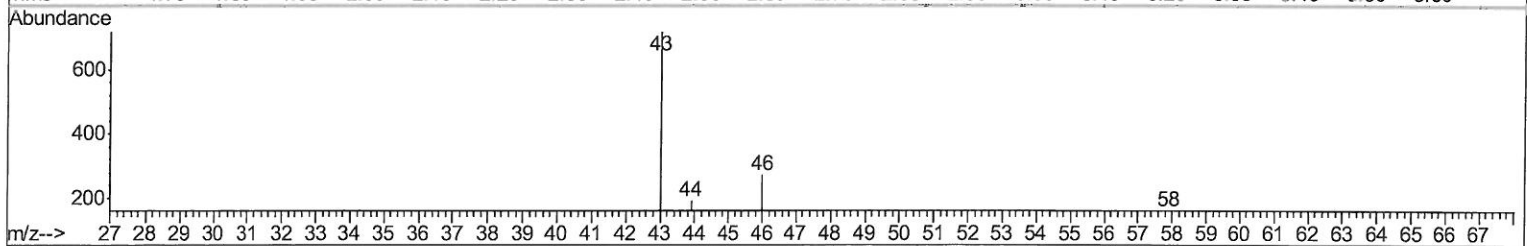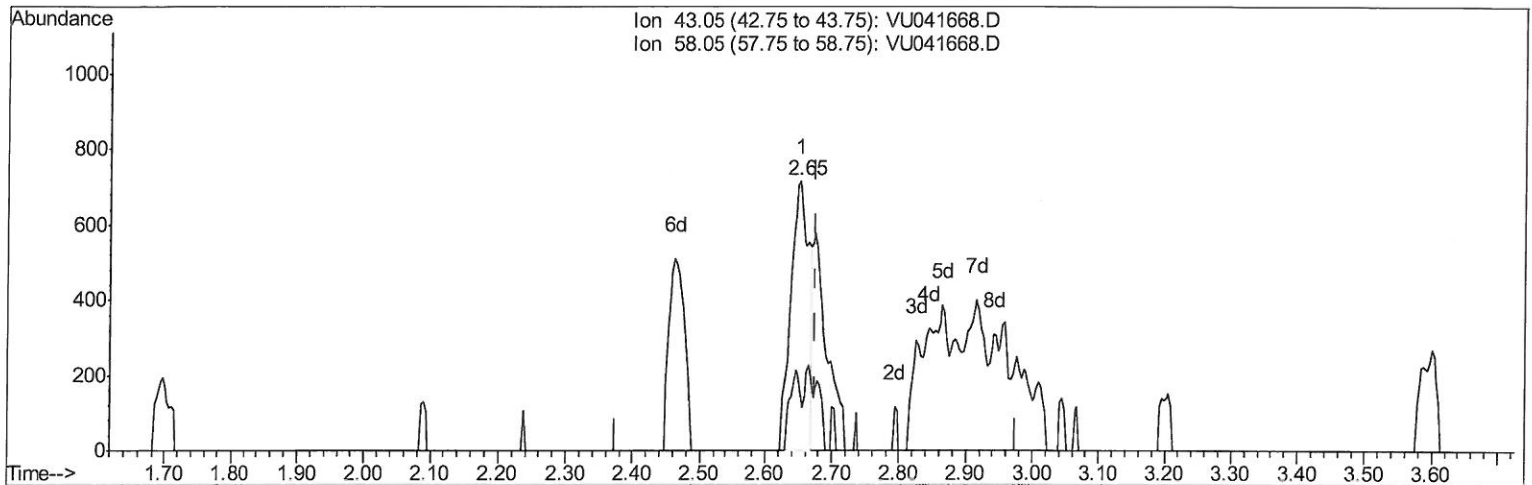

TIC: VU041668.D

(13) Acetone (T)

2.652min (-0.022) 0.79ug/L

response 1319

Ion	Exp%	Act%
43.05	100	100
58.05	36.60	18.42
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121820\
 Data File : VU041668.D
 Acq On : 18 Dec 2020 10:13
 Operator : SY/MD
 Sample : L5129-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAL8

Manual Integrations
 APPROVED

MMDadoda
 12/19/2020 12:46:08 PM

Quant Time: Dec 19 04:13:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Dec 19 04:12:21 2020
 Response via : Initial Calibration

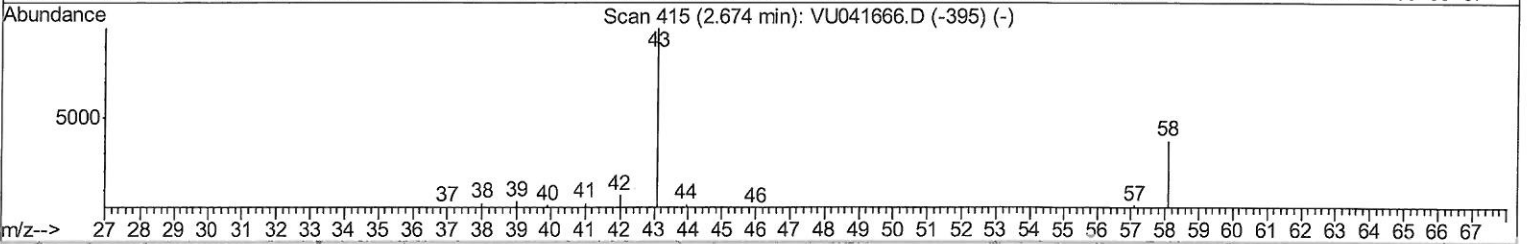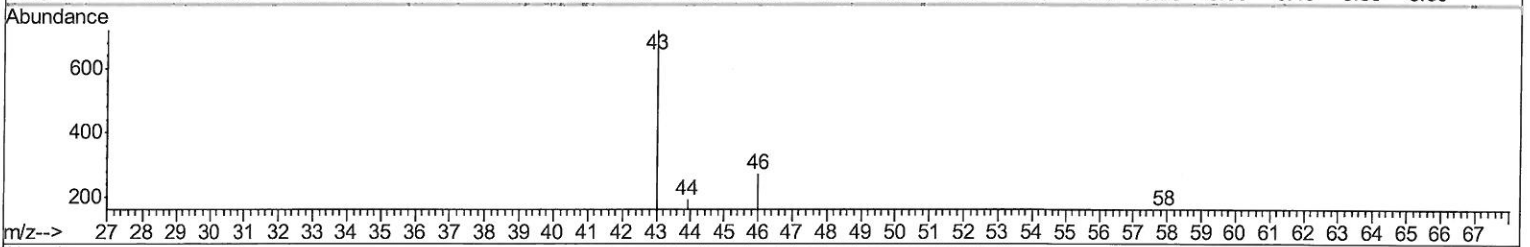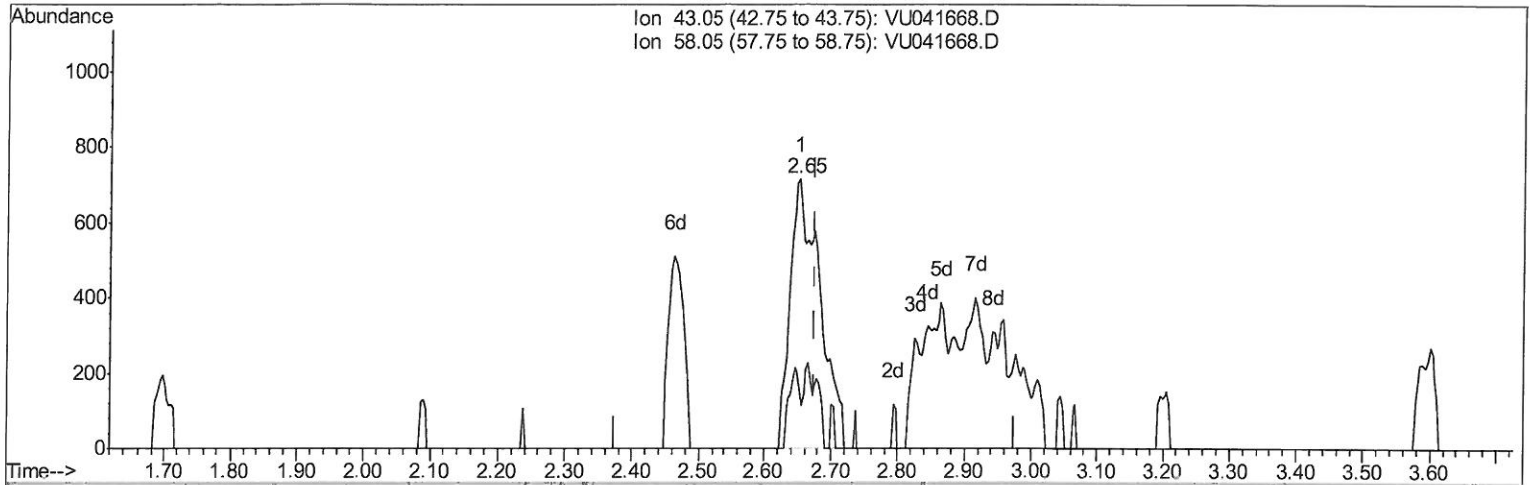

TIC: VU041668.D

(13) Acetone (T)

2.652min (-0.022) 1.31ug/L m

response 2182

Ion Exp% Act%

43.05 100 100

58.05 36.60 11.14

0.00 0.00 0.00

0.00 0.00 0.00

2mE
12/19/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121820\
 Data File : VU041668.D
 Acq On : 18 Dec 2020 10:13
 Operator : SY/MD
 Sample : L5129-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAL8

Manual Integrations
 APPROVED

MMDadoda
 12/19/2020 12:46:08 PM

Quant Time: Dec 19 04:21:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Dec 19 04:12:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.26	114	116524	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	113915	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	51969	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	12495	1.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	27.40%#
7) Chloroethane-d5	1.92	69	16760	2.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	47.60%#
11) 1,1-Dichloroethene-d2	2.58	63	22286	1.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	26.60%#
20) 2-Butanone-d5	4.65	46	137072	52.38	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.76%
24) Chloroform-d	5.08	84	48951	3.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	62.80%#
26) 1,2-Dichloroethane-d4	5.71	65	28855	3.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	65.20%#
32) Benzene-d6	5.74	84	78804	2.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	48.40%#
36) 1,2-Dichloropropane-d6	6.70	67	30434	2.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	59.60%#
41) Toluene-d8	7.90	98	59447	2.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	40.40%#
43) trans-1,3-Dichloropropene-	8.19	79	11391	2.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	49.60%#
46) 2-Hexanone-d5	8.64	63	102855	40.91	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.82%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	40275	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	31658	3.43	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	68.60%#

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.65	43	2182m	1.311	ug/L	
14) Carbon disulfide	2.81	76	17207	0.630	ug/L #	95
25) Chloroform	5.10	83	12687	0.824	ug/L	95
42) Toluene	7.97	91	1321	0.035	ug/L	97

2 mfd
 12/19/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed