


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121820\
 Data File : VU041665.D
 Acq On : 18 Dec 2020 08:30
 Operator : SY/MD
 Sample : BFB26
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB26

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Dec 19 04:12:21 2020

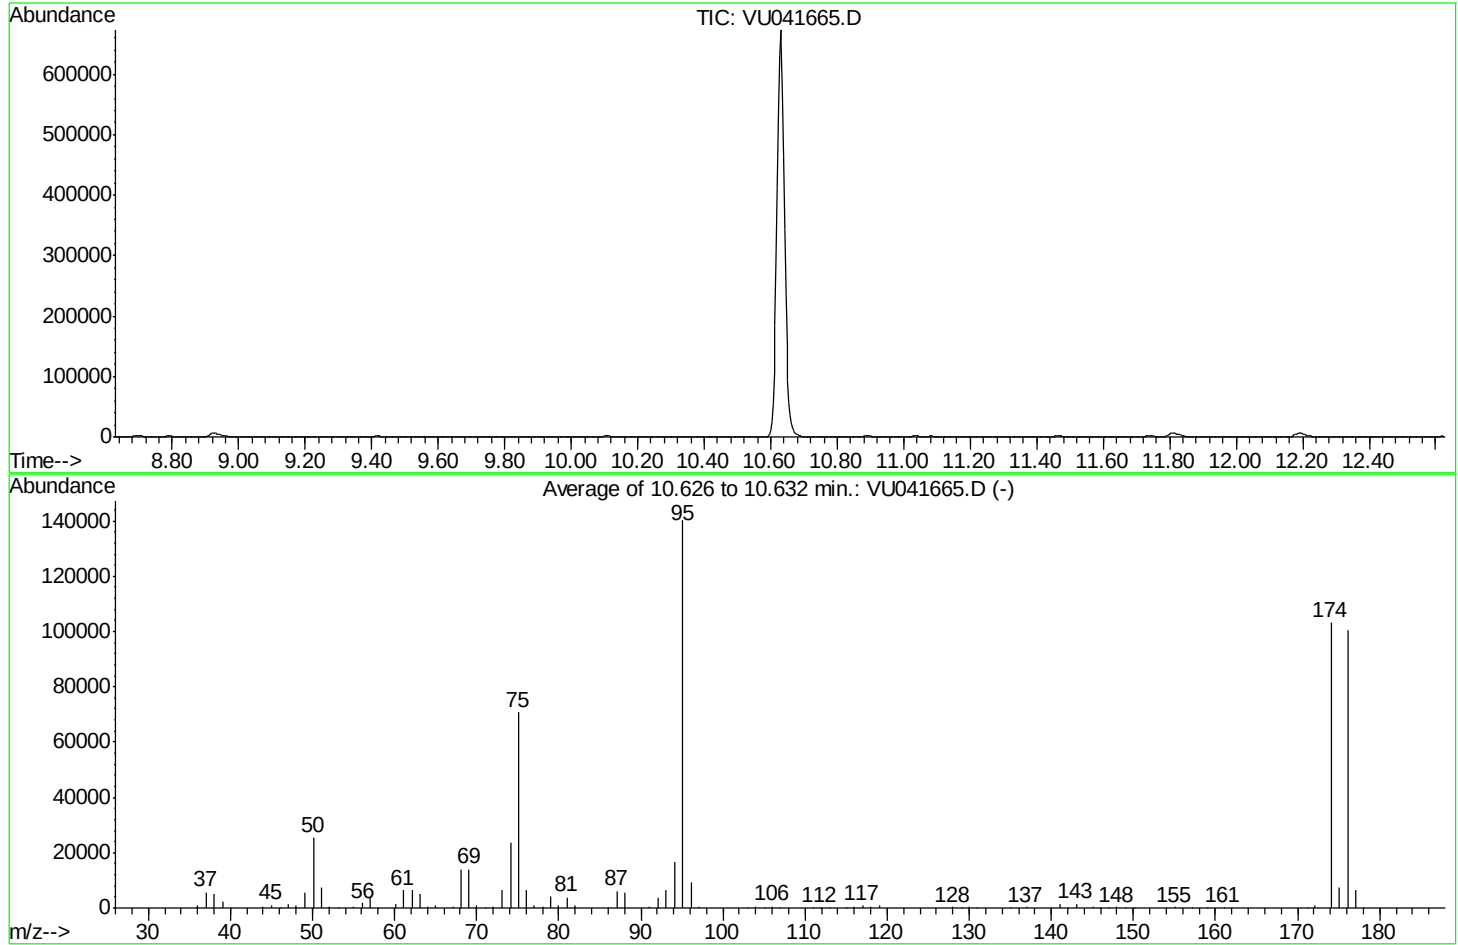

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2873

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	25304	PASS
75	95	30	80	50.4	70677	PASS
95	95	100	100	100.0	140202	PASS
96	95	5	9	6.6	9234	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	103141	PASS
175	174	5	9	7.4	7621	PASS
176	174	95	101	97.6	100693	PASS
177	176	5	9	6.4	6429	PASS

m/z	Abundance
36.00	1048.0
37.00	5389.0
38.00	5093.0
39.10	2442.0
40.00	238.0
44.00	894.0
45.00	938.0
46.10	178.0
47.10	1423.0
48.00	800.0
49.10	5425.0
50.10	24592.0
51.10	7316.0
52.10	347.0
54.90	308.0
56.10	1843.0
57.10	3497.0
57.90	212.0
60.10	1301.0
61.10	6487.0
62.10	6256.0
63.10	5352.0
64.10	663.0
65.00	880.0
67.10	455.0
68.10	13641.0
69.10	13755.0
70.00	1074.0
72.10	667.0
73.10	6085.0
74.10	23032.0
75.10	68888.0
76.10	5990.0
77.00	881.0
78.00	631.0
79.00	3815.0
80.00	1140.0
81.00	3938.0
82.00	912.0
86.00	135.0
87.00	6004.0
88.00	5617.0
91.00	397.0
92.10	3540.0
93.10	5982.0
94.10	16048.0
95.10	136960.0
96.10	9266.0
97.10	268.0
103.00	112.0
104.00	436.0
105.00	228.0
106.00	593.0
106.90	124.0
110.90	122.0
112.90	131.0
116.00	387.0
117.00	774.0
118.00	516.0
119.00	809.0
128.00	387.0
129.00	215.0
130.00	355.0
131.00	127.0
135.00	121.0
137.00	271.0
141.00	1065.0
141.90	130.0
143.00	1463.0
145.10	406.0
145.90	137.0
147.00	175.0
148.00	381.0
149.10	106.0
154.00	146.0
155.10	299.0
157.10	151.0
159.10	182.0
161.00	119.0
171.10	176.0
172.10	992.0
174.10	97504.0
175.10	7234.0
176.10	95912.0
177.10	6235.0
178.00	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	1035.0
37.00	5823.0
38.00	5076.0
39.10	2275.0
40.00	228.0
44.00	864.0
45.00	979.0
46.10	156.0
47.10	1515.0
48.00	819.0
49.00	5639.0
50.10	26272.0
51.10	7649.0
52.10	365.0
55.00	315.0
56.10	1819.0
57.10	3746.0
58.00	199.0
60.10	1401.0
61.10	6729.0
62.10	6654.0
63.10	5535.0
64.10	673.0
65.00	779.0
67.10	431.0
68.10	14464.0
69.10	14426.0
70.00	1053.0
71.00	110.0
72.00	679.0
73.10	6759.0
74.10	24536.0
75.10	73032.0
76.10	6506.0
77.00	912.0
78.00	662.0
79.00	4093.0
80.00	1223.0
81.00	4021.0
82.00	888.0
86.00	156.0
87.10	6278.0
88.00	5988.0
91.00	426.0
92.10	3852.0
93.10	6538.0
94.10	17136.0
95.10	144576.0
96.10	9549.0
97.10	338.0
104.00	537.0
105.00	230.0
106.00	622.0
106.90	130.0
111.90	117.0
113.00	181.0
115.00	106.0
116.00	487.0
117.00	814.0
118.00	562.0
119.10	739.0
128.00	449.0
129.00	254.0
130.00	338.0
131.00	115.0
134.90	146.0
137.00	314.0
140.00	126.0
141.10	1240.0
141.90	175.0
143.10	1586.0
145.10	415.0
145.90	125.0
146.90	158.0
148.00	425.0
149.10	137.0
150.10	127.0
154.00	130.0
155.10	357.0
157.10	217.0
159.00	145.0
161.00	128.0
171.20	175.0
172.10	1036.0
174.10	106416.0
175.10	7802.0
176.10	104192.0
177.10	6617.0
178.00	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	968.0
37.00	5582.0
38.10	4708.0
39.00	1974.0
40.10	229.0
44.00	815.0
45.00	964.0
47.10	1408.0
48.10	747.0
49.00	5354.0
50.10	25048.0
51.10	7361.0
52.10	319.0
53.10	102.0
55.00	322.0
56.10	1678.0
57.10	3513.0
58.00	171.0
60.10	1415.0
61.00	6227.0
62.10	6501.0
63.10	5087.0
64.00	590.0
65.10	626.0
67.20	414.0
68.10	13655.0
69.10	13826.0
70.00	977.0
71.00	120.0
72.00	656.0
73.10	6568.0
74.10	23792.0
75.10	70112.0
76.10	6344.0
77.00	832.0
78.00	624.0
79.00	4080.0
80.00	1164.0
81.00	3683.0
82.00	845.0
86.00	188.0
87.10	6058.0
88.00	5723.0
91.00	392.0
92.10	3770.0
93.10	6315.0
94.10	16864.0
95.10	139072.0
96.10	8888.0
97.10	358.0
104.00	554.0
105.00	209.0
106.00	584.0
106.90	121.0
111.90	147.0
113.00	203.0
115.00	142.0
116.00	502.0
117.00	744.0
117.90	520.0
119.10	598.0
128.00	466.0
129.00	245.0
130.00	342.0
134.90	149.0
137.00	319.0
140.00	119.0
141.10	1311.0
142.00	195.0
143.10	1574.0
145.00	377.0
146.00	132.0
146.90	112.0
148.00	386.0
149.00	119.0
150.10	157.0
154.00	115.0
155.10	310.0
157.10	238.0
158.90	119.0
161.00	138.0
171.10	142.0
172.10	892.0
174.10	105504.0
175.10	7829.0
176.10	101976.0
177.10	6435.0
178.00	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
44.10	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26