

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
 Data File : VU057000.D
 Acq On : 18 Dec 2023 17:57
 Operator : MD/SY
 Sample : 05810-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C91

Quant Time: Dec 19 01:42:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 19 01:20:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	236875	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	257143	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	98743	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	94188	4.639	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.800%
7) Chloroethane-d5	1.907	69	76103	5.009	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.200%
11) 1,1-Dichloroethene-d2	2.560	65	40970	4.716	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.400%
20) 2-Butanone-d5	4.615	46	169429	42.254	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.500%
24) Chloroform-d	5.055	84	179115	4.659	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
26) 1,2-Dichloroethane-d4	5.695	65	84749	4.658	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	5.721	84	340422	4.268	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%
36) 1,2-Dichloropropane-d6	6.685	67	108724	4.355	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.200%
41) Toluene-d8	7.894	98	294239	4.128	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	8.177	79	39664	4.097	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.000%
46) 2-Hexanone-d5	8.627	63	145376	39.814	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.620%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	77547	4.293	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.800%
66) 1,2-Dichlorobenzene-d4	12.190	152	92864	4.784	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds					Qvalue	
13) Acetone	2.624	43	14194	5.809	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
Data File : VU057000.D
Acq On : 18 Dec 2023 17:57
Operator : MD/SY
Sample : 05810-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C91

Quant Time: Dec 19 01:42:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 19 01:20:32 2023
Response via : Initial Calibration

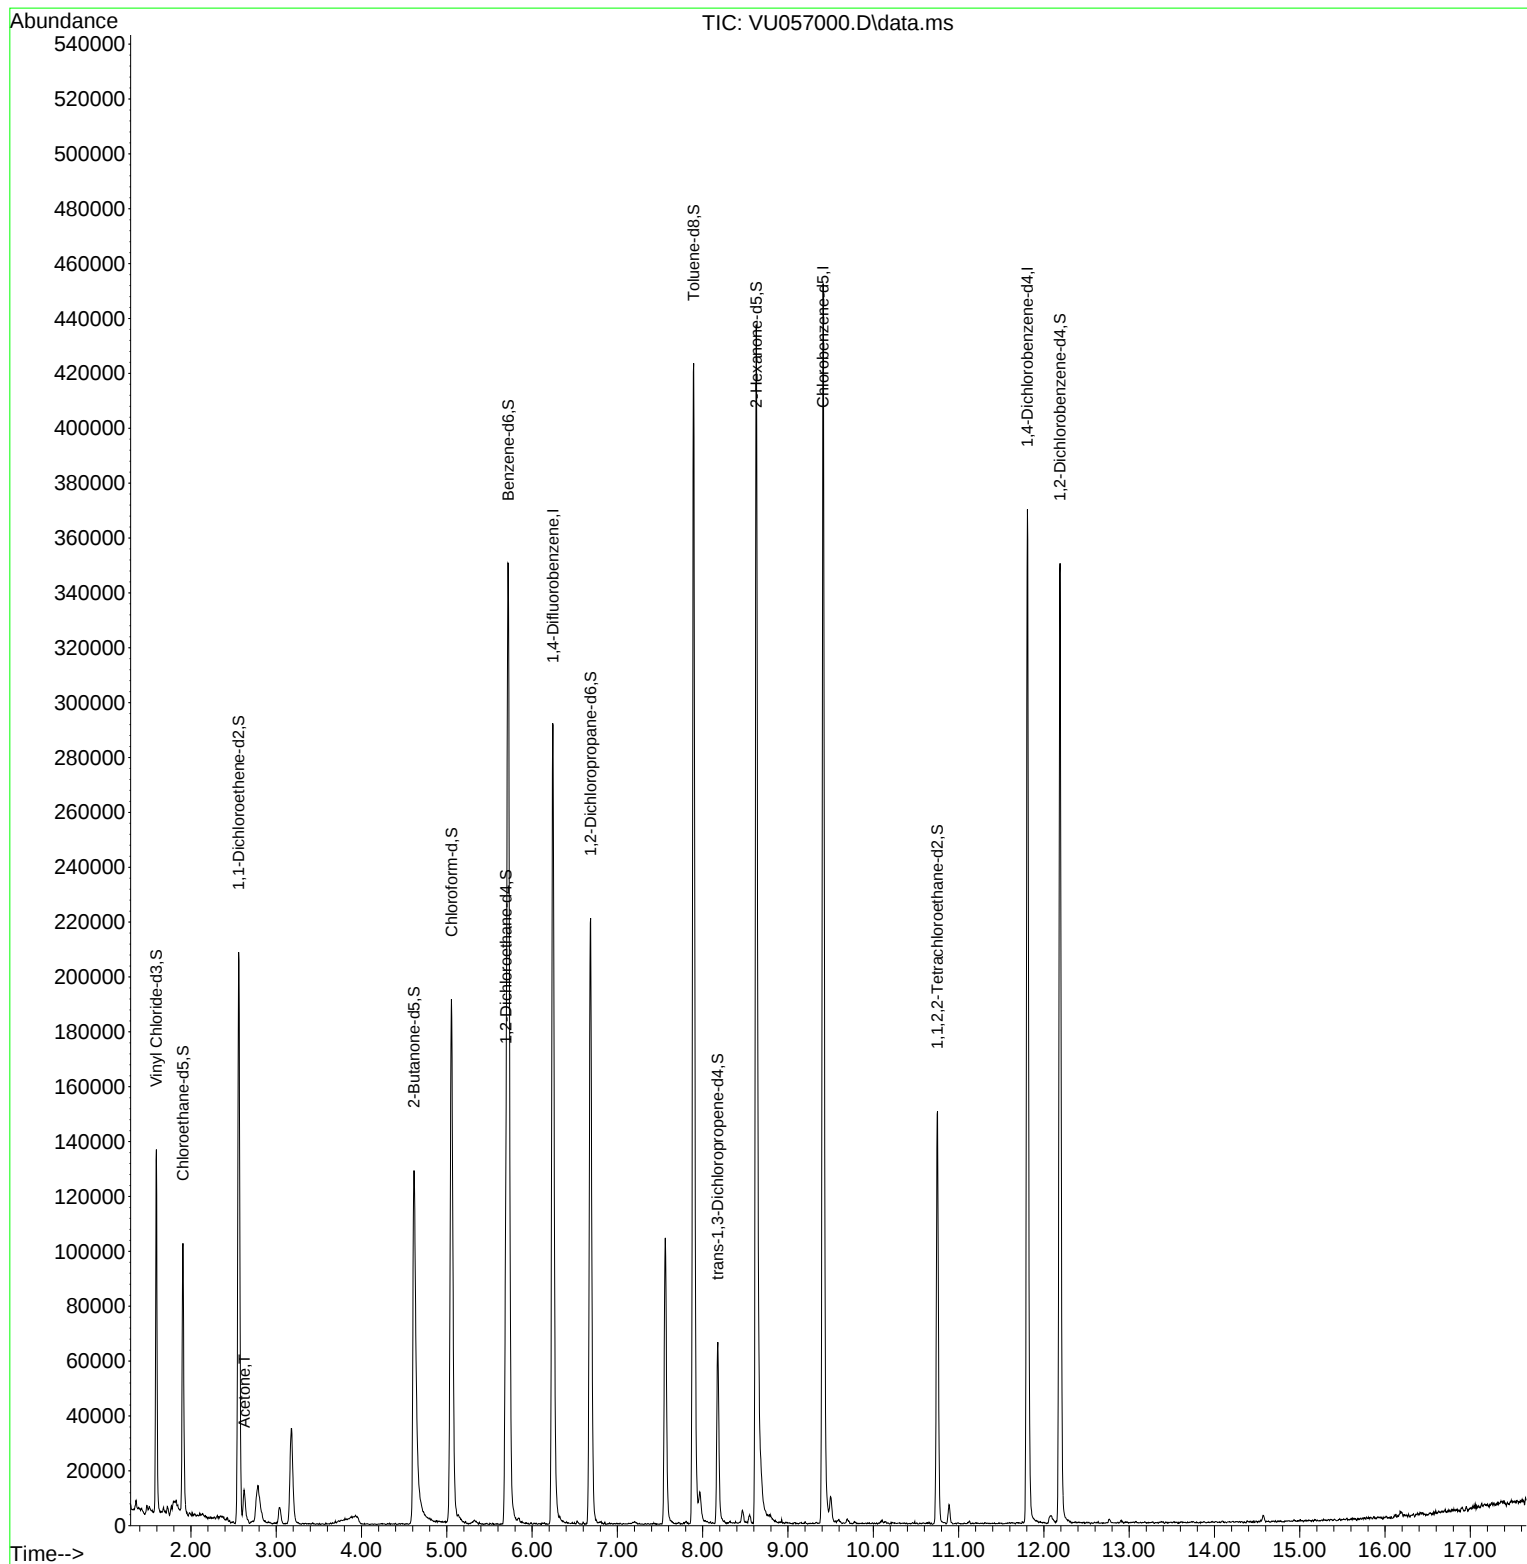

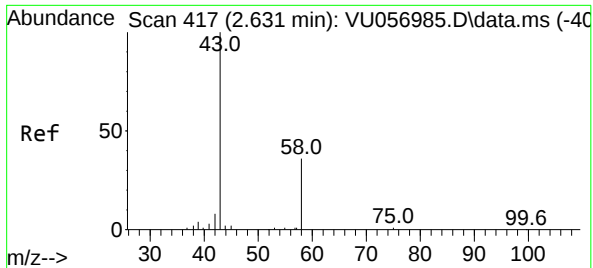

#13
 Acetone
 Concen: 5.809 ug/L
 RT: 2.624 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VU057000.D
 Acq: 18 Dec 2023 17:57

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C91

Tgt Ion: 43 Resp: 14194
 Ion Ratio Lower Upper
 43 100
 58 38.6 0.0 72.6

