

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
 Data File : VU057014.D
 Acq On : 19 Dec 2023 00:29
 Operator : MD/SY
 Sample : 05830-03 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rVB	120159	138972	15.82%	1.835%
2	1.911	184	193	206	rBV	92132	125088	14.24%	1.652%
3	2.563	383	396	414	rBV2	206908	355016	40.40%	4.689%
4	3.039	533	544	558	rBV2	11003	22064	2.51%	0.291%
5	3.174	572	586	604	rBV	20496	49691	5.66%	0.656%
6	4.628	1025	1038	1076	rBV	107289	341955	38.92%	4.516%
7	5.055	1155	1171	1191	rBV	176576	398544	45.36%	5.264%
8	5.718	1355	1377	1402	rBV2	336984	878652	100.00%	11.604%
9	6.242	1525	1540	1567	rBV	306511	602102	68.53%	7.952%
10	6.538	1620	1632	1655	rVB	70975	135471	15.42%	1.789%
11	6.685	1664	1678	1701	rBV	212729	421882	48.01%	5.572%
12	7.560	1935	1950	1970	rBV2	90517	167099	19.02%	2.207%
13	7.894	2041	2054	2074	rBV	375276	684933	77.95%	9.046%
14	8.177	2131	2142	2163	rBV2	56329	100895	11.48%	1.333%
15	8.547	2245	2257	2272	rBV2	215491	370058	42.12%	4.887%
16	8.631	2272	2283	2320	rVV2	372998	786167	89.47%	10.383%
17	9.412	2513	2526	2554	rBV	411191	718240	81.74%	9.486%
18	10.750	2931	2942	2961	rBV	125301	207285	23.59%	2.738%
19	11.807	3256	3271	3293	rBV	342957	565207	64.33%	7.465%
20	12.190	3377	3390	3408	rBV	294062	502445	57.18%	6.636%




Sum of corrected areas: 7571766

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
Data File : VU057014.D
Acq On : 19 Dec 2023 00:29
Operator : MD/SY
Sample : 05830-03 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

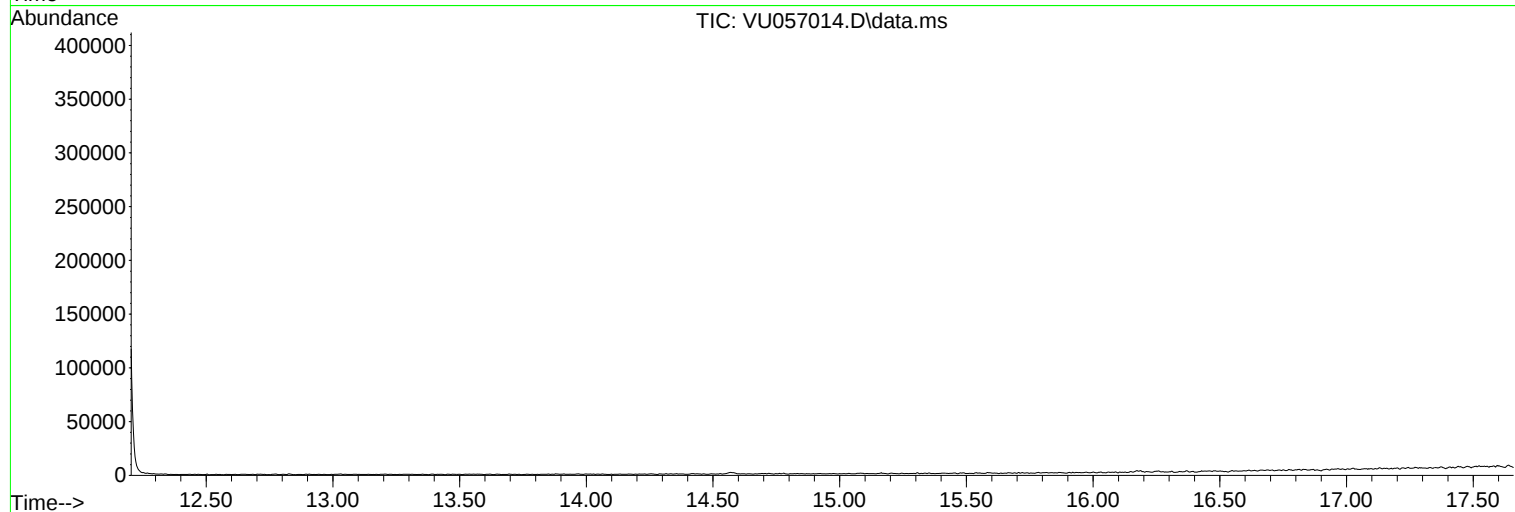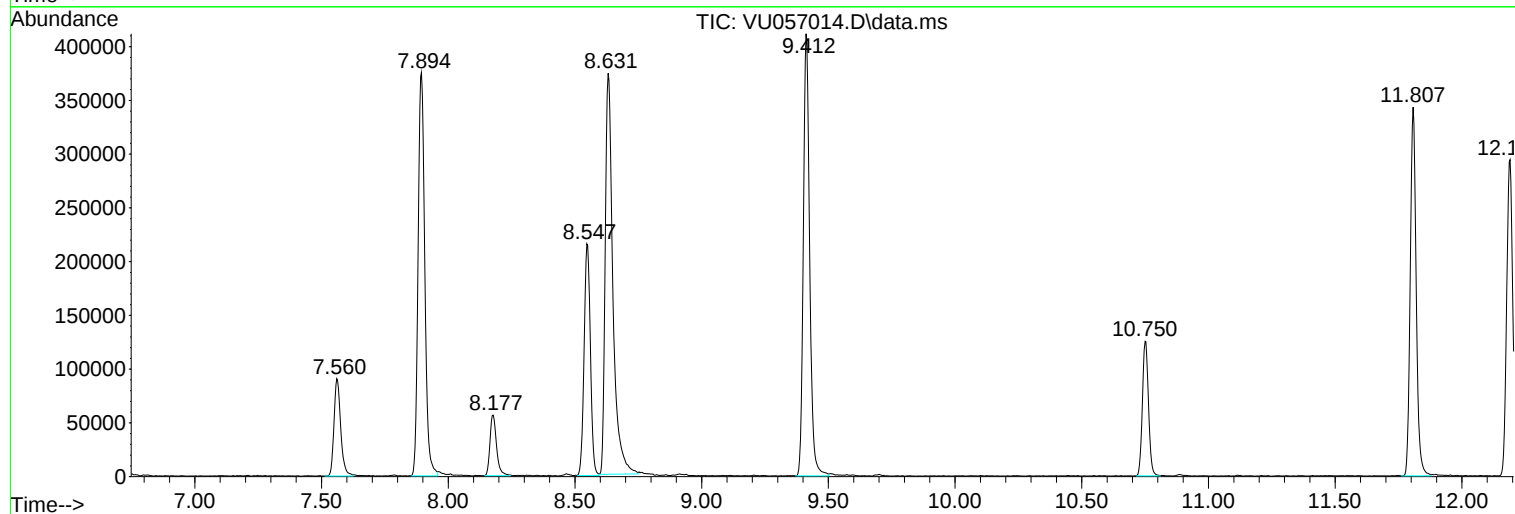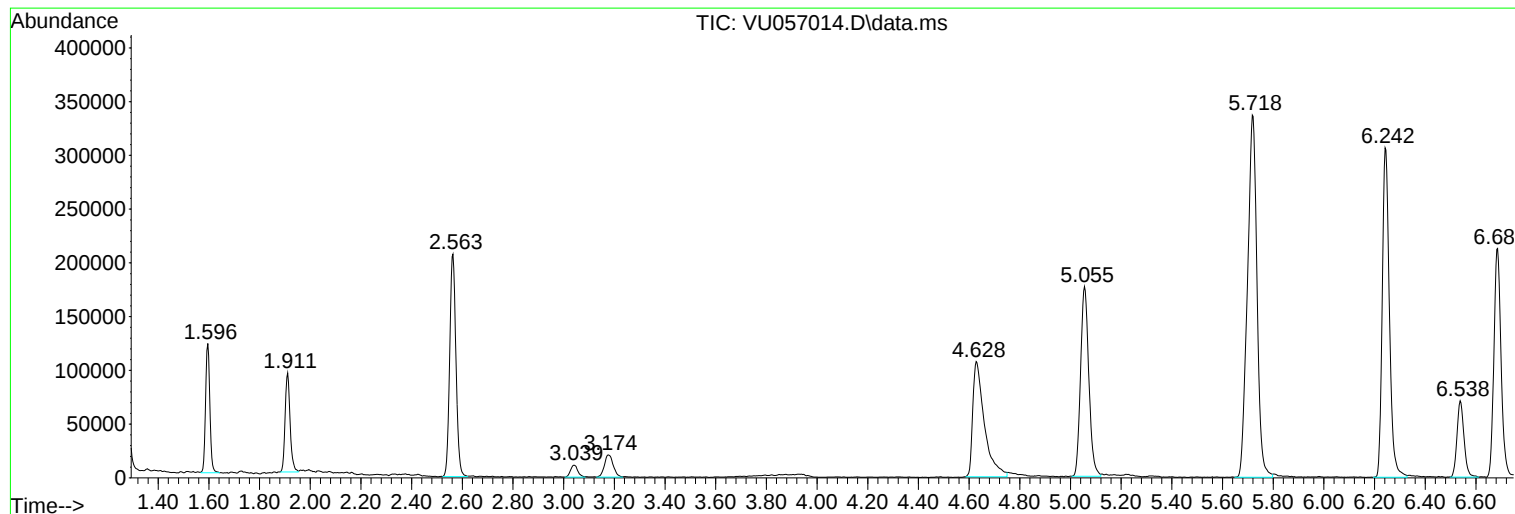

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
Data File : VU057014.D
Acq On : 19 Dec 2023 00:29
Operator : MD/SY
Sample : 05830-03 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
Data File : VU057014.D
Acq On : 19 Dec 2023 00:29
Operator : MD/SY
Sample : 05830-03 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc