

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
 Data File : VU057024.D
 Acq On : 19 Dec 2023 04:31
 Operator : MD/SY
 Sample : 05843-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C67

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	107	rVB	118002	137293	16.81%	1.998%
2	1.907	184	192	205	rVB	84932	117402	14.37%	1.709%
3	2.563	384	396	412	rBV	196424	320380	39.22%	4.662%
4	4.624	1025	1037	1076	rBV	92151	265224	32.47%	3.860%
5	5.055	1156	1171	1194	rBV	156838	361393	44.25%	5.259%
6	5.721	1358	1378	1407	rBV2	315070	816784	100.00%	11.887%
7	6.242	1528	1540	1573	rBV	282309	549379	67.26%	7.995%
8	6.685	1662	1678	1700	rBV	189962	380142	46.54%	5.532%
9	7.560	1938	1950	1970	rBV	90001	166620	20.40%	2.425%
10	7.894	2041	2054	2073	rBV	366680	663778	81.27%	9.660%
11	7.968	2074	2077	2086	rVB2	6630	8173	1.00%	0.119%
12	8.177	2131	2142	2163	rBV	54934	98221	12.03%	1.429%
13	8.550	2246	2258	2272	rBV2	69655	120828	14.79%	1.758%
14	8.631	2272	2283	2313	rBV2	371969	750908	91.93%	10.928%
15	9.412	2513	2526	2548	rBV	425804	747830	91.56%	10.883%
16	10.749	2931	2942	2960	rBV	143040	237378	29.06%	3.455%
17	10.888	2976	2985	2995	rBV3	7084	10955	1.34%	0.159%
18	11.807	3259	3271	3301	rBV	356996	585578	71.69%	8.522%
19	12.187	3375	3389	3412	rBV	309637	533173	65.28%	7.759%




Sum of corrected areas: 6871439

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
Data File : VU057024.D
Acq On : 19 Dec 2023 04:31
Operator : MD/SY
Sample : 05843-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

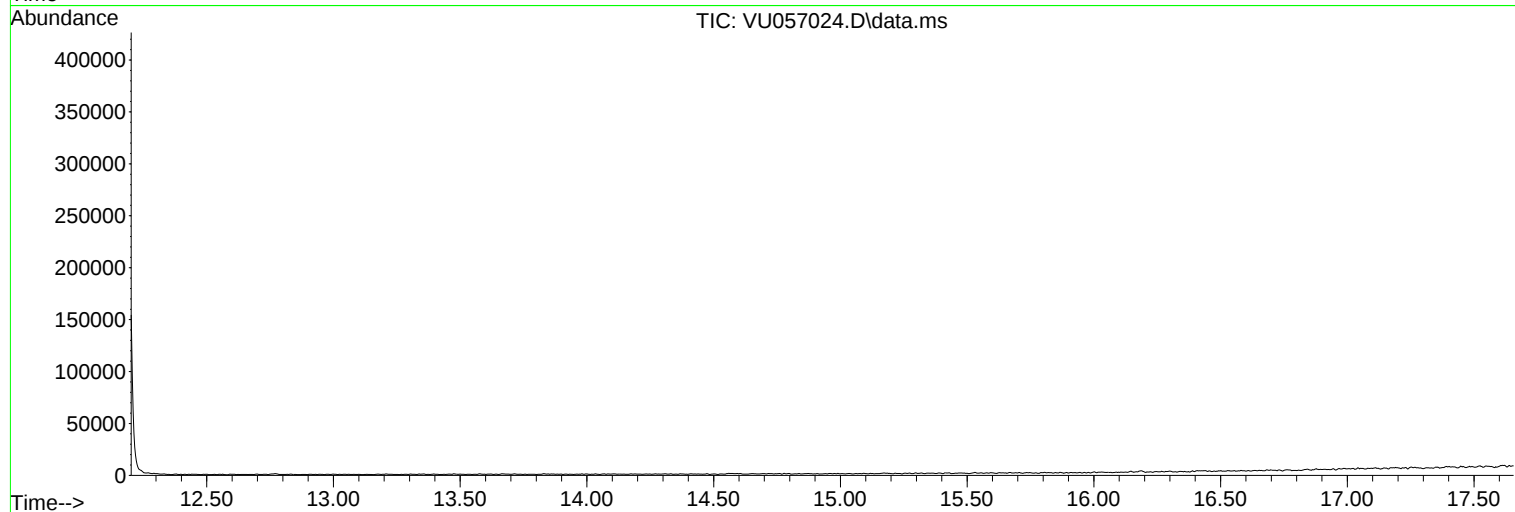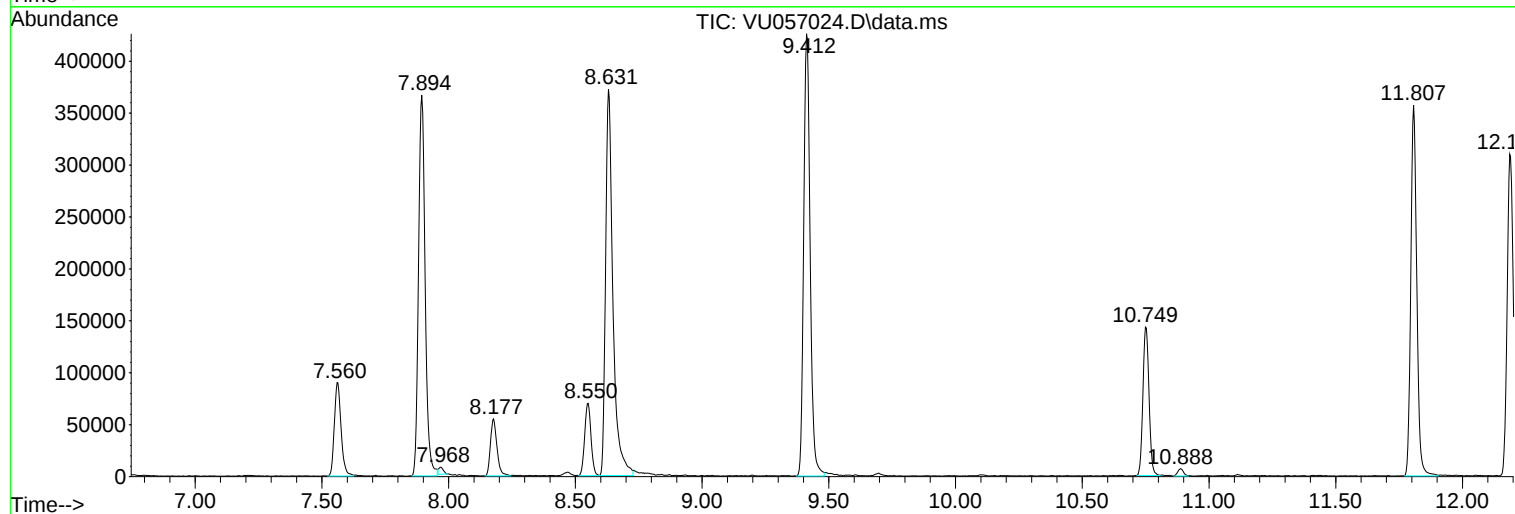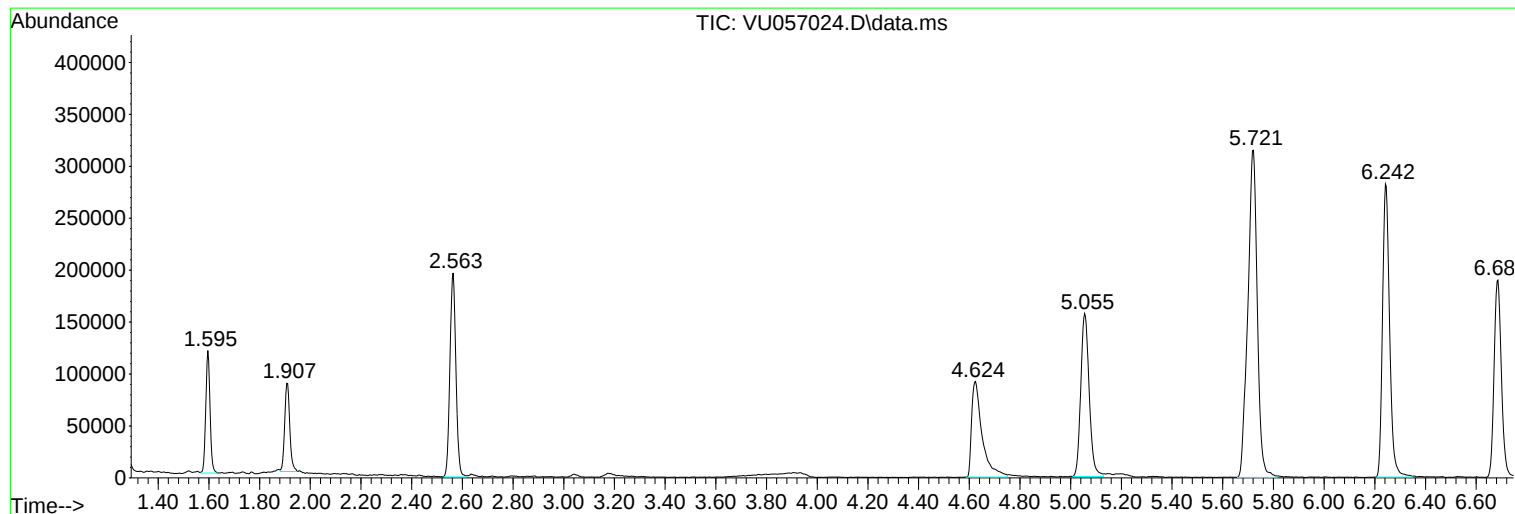

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
Data File : VU057024.D
Acq On : 19 Dec 2023 04:31
Operator : MD/SY
Sample : 05843-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
Data File : VU057024.D
Acq On : 19 Dec 2023 04:31
Operator : MD/SY
Sample : 05843-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc