


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121823\
Data File : VU056984.D
Acq On : 18 Dec 2023 09:28
Operator : MD/SY
Sample : BFB096
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB096

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 19 02:36:03 2023

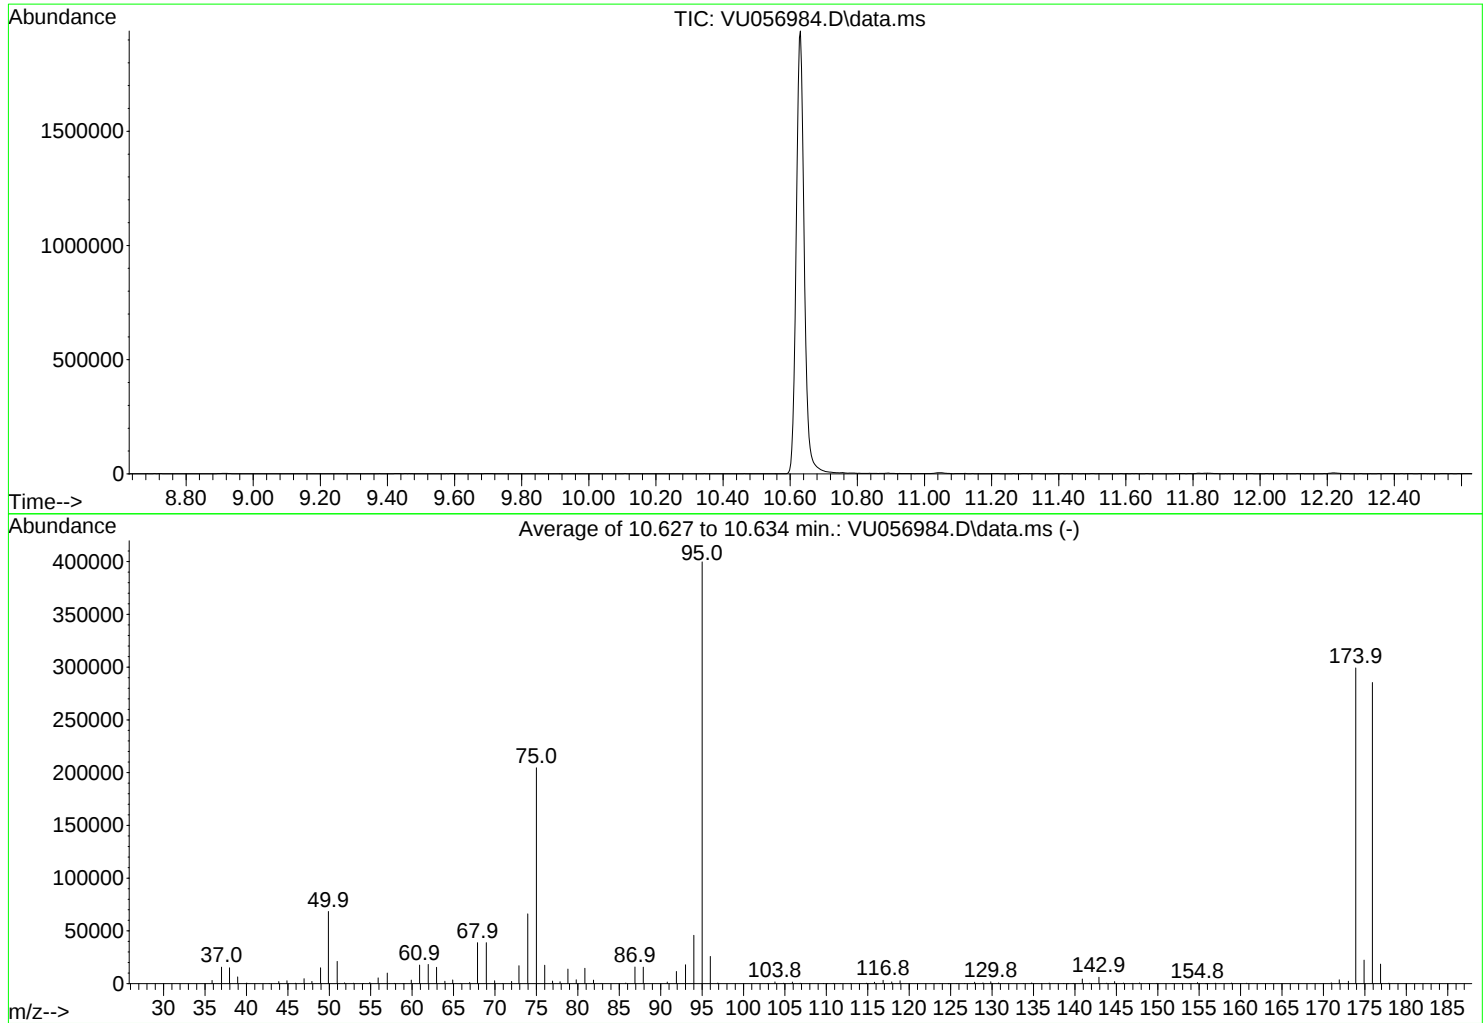

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	68475	PASS
75	95	30	80	51.2	204565	PASS
95	95	100	100	100.0	399787	PASS
96	95	5	9	6.5	25827	PASS
173	174	0.00	2	0.7	2218	PASS
174	95	50	120	74.8	299200	PASS
175	174	5	9	7.5	22328	PASS
176	174	95	101	95.4	285419	PASS
177	176	5	9	6.5	18549	PASS

Scan 2889 (10.579 min): VU056984.D\data.ms
BFB096

m/z	Abundance
39.80	300.0
43.90	445.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.90	3190.0
37.00	15782.0
37.90	15324.0
38.90	6922.0
40.10	660.0
42.80	184.0
43.90	2642.0
44.90	2856.0
46.00	531.0
46.90	4730.0
47.90	2302.0
49.00	15815.0
49.90	70928.0
51.00	21912.0
51.90	781.0
53.00	437.0
54.10	154.0
54.90	1005.0
55.90	5705.0
57.00	10807.0
57.80	343.0
58.90	143.0
59.90	3497.0
60.90	18728.0
62.00	18520.0
63.00	16141.0
63.90	2586.0
64.90	3726.0
65.80	392.0
67.00	1164.0
67.90	39928.0
69.00	40392.0
69.90	2891.0
70.90	199.0
72.00	2245.0
72.90	17360.0
73.90	67648.0
75.00	210624.0
76.00	18336.0
77.00	2388.0
77.80	1922.0
78.80	14456.0
79.80	3737.0
80.80	15198.0
81.90	3575.0
82.80	389.0
85.80	641.0
86.90	16033.0
87.90	15614.0
90.80	1519.0
91.90	12121.0
93.00	18096.0
94.00	46896.0
95.00	409664.0
96.00	26336.0
96.90	647.0
102.90	272.0
103.80	1544.0
104.90	553.0
105.90	1566.0
106.80	418.0
108.00	176.0
109.70	204.0
110.90	331.0
111.90	250.0
112.90	338.0
114.80	446.0
115.80	1393.0
116.90	3456.0
117.90	1839.0
118.90	2874.0
123.70	150.0
125.70	159.0
126.70	203.0
127.90	1433.0
128.90	812.0
129.80	1703.0
130.80	678.0
133.80	151.0
134.80	709.0
135.90	177.0
136.90	557.0
138.70	213.0
139.80	288.0
140.90	4319.0
141.80	455.0
142.90	6396.0
143.80	460.0
144.80	2073.0
145.80	563.0
146.90	235.0
147.80	732.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

148.80	178.0
149.90	274.0
151.90	169.0
152.90	264.0
153.90	223.0
154.80	1250.0
156.10	174.0
156.90	520.0
158.90	551.0
160.80	360.0
171.00	827.0
171.90	4082.0
173.90	299328.0
174.90	21952.0
175.90	285568.0
176.90	18768.0
177.80	423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.90	3162.0
37.00	15994.0
38.00	15333.0
39.00	6529.0
40.00	642.0
42.70	183.0
43.90	2474.0
44.90	2919.0
45.90	464.0
47.00	4946.0
47.90	2207.0
48.90	15479.0
49.90	71144.0
50.90	21944.0
51.80	764.0
52.90	422.0
54.10	196.0
54.90	1051.0
55.90	5705.0
57.00	10343.0
57.80	368.0
59.90	3528.0
60.90	18024.0
61.90	18888.0
63.00	15970.0
63.90	2412.0
64.90	3648.0
65.80	328.0
67.00	1060.0
67.90	40136.0
68.90	40040.0
69.90	2876.0
70.90	157.0
72.00	2216.0
72.90	17672.0
73.90	68208.0
75.00	211392.0
76.00	18088.0
77.00	2485.0
77.80	1800.0
78.80	14276.0
79.80	3636.0
80.80	15105.0
81.90	3480.0
82.80	343.0
85.80	687.0
86.90	16366.0
87.90	16245.0
90.80	1605.0
91.90	11869.0
93.00	18600.0
94.00	47520.0
95.00	412416.0
96.00	26648.0
96.90	656.0
102.90	195.0
103.80	1710.0
104.80	575.0
105.90	1653.0
106.80	418.0
108.00	122.0
109.60	202.0
110.10	212.0
110.70	287.0
111.70	203.0
112.90	352.0
114.90	535.0
115.80	1548.0
116.90	3244.0
117.90	1692.0
118.90	2873.0
123.70	212.0
125.80	159.0
126.70	204.0
127.90	1423.0
128.90	836.0
129.90	1885.0
130.80	739.0
133.80	179.0
134.80	724.0
136.00	200.0
136.90	618.0
138.60	114.0
139.10	108.0
139.80	233.0
140.90	4627.0
141.80	455.0
142.90	6348.0
143.80	439.0
144.80	1922.0
145.90	608.0
146.90	266.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

147.80	877.0
148.90	241.0
149.90	305.0
151.90	174.0
152.80	275.0
153.90	214.0
154.80	1129.0
156.00	174.0
157.00	544.0
158.90	578.0
160.70	399.0
171.00	761.0
171.90	3785.0
173.00	3389.0
173.90	309632.0
174.90	23176.0
175.90	294848.0
176.90	19176.0
177.90	386.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.80	2760.0
37.00	14908.0
38.00	14253.0
39.00	5806.0
40.00	537.0
42.70	106.0
43.90	2117.0
44.90	2662.0
45.90	439.0
47.00	4486.0
47.90	1928.0
48.90	13792.0
49.90	63352.0
50.90	19392.0
51.90	715.0
52.90	387.0
54.10	224.0
54.90	997.0
55.90	5137.0
57.00	8813.0
57.90	313.0
59.90	3135.0
60.90	15963.0
61.90	17424.0
62.90	14379.0
64.00	2083.0
64.90	3273.0
65.80	289.0
66.90	882.0
67.90	36296.0
69.00	36104.0
70.00	2401.0
70.90	126.0
72.00	2124.0
72.90	16164.0
74.00	62424.0
75.00	191680.0
76.00	16105.0
76.90	2282.0
77.90	1596.0
78.80	12811.0
79.80	3434.0
80.90	13425.0
81.90	2870.0
82.80	282.0
85.80	641.0
86.90	14841.0
87.90	15132.0
90.80	1541.0
91.90	10529.0
93.00	17224.0
94.00	42984.0
95.00	377280.0
96.00	24496.0
96.90	600.0
102.90	105.0
103.80	1732.0
104.80	501.0
105.90	1541.0
106.90	374.0
109.60	145.0
110.10	240.0
110.90	284.0
111.70	165.0
112.90	346.0
114.80	519.0
115.80	1424.0
116.80	2924.0
117.90	1473.0
118.90	2532.0
123.70	228.0
124.70	103.0
125.70	158.0
126.70	133.0
127.90	1350.0
128.90	750.0
129.90	1820.0
130.80	682.0
133.80	160.0
134.80	676.0
136.00	153.0
136.90	634.0
139.10	176.0
139.80	199.0
140.90	4327.0
141.80	391.0
142.90	5725.0
143.90	332.0
144.80	1760.0
145.90	697.0
146.90	269.0
147.80	927.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

148.90	272.0
149.90	350.0
151.80	151.0
152.80	225.0
153.80	209.0
154.80	944.0
155.80	170.0
157.00	546.0
158.90	548.0
160.70	438.0
170.90	646.0
171.90	3258.0
173.00	3264.0
173.90	288640.0
174.90	21856.0
175.90	275840.0
176.90	17704.0
178.00	405.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096