

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121918\
 Data File : VU028785.D
 Acq On : 19 Dec 2018 11:43
 Operator : MD/SY
 Sample : J6474-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 S49-TB-2018-1

Quant Time: Dec 20 05:54:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 07 00:39:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	128025	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	218353	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	195795	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	79712	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.31	65	84176	43.08	ug/l	0.00
Spiked Amount			Recovery	=	86.16%	
35) Dibromofluoromethane	4.88	113	71292	51.88	ug/l	0.00
Spiked Amount			Recovery	=	103.76%	
50) Toluene-d8	7.57	98	276977	50.95	ug/l	0.00
Spiked Amount			Recovery	=	101.90%	
62) 4-Bromofluorobenzene	10.30	95	88801	43.71	ug/l	0.00
Spiked Amount			Recovery	=	87.42%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121918\
Data File : VU028785.D
Acq On : 19 Dec 2018 11:43
Operator : MD/SY
Sample : J6474-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
S49-TB-2018-1

Quant Time: Dec 20 05:54:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 07 00:39:42 2018
Response via : Initial Calibration

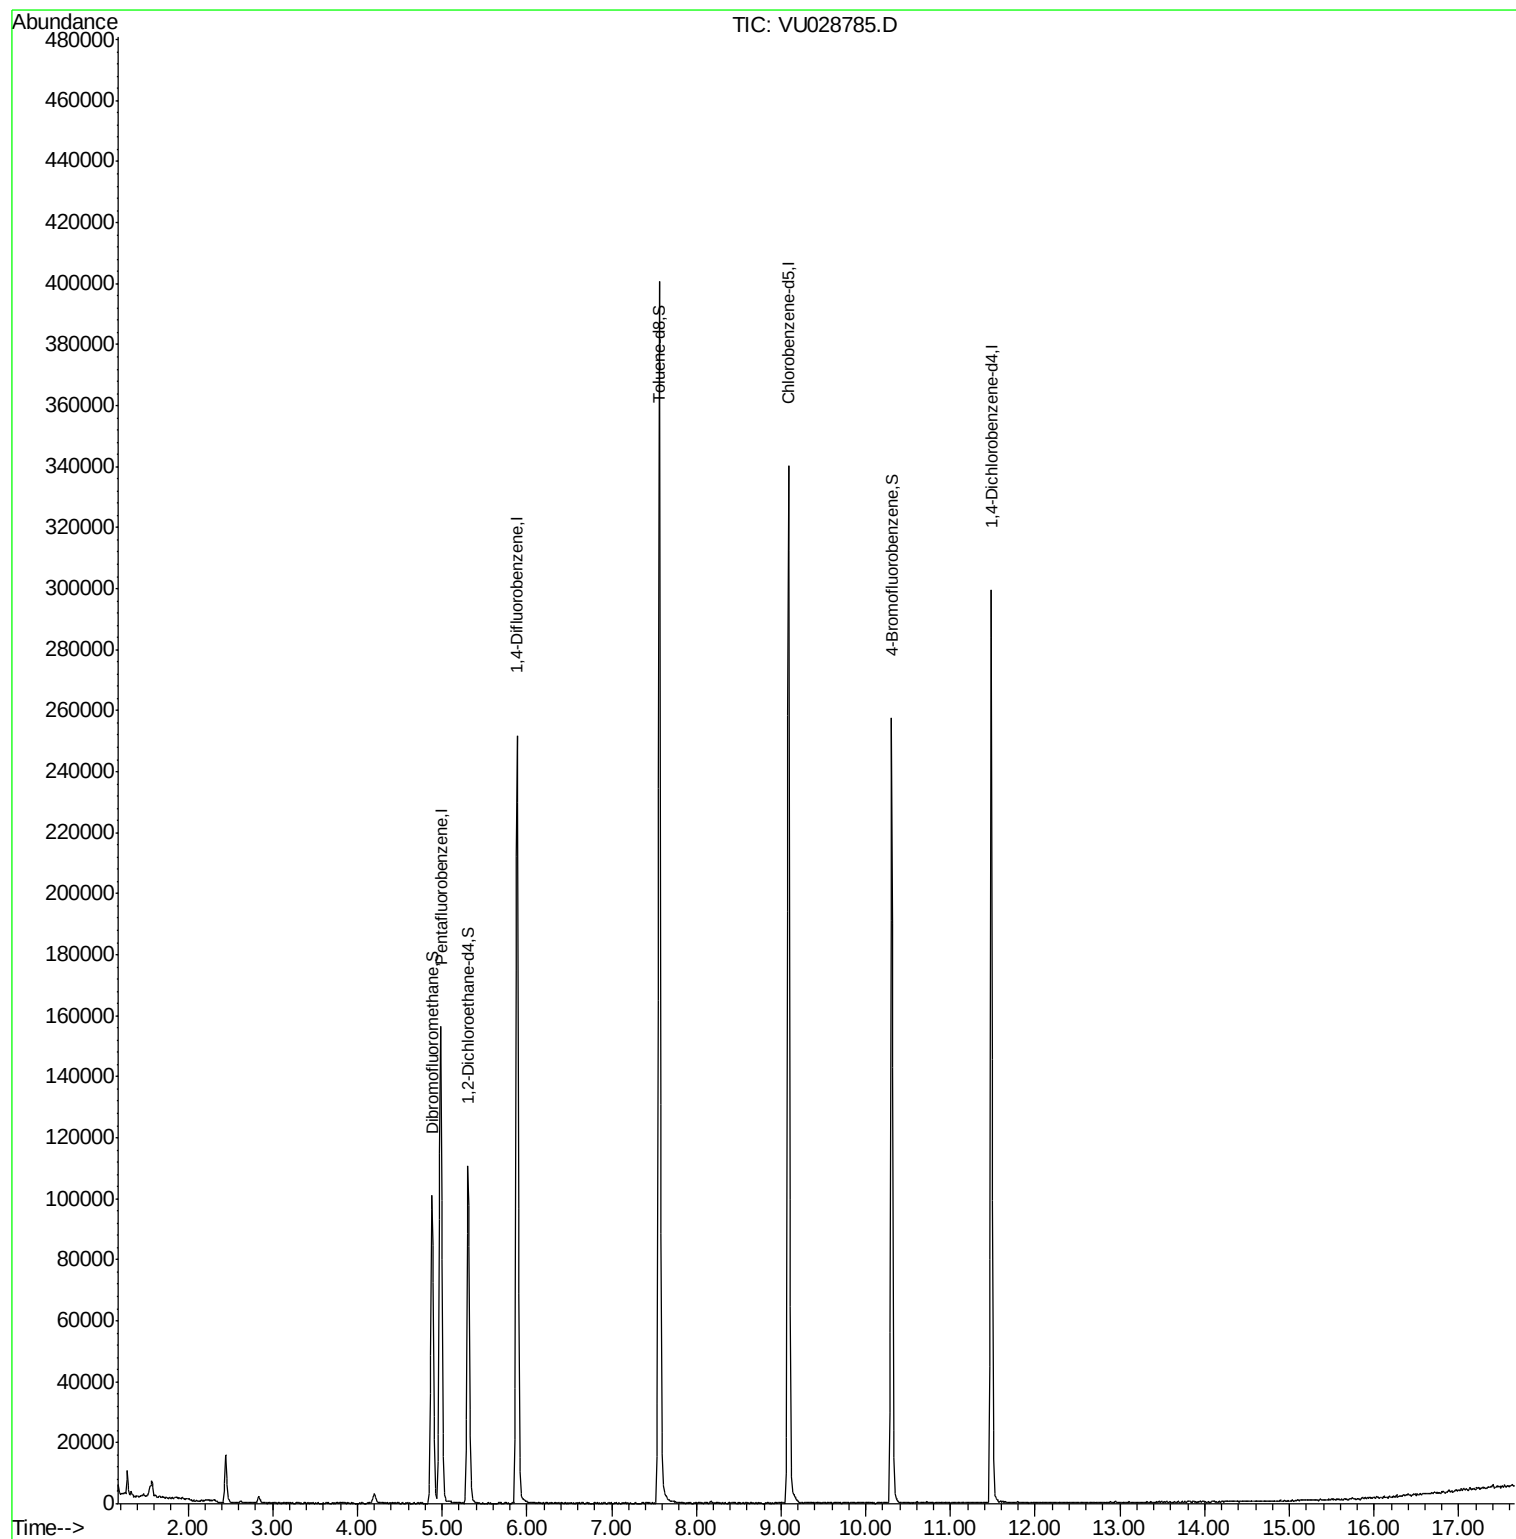

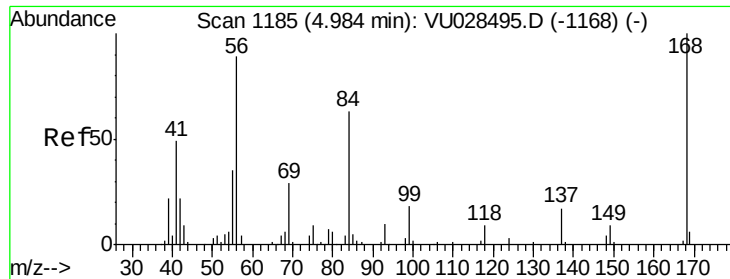

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1184

Delta R.T. -0.00 min

Lab File: VU028785.D

Acq: 19 Dec 2018 11:43


Instrument :
MSVOA_U
ClientSampleId :
S49-TB-2018-1

Tot Ion:168 Resp: 128025

Ion Ratio Lower Upper

168 100

99 51.3 46.6 69.8

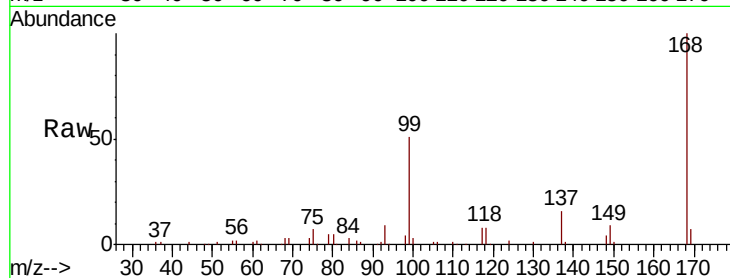

Abundance Ion 167.90 (167.60 to 168.60): VU028495.D (-1168) (-)

Ion 98.90 (98.60 to 99.60): VU028495.D (-1168) (-)

4.98

60000



40000

20000

0

4.90 5.00 5.10

Time-->

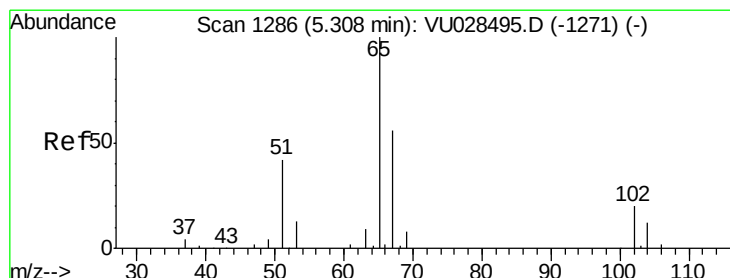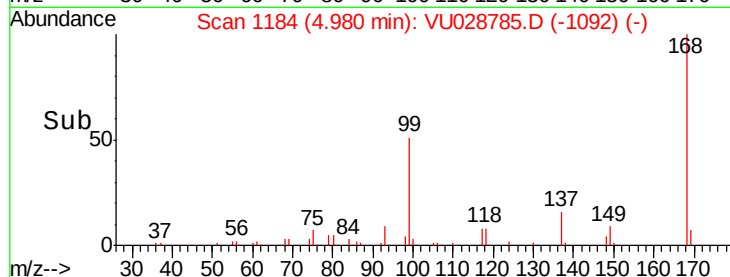

#33

1,2-Dichloroethane-d4

Concen: 43.084 ug/l

RT: 5.31 min Scan# 1286

Delta R.T. -0.00 min

Lab File: VU028785.D


Acq: 19 Dec 2018 11:43

Tgt Ion: 65 Resp: 84176

Ion Ratio Lower Upper

65 100

67 54.8 0.0 110.6

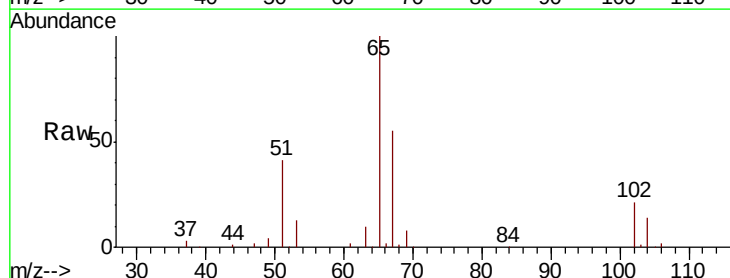

Abundance Ion 64.90 (64.60 to 65.60): VU028495.D (-1271) (-)

Ion 66.90 (66.60 to 67.60): VU028495.D (-1271) (-)

5.31

40000

30000


20000


10000

0

5.20 5.25 5.30 5.35 5.40

Time-->

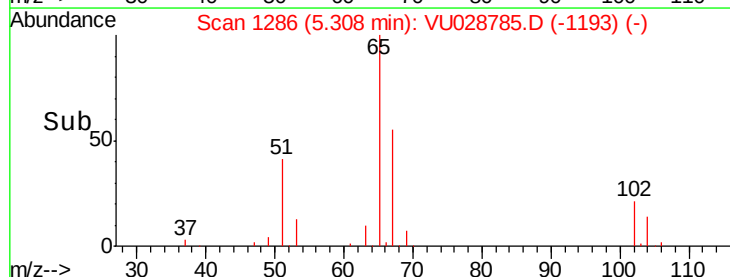


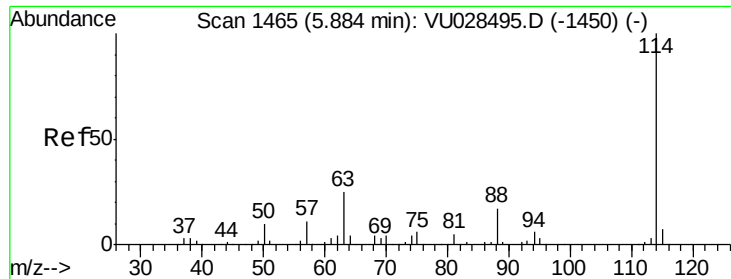




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.88 min Scan# 1465
 Delta R.T. -0.00 min
 Lab File: VU028785.D
 Acq: 19 Dec 2018 11:43

Instrument :
 MSVOA_U
 ClientSampleId :
 S49-TB-2018-1

Tot Ion	Ratio	Lower	Upper
114	100		
63	21.1	0.0	49.2
88	15.7	0.0	33.4

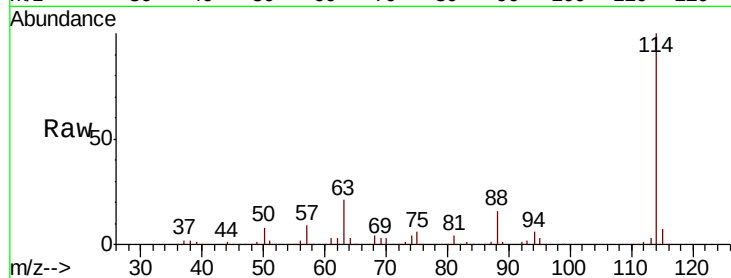


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VU0
 Ion 87.90 (87.60 to 88.60): VU0

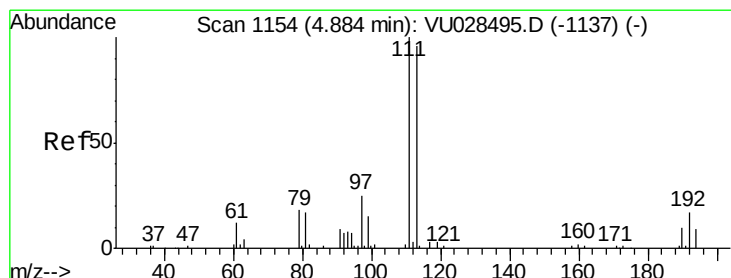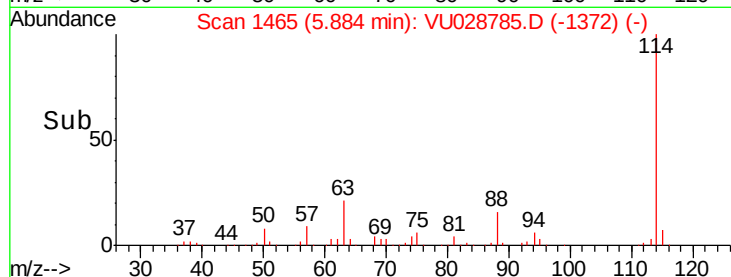
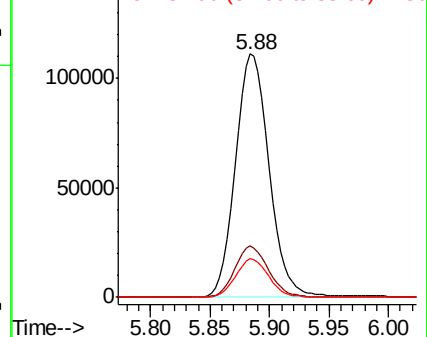



#35
 Dibromofluoromethane
 Concen: 51.882 ug/l
 RT: 4.88 min Scan# 1153
 Delta R.T. -0.00 min
 Lab File: VU028785.D
 Acq: 19 Dec 2018 11:43

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.0	83.4	125.0
192	20.5	14.8	22.2

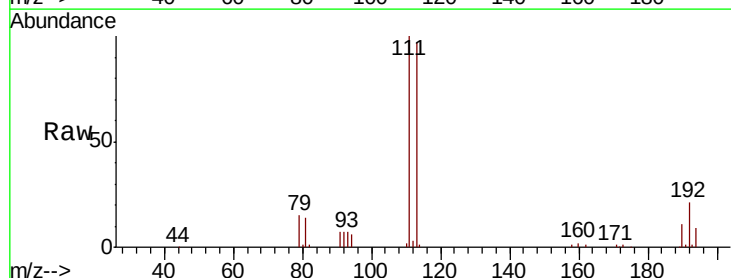

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

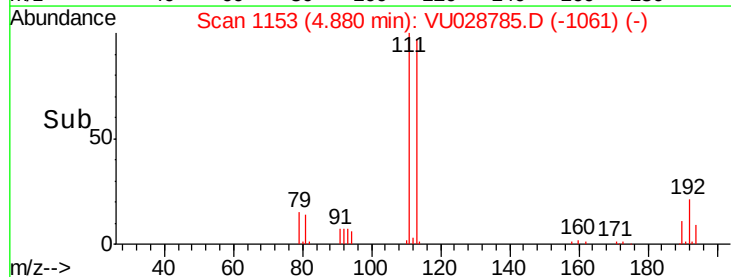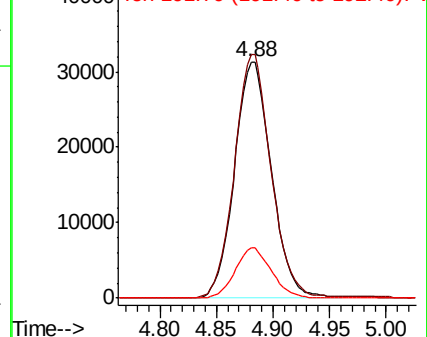

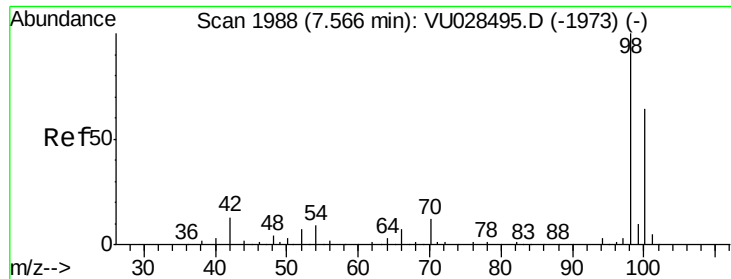

#50

Toluene-d8

Concen: 50.955 ug/l

RT: 7.57 min Scan# 1988

Delta R.T. -0.00 min

Lab File: VU028785.D

Acq: 19 Dec 2018 11:43

Instrument :

MSVOA_U

ClientSampleId :


S49-TB-2018-1

Tot Ion: 98 Resp: 276977

Ion Ratio Lower Upper

98 100

100 63.3 51.0 76.6

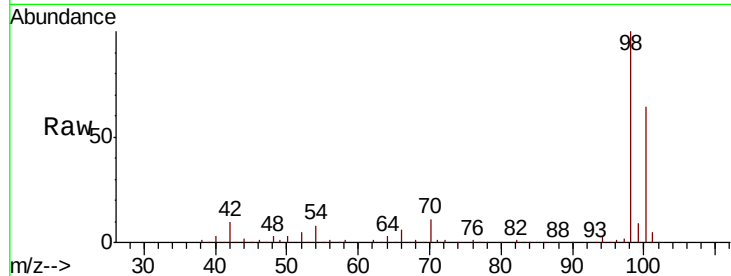

Abundance Ion 98.00 (97.70 to 98.70): VU028495.D (-1973) (-)

Ion 100.00 (99.70 to 100.70): VU028495.D (-1973) (-)

7.57

150000



100000

50000

0

7.50 7.60 7.70

Time-->

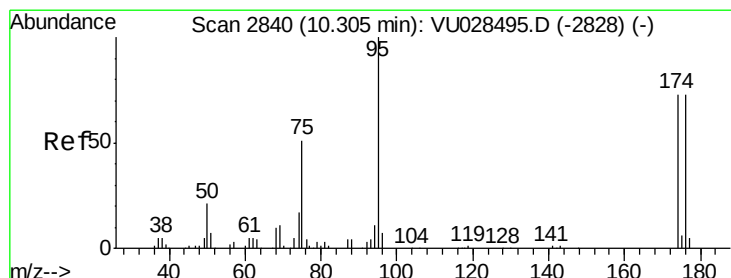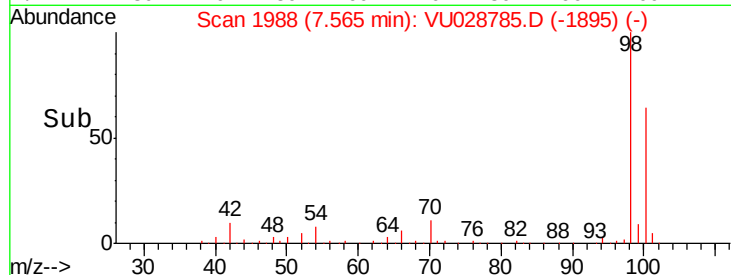

#62

4-Bromofluorobenzene

Concen: 43.708 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.00 min

Lab File: VU028785.D

Acq: 19 Dec 2018 11:43


Tgt Ion: 95 Resp: 88801

Ion Ratio Lower Upper

95 100

174 81.1 0.0 150.4

176 79.2 0.0 145.2

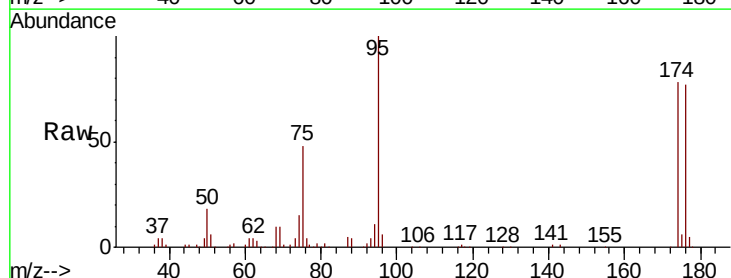

Abundance Ion 94.90 (94.60 to 95.60): VU028495.D (-2828) (-)

Ion 173.80 (173.50 to 174.50): VU028495.D (-2828) (-)

Ion 175.80 (175.50 to 176.50): VU028495.D (-2828) (-)

10.30

60000


40000


20000

0

10.20 10.30 10.40

Time-->

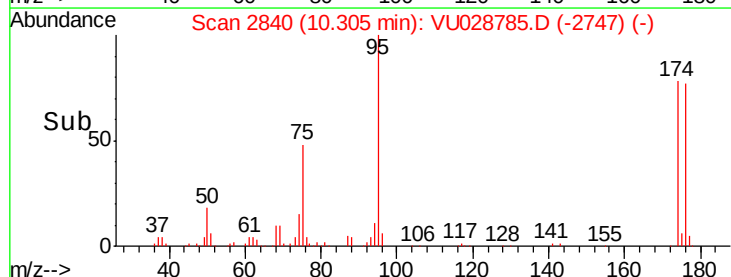


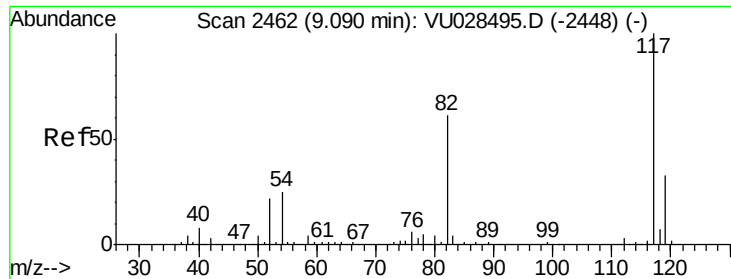




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2462
Delta R.T. -0.00 min
Lab File: VU028785.D
Acq: 19 Dec 2018 11:43

Instrument :
MSVOA_U
ClientSampleId :
S49-TB-2018-1

Tot Ion:117 Resp: 195795
Ion Ratio Lower Upper
117 100
82 56.2 48.9 73.3
119 32.6 26.2 39.4

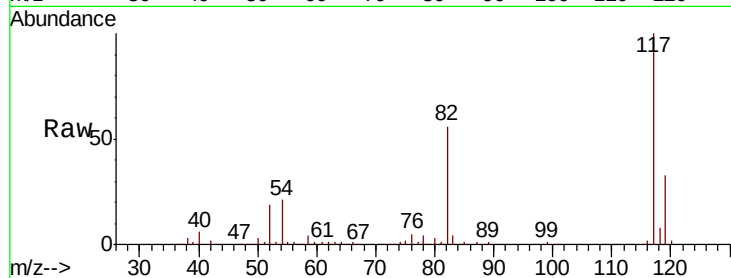


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VU0
Ion 118.90 (118.60 to 119.60): V

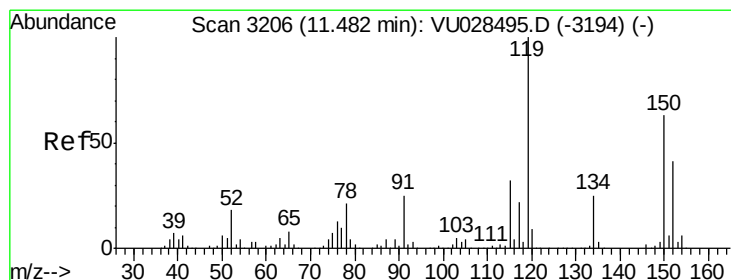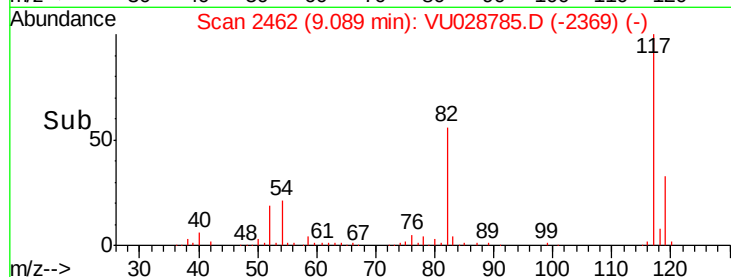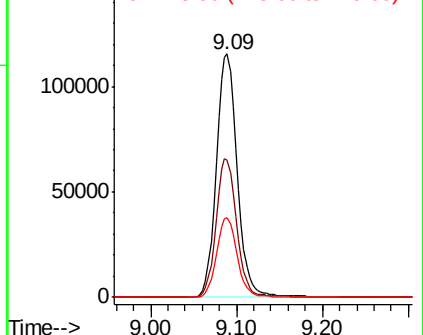

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3206
Delta R.T. -0.00 min
Lab File: VU028785.D
Acq: 19 Dec 2018 11:43

Tgt Ion:152 Resp: 79712
Ion Ratio Lower Upper
152 100
115 58.2 42.7 128.1
150 155.4 0.0 346.0

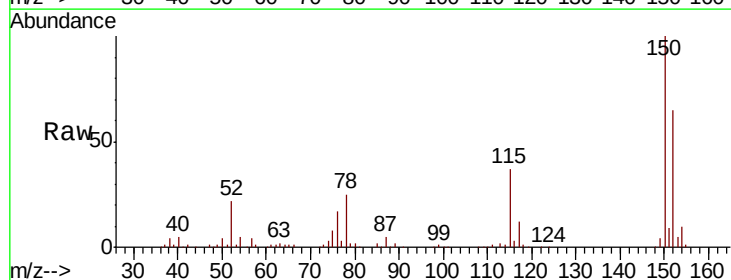

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

