




Data File : VU036300.D
Acq On : 19 Dec 2019 22:31
Operator : JC/MD
Sample : K6282-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDX3

Manual Integrations
APPROVED

apatel
12/20/2019 1:05:47 PM

Quant Time: Dec 20 06:06:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 20 05:33:55 2019
Response via : Initial Calibration

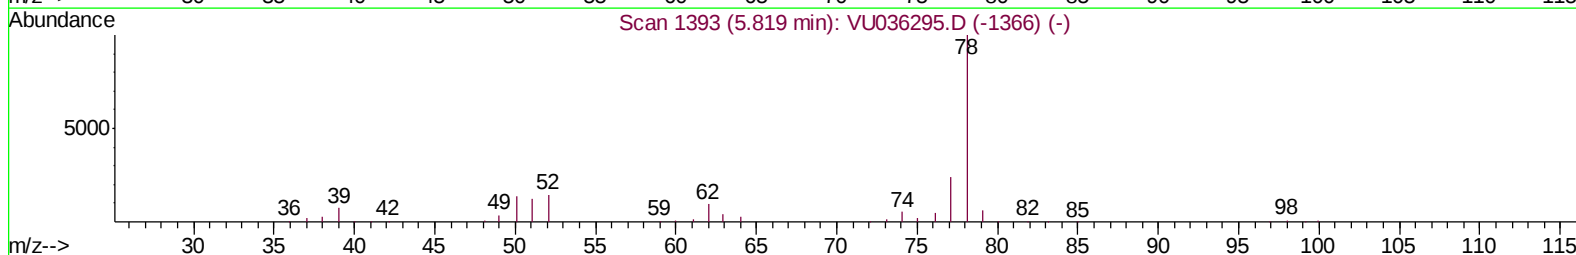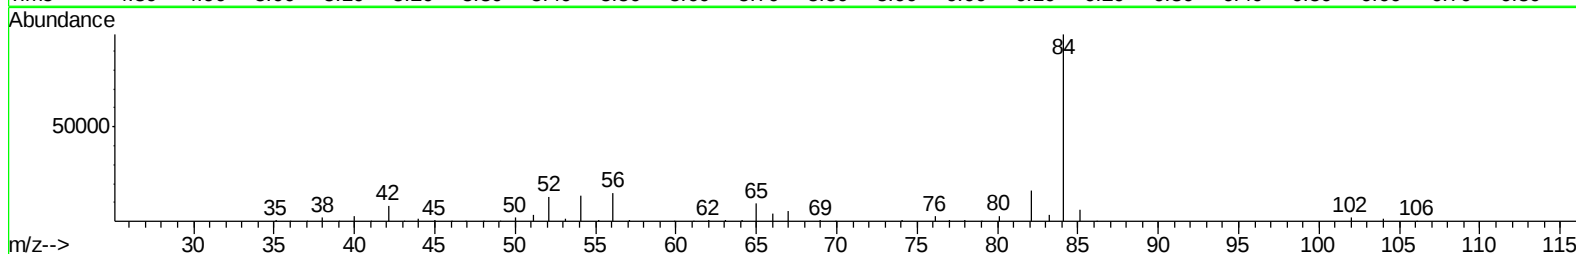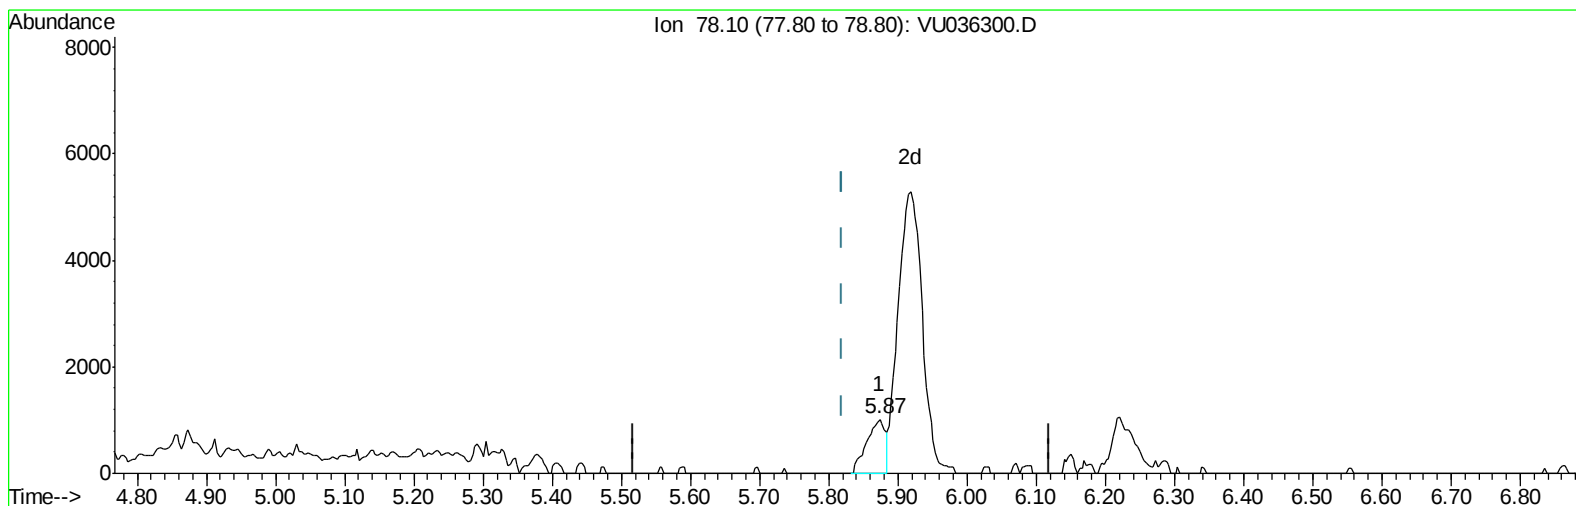

TIC: VU036300.D

(33) Benzene (T)

5.874min (+0.055) 0.03ug/L

response 1891

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VU036300.D
Acq On : 19 Dec 2019 22:31
Operator : JC/MD
Sample : K6282-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDX3

Manual Integrations
APPROVED

apatel
12/20/2019 1:05:47 PM

Quant Time: Dec 20 06:06:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 20 05:33:55 2019
Response via : Initial Calibration

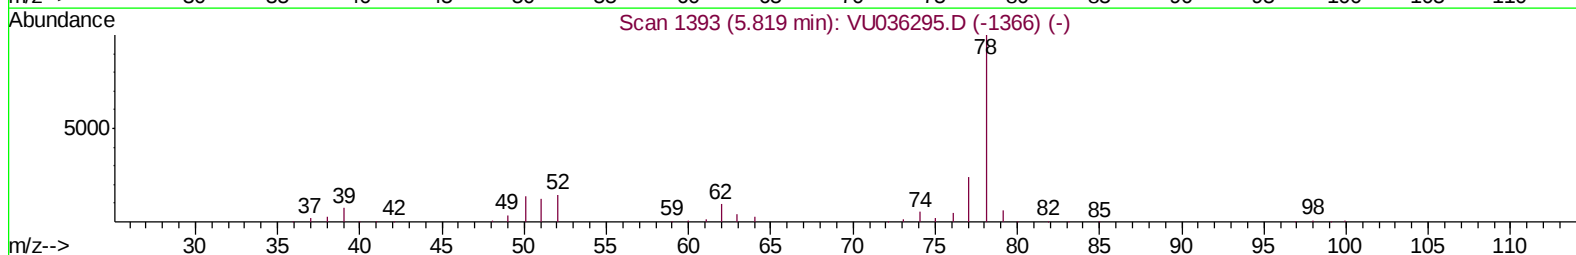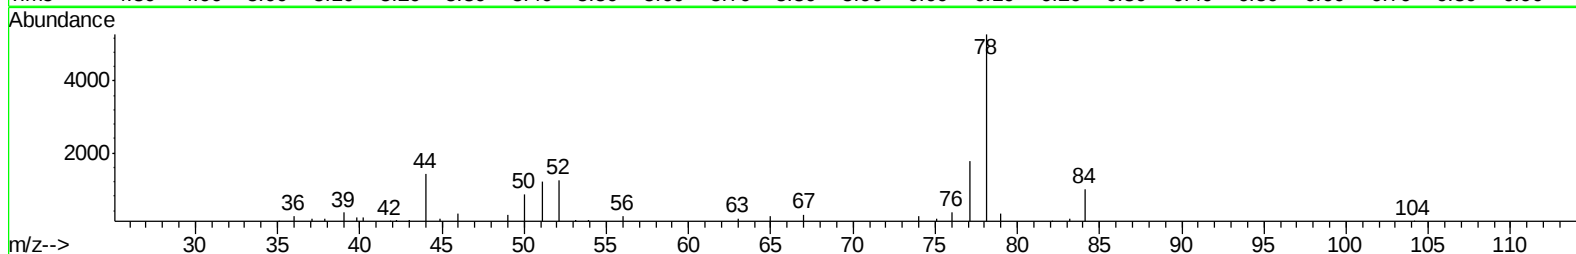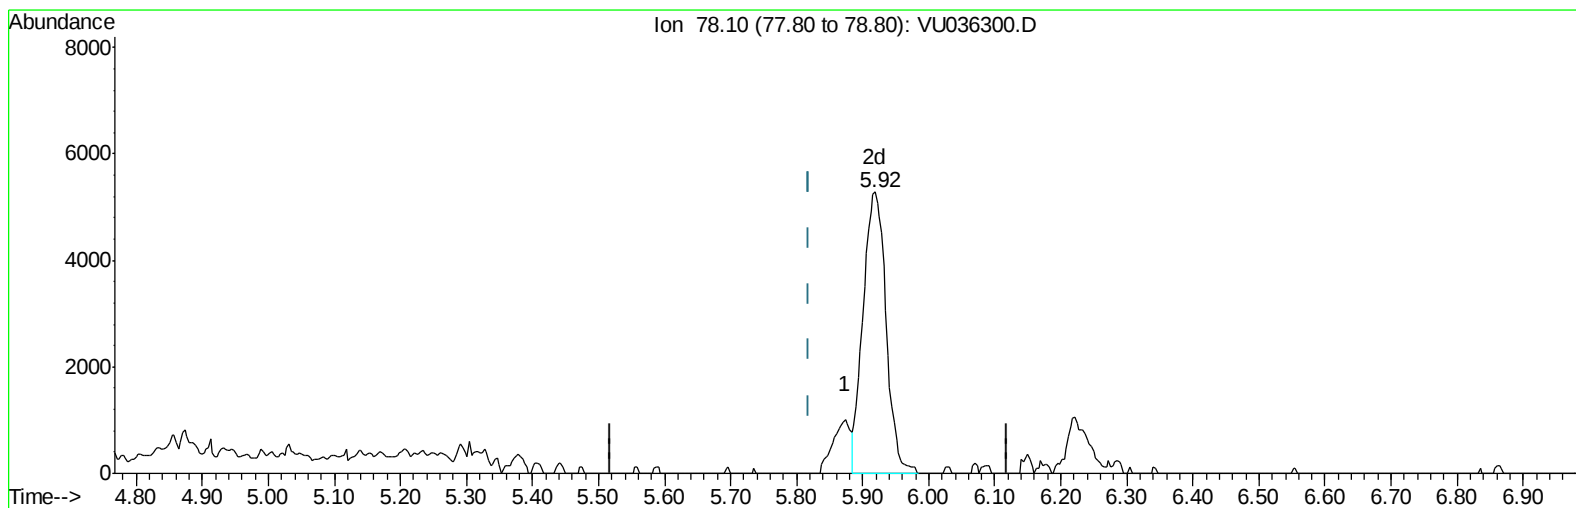

TIC: VU036300.D

(33) Benzene (T)

5.919min (+0.100) 0.19ug/L m

response 12820

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VU036300.D
Acq On : 19 Dec 2019 22:31
Operator : JC/MD
Sample : K6282-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDX3

Manual Integrations
APPROVED

apatel
12/20/2019 1:05:47 PM

Quant Time: Dec 20 06:09:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 20 05:33:55 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.39	114	186132	5.00	ug/L	0.10
28) Chlorobenzene-d5	9.47	117	223323	5.00	ug/L	0.03
60) 1,4-Dichlorobenzene-d4	11.84	152	109459	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.69	65	103597	6.32	ug/L	0.08
Spiked Amount	5.000	Range	40 - 130	Recovery	=	126.40%
7) Chloroethane-d5	2.03	69	91247	6.21	ug/L	0.10
Spiked Amount	5.000	Range	65 - 130	Recovery	=	124.20%
11) 1,1-Dichloroethene-d2	2.70	63	121041	5.12	ug/L	0.10
Spiked Amount	5.000	Range	60 - 125	Recovery	=	102.40%
20) 2-Butanone-d5	4.86	46	132789	43.24	ug/L	0.18
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.48%
24) Chloroform-d	5.19	84	164430	6.24	ug/L	0.08
Spiked Amount	5.000	Range	70 - 125	Recovery	=	124.80%
26) 1,2-Dichloroethane-d4	5.85	65	60202	4.35	ug/L	0.11
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
32) Benzene-d6	5.87	84	225774	4.02	ug/L	0.10
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.40%
36) 1,2-Dichloropropane-d6	6.82	67	71092	4.02	ug/L	0.09
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.40%
41) Toluene-d8	7.98	98	177099	3.35	ug/L	0.05
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.00%#
43) trans-1,3-Dichloropropene-	8.25	79	22731	3.12	ug/L	0.04
Spiked Amount	5.000	Range	55 - 130	Recovery	=	62.40%
46) 2-Hexanone-d5	8.71	63	79064	28.41	ug/L	0.04
Spiked Amount	50.000	Range	45 - 130	Recovery	=	56.82%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	77209	4.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.40%
64) 1,2-Dichlorobenzene-d4	12.22	152	90671	4.33	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.60%

Target Compounds					Qvalue
33) Benzene	5.92	78	12820m	0.187 ug/L	
34) Trichloroethene	6.67	95	10962	0.620 ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU036300.D
Acq On : 19 Dec 2019 22:31
Operator : JC/MD
Sample : K6282-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDX3

Manual Integrations
APPROVED

apatel
12/20/2019 1:05:47 PM

Quant Time: Dec 20 06:09:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 20 05:33:55 2019
Response via : Initial Calibration

