

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121919\
 Data File : VU036283.D
 Acq On : 19 Dec 2019 15:24
 Operator : JC/MD
 Sample : K6282-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFDTS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.617	78	86	97	rBV	168750	189510	22.03%	2.693%
2	1.935	177	185	199	rVB	150964	193233	22.46%	2.746%
3	2.597	378	391	405	rBV	196805	324436	37.71%	4.610%
4	4.684	1023	1040	1079	rBV3	109286	323342	37.58%	4.595%
5	5.115	1157	1174	1194	rBV2	169147	403711	46.92%	5.737%
6	5.771	1355	1378	1399	rBV3	326308	860391	100.00%	12.227%
7	6.292	1525	1540	1559	rBV	286900	558147	64.87%	7.932%
8	6.732	1662	1677	1700	rBV	207125	412480	47.94%	5.862%
9	7.600	1934	1947	1972	rBV	90679	174156	20.24%	2.475%
10	7.932	2034	2050	2065	rBV	348247	627607	72.94%	8.919%
11	8.006	2065	2073	2082	rVB2	16342	31269	3.63%	0.444%
12	8.215	2126	2138	2156	rBV2	59581	112772	13.11%	1.603%
13	8.684	2267	2284	2322	rBV	261593	785001	91.24%	11.155%
14	8.832	2323	2330	2338	rVB8	5247	10359	1.20%	0.147%
15	9.446	2508	2521	2562	rVB	422966	779544	90.60%	11.078%
16	10.124	2721	2732	2747	rVB7	6780	15133	1.76%	0.215%
17	10.784	2925	2937	2955	rVB	167191	286505	33.30%	4.071%
18	10.919	2969	2979	2990	rBV4	5694	10580	1.23%	0.150%
19	11.838	3253	3265	3281	rVB	277140	483868	56.24%	6.876%
20	12.218	3366	3383	3400	rBV	270562	455024	52.89%	6.466%


Sum of corrected areas: 7037068

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121919\
Data File : VU036283.D
Acq On : 19 Dec 2019 15:24
Operator : JC/MD
Sample : K6282-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDT8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

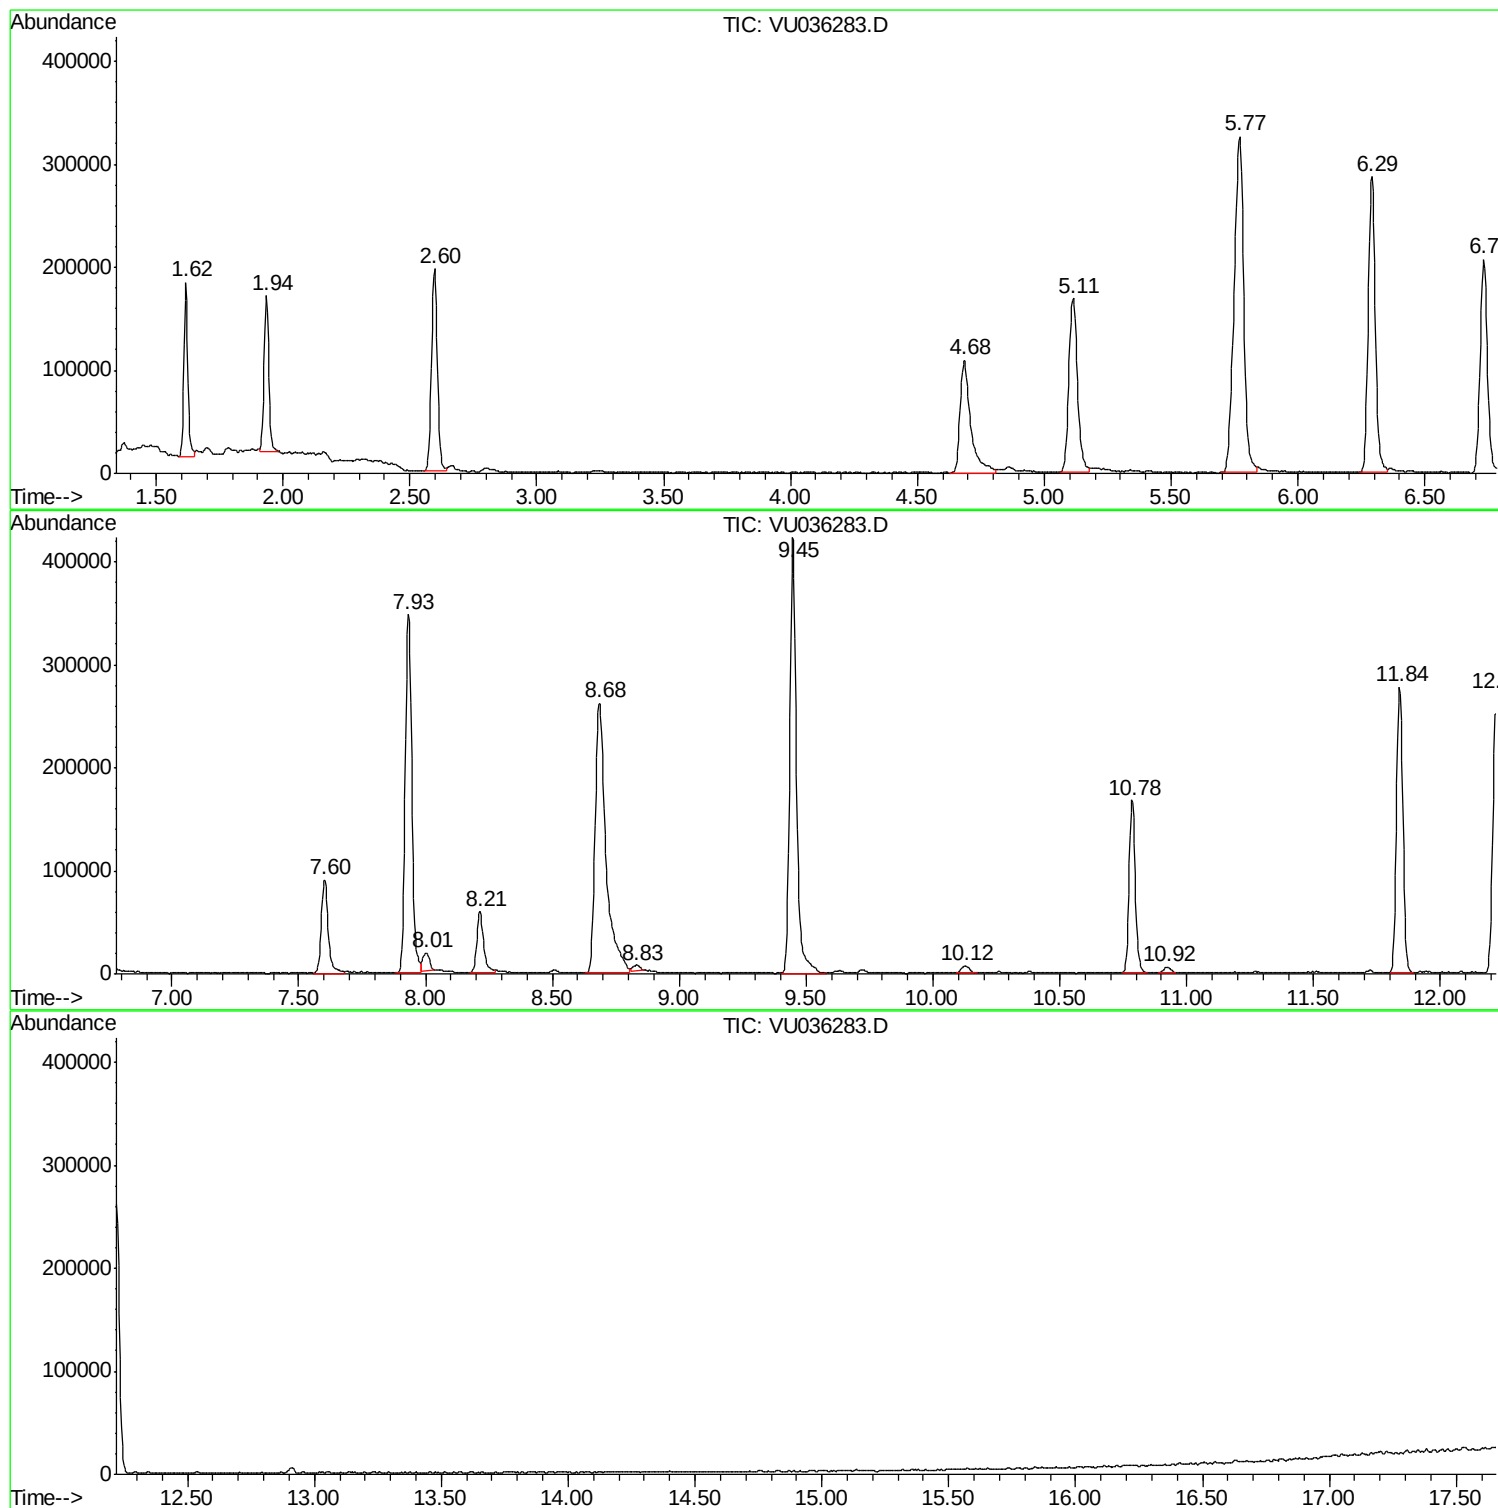

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU121919\
Data File : VU036283.D
Acq On : 19 Dec 2019 15:24
Operator : JC/MD
Sample : K6282-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDT8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU121919\
Data File : VU036283.D
Acq On : 19 Dec 2019 15:24
Operator : JC/MD
Sample : K6282-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDT8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc