


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121919\
 Data File : VU036278.D
 Acq On : 19 Dec 2019 08:45
 Operator : JC/MD
 Sample : BFB22
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB22

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 20 05:33:55 2019

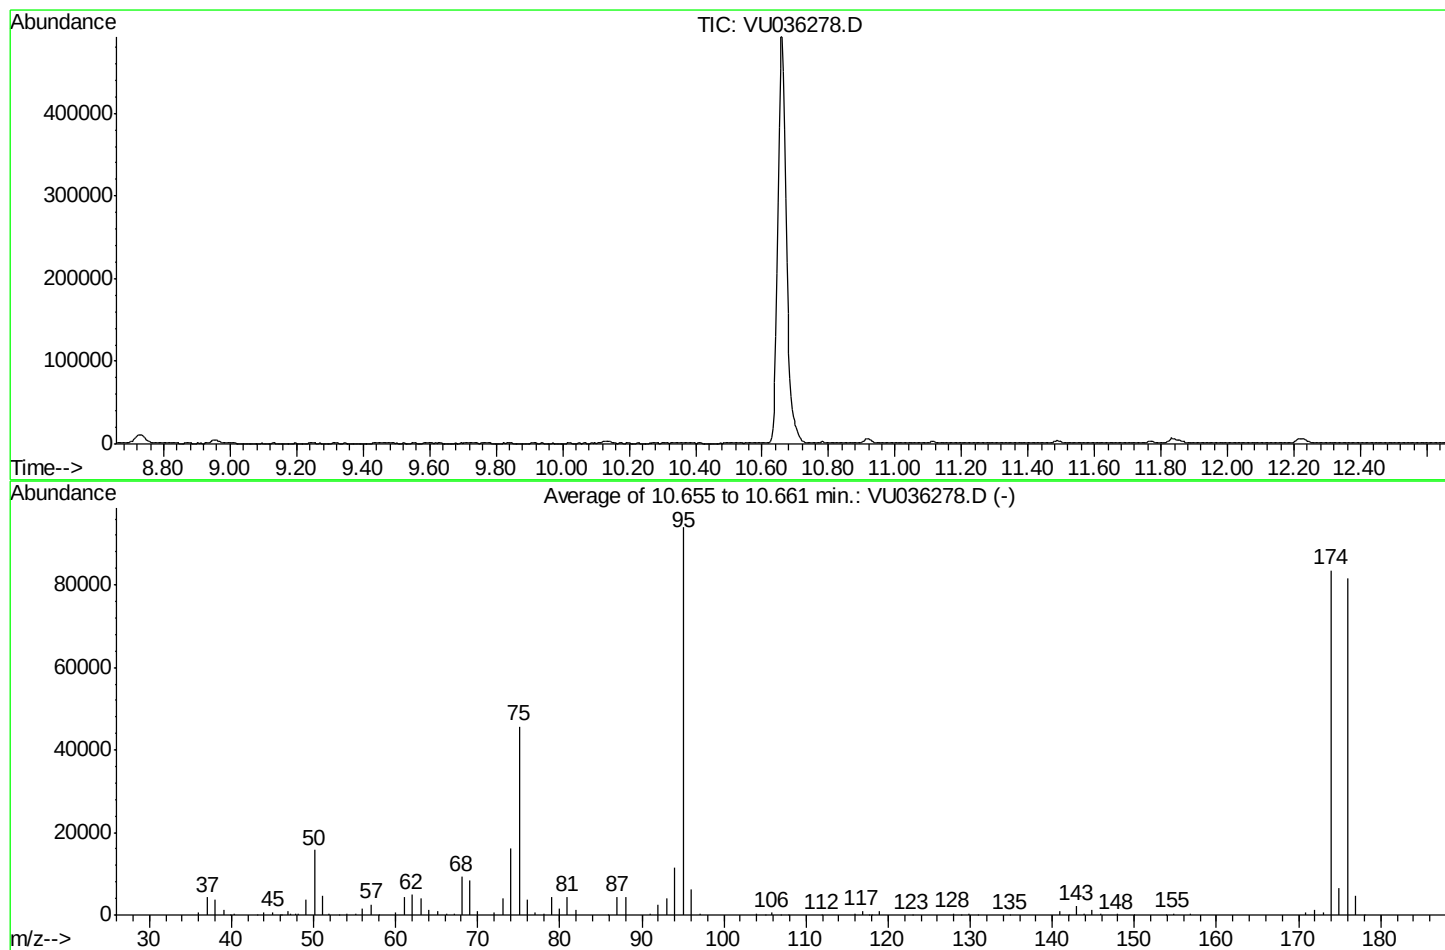

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	15703	PASS
75	95	30	80	48.7	45770	PASS
95	95	100	100	100.0	93960	PASS
96	95	5	9	6.6	6166	PASS
173	174	0.00	2	0.8	633	PASS
174	95	50	120	88.9	83488	PASS
175	174	5	9	7.7	6430	PASS
176	174	95	101	97.8	81640	PASS
177	176	5	9	5.9	4805	PASS

m/z	Abundance
36.00	884.0
37.10	4328.0
38.10	3528.0
39.10	1194.0
39.80	327.0
40.30	305.0
44.00	1156.0
45.10	599.0
45.90	137.0
46.80	782.0
47.20	708.0
47.90	504.0
49.00	3847.0
50.10	14891.0
51.10	4812.0
52.00	275.0
53.10	127.0
54.00	162.0
55.10	227.0
56.00	1817.0
57.10	2292.0
58.00	223.0
60.00	736.0
61.00	3979.0
62.00	4777.0
63.10	3637.0
64.00	1068.0
65.10	1041.0
66.20	169.0
68.00	8862.0
69.00	8155.0
70.00	966.0
72.00	415.0
73.00	3984.0
74.00	14809.0
75.10	43904.0
76.10	3764.0
76.90	591.0
78.10	530.0
79.00	4020.0
80.00	1500.0
81.00	4386.0
81.90	1093.0
87.00	4098.0
88.00	4098.0
91.10	358.0
92.00	2489.0
93.10	3631.0
94.10	10783.0
95.10	89824.0
96.00	5752.0
97.20	182.0
103.80	419.0
105.00	130.0
105.90	481.0
112.00	176.0
116.00	291.0
116.90	1023.0
118.00	247.0
118.90	818.0
128.00	375.0
129.00	132.0
129.90	276.0
130.80	174.0
134.80	134.0
140.90	828.0
142.10	142.0
143.00	1882.0
143.90	154.0
144.80	1095.0
145.90	340.0
147.80	302.0
153.90	124.0
154.70	336.0
156.80	193.0
170.90	626.0
171.90	1372.0
174.00	78288.0
175.00	6429.0
176.00	75304.0
177.00	4173.0
178.00	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	864.0
37.10	4414.0
38.00	3927.0
39.10	1253.0
39.80	333.0
40.30	390.0
44.00	1175.0
45.00	752.0
46.10	195.0
46.90	933.0
48.10	509.0
49.00	3742.0
50.10	16255.0
51.10	4946.0
51.90	303.0
53.10	117.0
54.10	194.0
55.10	242.0
56.00	1750.0
57.10	2600.0
58.00	168.0
60.00	777.0
61.00	4418.0
62.00	5141.0
63.10	4275.0
64.00	1204.0
65.10	1003.0
66.10	168.0
67.10	354.0
68.10	9463.0
69.00	8704.0
70.00	916.0
72.00	502.0
73.10	4138.0
74.00	16536.0
75.00	46960.0
76.10	4024.0
76.90	558.0
78.90	4386.0
80.00	1534.0
81.00	4597.0
81.90	1320.0
85.80	197.0
87.00	4542.0
88.00	4538.0
91.00	347.0
92.00	2715.0
93.00	4109.0
94.10	11756.0
95.10	96344.0
96.00	6314.0
97.20	169.0
103.90	426.0
105.00	158.0
105.90	573.0
111.90	158.0
116.00	275.0
116.90	1044.0
117.70	237.0
118.90	927.0
128.00	432.0
129.00	144.0
129.90	331.0
130.90	163.0
134.80	149.0
140.90	1021.0
142.00	174.0
143.00	2263.0
143.90	188.0
144.80	1196.0
145.90	350.0
147.80	287.0
149.90	169.0
154.80	394.0
156.80	241.0
170.90	610.0
171.90	1433.0
174.00	85544.0
175.00	6604.0
176.00	84208.0
177.00	4967.0
178.00	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	836.0
37.10	4185.0
38.00	3895.0
39.00	1392.0
39.80	298.0
40.30	318.0
43.10	109.0
44.00	1137.0
45.00	736.0
46.20	272.0
46.90	1091.0
48.10	514.0
49.00	3466.0
50.10	15965.0
51.10	4604.0
51.90	278.0
54.10	191.0
55.10	234.0
56.00	1438.0
57.00	2640.0
60.00	709.0
61.00	4345.0
62.00	4919.0
63.10	4382.0
64.00	1243.0
65.10	826.0
66.10	199.0
67.10	324.0
68.10	9177.0
69.00	8234.0
70.00	794.0
72.00	576.0
73.10	3838.0
74.00	16928.0
75.00	46448.0
76.10	3777.0
77.00	544.0
78.90	4406.0
80.00	1339.0
80.90	4426.0
81.90	1383.0
85.90	220.0
87.00	4431.0
88.00	4381.0
90.90	319.0
92.00	2710.0
93.00	4148.0
94.00	11985.0
95.10	95712.0
96.00	6433.0
97.00	188.0
104.00	417.0
105.00	171.0
105.90	561.0
106.90	106.0
107.90	159.0
111.90	152.0
115.90	262.0
116.90	950.0
117.70	226.0
118.80	959.0
122.90	110.0
127.90	465.0
128.90	122.0
129.90	414.0
131.00	143.0
134.90	134.0
140.90	1142.0
142.00	171.0
143.00	2499.0
143.90	169.0
144.90	1273.0
145.90	304.0
147.90	244.0
149.90	184.0
154.80	376.0
156.80	242.0
170.90	525.0
172.00	1307.0
173.00	1900.0
174.00	86632.0
174.90	6257.0
176.00	85408.0
177.00	5275.0
178.00	188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

Scan 2885 (10.616 min): VU036278.D
BFB22

m/z	Abundance
36.00	164.0
39.80	236.0
44.00	599.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22