

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
 Data File : VU046499.D
 Acq On : 19 Dec 2021 16:53
 Operator : SY/MD
 Sample : M5062-07ME
 Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL06ME

Quant Time: Dec 20 00:28:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Dec 20 00:25:10 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 12/20/2021
 Supervised By : Mahesh Dadoda 12/21/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	148216	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.430	117	160653	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.822	152	77979	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	42111	34.491	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.980%		
7) Chloroethane-d5	1.919	69	34108	36.385	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	72.780%		
11) 1,1-Dichloroethene-d2	2.562	63	60689	27.689	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.380%#		
21) 2-Butanone-d5	4.665	46	85376m	87.964	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.960%		
24) Chloroform-d	5.067	84	87877	43.101	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.200%		
26) 1,2-Dichloroethane-d4	5.703	65	61717	45.104	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.200%		
32) Benzene-d6	5.726	84	171704	37.290	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	74.580%		
36) 1,2-Dichloropropane-d6	6.690	67	54595	38.257	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	76.520%		
41) Toluene-d8	7.899	98	150128	35.809	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	71.620%#		
43) trans-1,3-Dichloroprop...	8.189	79	28379	41.196	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.400%		
47) 2-Hexanone-d5	8.694	63	63918	94.467	ug/L	0.06
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.470%		
56) 1,1,2,2-Tetrachloroeth...	10.777	84	90824	41.967	ug/L	0.02
Spiked Amount 50.000	Range 65 - 120		Recovery =	83.940%		
66) 1,2-Dichlorobenzene-d4	12.201	152	62978	41.937	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.880%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.575	96	20883	20.377	ug/L	84
15) Methyl Acetate	2.967	43	3175	2.245	ug/L	96
19) 1,1-Dichloroethane	3.867	63	159557	80.914	ug/L	98
22) 2-Butanone	4.745	43	10988m	8.321	ug/L	
30) 1,1,1-Trichloroethane	5.311	97	1372	0.696	ug/L #	72
34) Trichloroethene	6.543	95	47730	37.261	ug/L	97
46) Tetrachloroethene	8.555	164	50786	53.951	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
Data File : VU046499.D
Acq On : 19 Dec 2021 16:53
Operator : SY/MD
Sample : M5062-07ME
Misc : 6.07g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BGL06ME

Quant Time: Dec 20 00:28:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Dec 20 00:25:10 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : John Carlone 12/20/2021
Supervised By : Mahesh Dadoda 12/21/2021

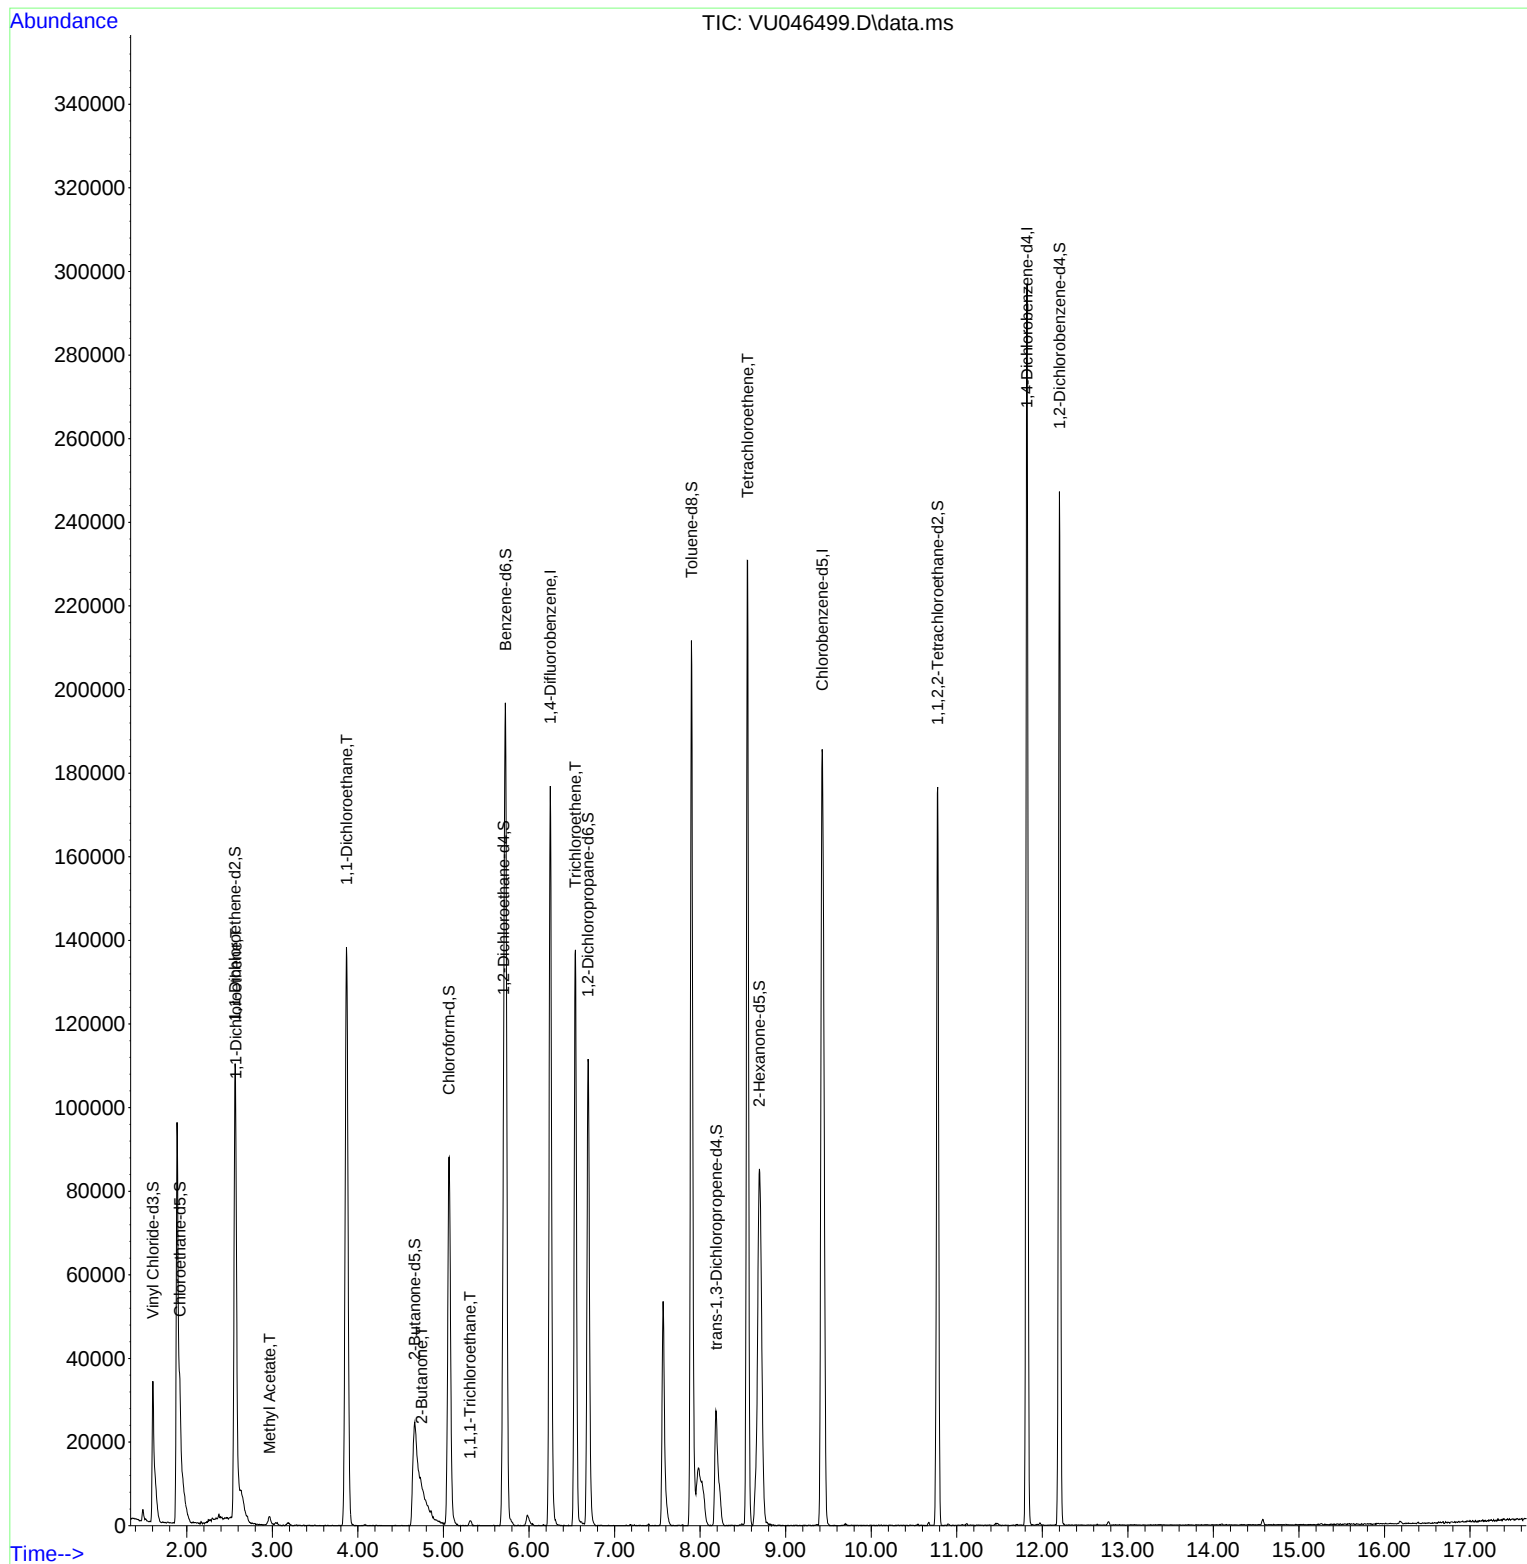

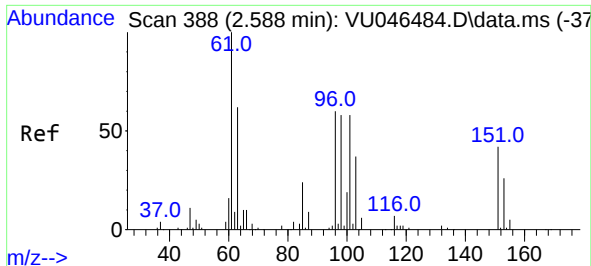

#12

1,1-Dichloroethene

Concen: 20.377 ug/L

RT: 2.575 min Scan# 31

Delta R.T. -0.013 min

Lab File: VU046499.D

Acq: 19 Dec 2021 16:53

Instrument :

MSVOA_U

ClientSampleId :

BGL06ME

Tgt Ion: 96 Resp: 2088





Ion	Ratio	Lower	Upper
96	100		
61	183.7	118.6	220.2
63	159.5	93.0	172.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 12/20/2021

Supervised By :Mahesh Dadoda 12/21/2021

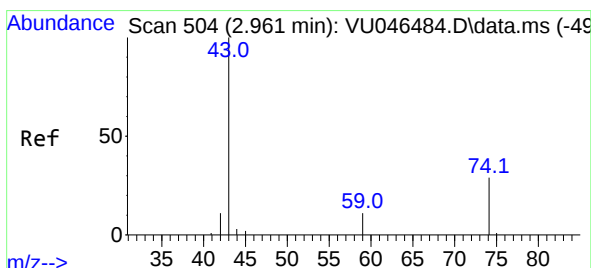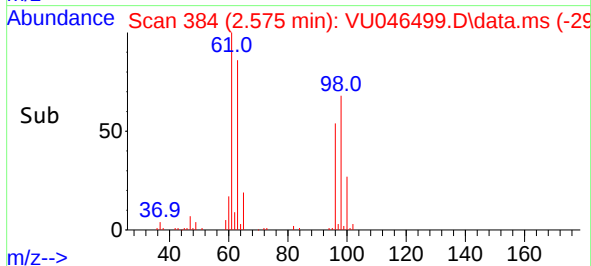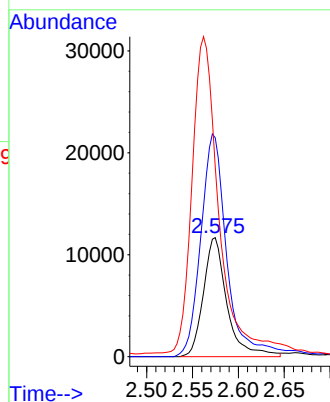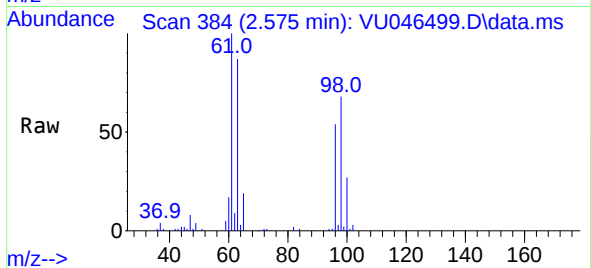

#15

Methyl Acetate

Concen: 2.245 ug/L

RT: 2.967 min Scan# 506




Delta R.T. 0.007 min


Lab File: VU046499.D

Acq: 19 Dec 2021 16:53

Tgt Ion: 43 Resp: 3175

Ion	Ratio	Lower	Upper
43	100		
74	24.1	20.8	31.2

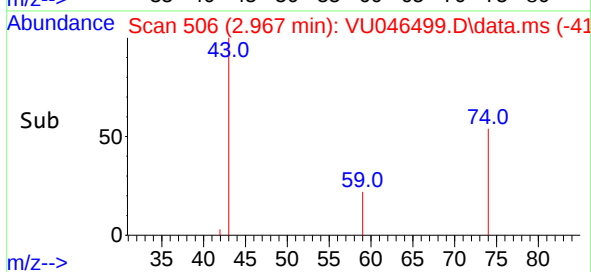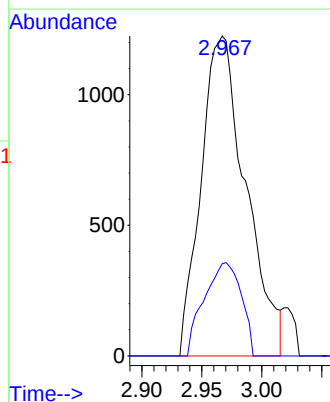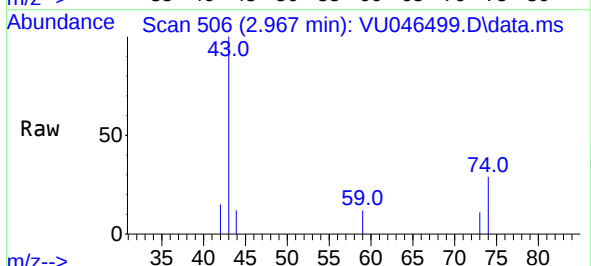

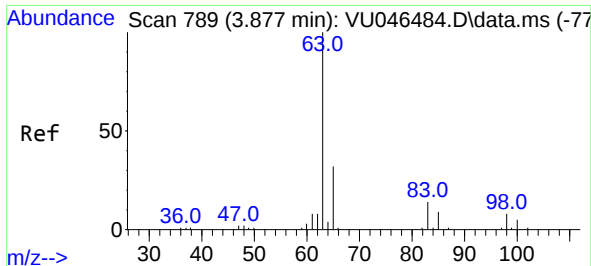

#19

1,1-Dichloroethane

Concen: 80.914 ug/L

RT: 3.867 min Scan# 71

Delta R.T. -0.009 min

Lab File: VU046499.D

Acq: 19 Dec 2021 16:53

Instrument :

MSVOA_U

ClientSampleId :

BGL06ME

Tgt Ion: 63 Resp: 15955

Ion Ratio Lower Upper

63 100

65 31.4 22.8 42.4





83 13.9 9.6 17.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 12/20/2021

Supervised By :Mahesh Dadoda 12/21/2021

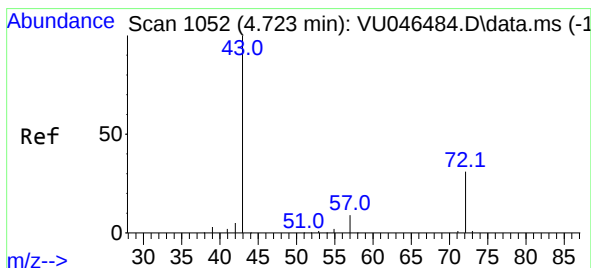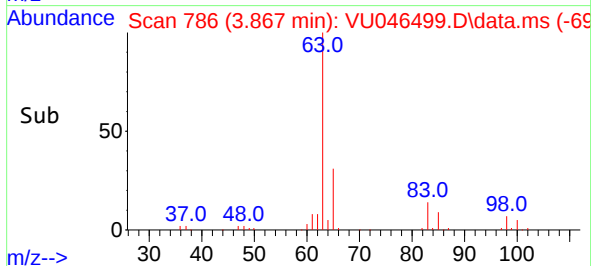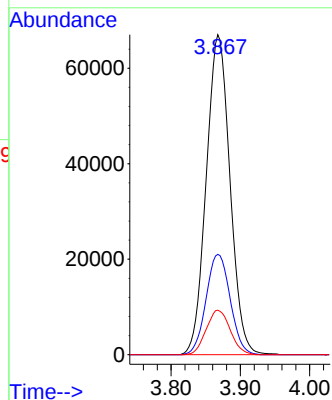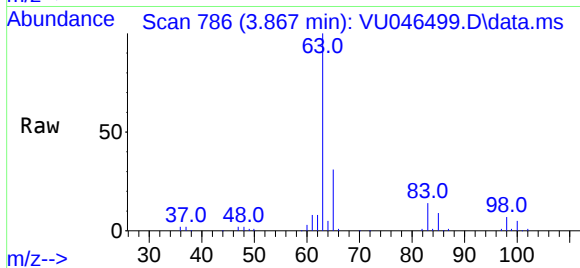

#22

2-Butanone

Concen: 8.321 ug/L m

RT: 4.745 min Scan# 1059

Delta R.T. 0.023 min

Lab File: VU046499.D




Acq: 19 Dec 2021 16:53


Tgt Ion: 43 Resp: 10988

Ion Ratio Lower Upper

43 100

72 6.5 14.5 43.6#

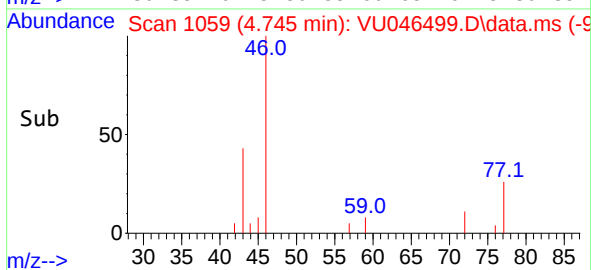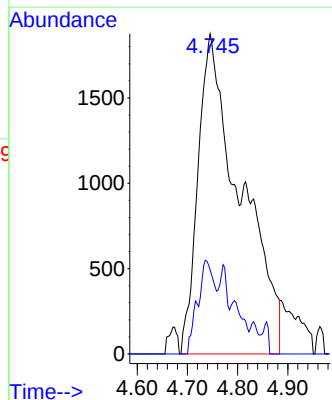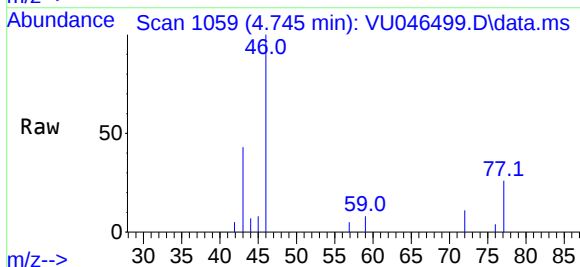

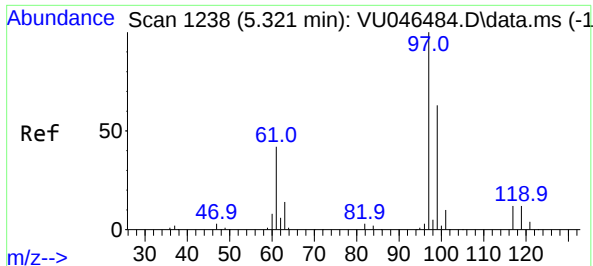

#30
1,1,1-Trichloroethane
Concen: 0.696 ug/L
RT: 5.311 min Scan# 1235
Delta R.T. -0.010 min
Lab File: VU046499.D
Acq: 19 Dec 2021 16:53





Instrument :
MSVOA_U
ClientSampleId :
BGL06ME

Tgt Ion: 97 Resp: 1372

Ion	Ratio	Lower	Upper
97	100		
99	48.7	51.8	77.6
61	18.3	34.4	51.6

Manual Integrations
APPROVED




Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/21/2021

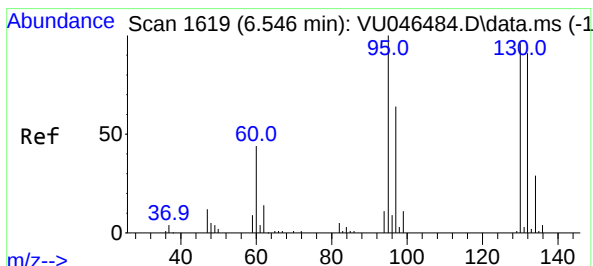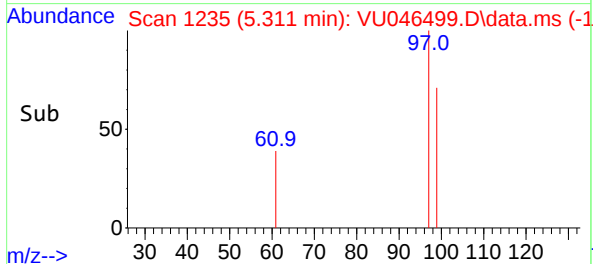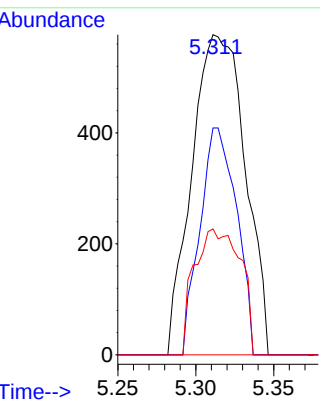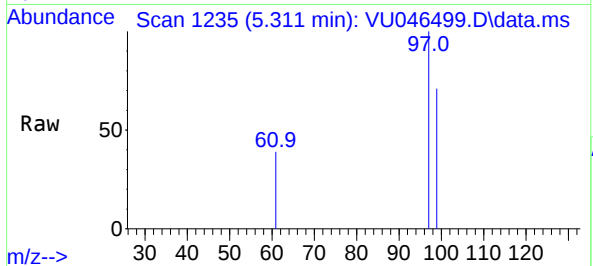


#34
Trichloroethene
Concen: 37.261 ug/L
RT: 6.543 min Scan# 1618
Delta R.T. -0.003 min
Lab File: VU046499.D
Acq: 19 Dec 2021 16:53

Tgt Ion: 95 Resp: 47730


Ion	Ratio	Lower	Upper
95	100		
97	61.8	44.1	81.9
132	92.5	66.8	124.0
130	93.9	69.0	128.1

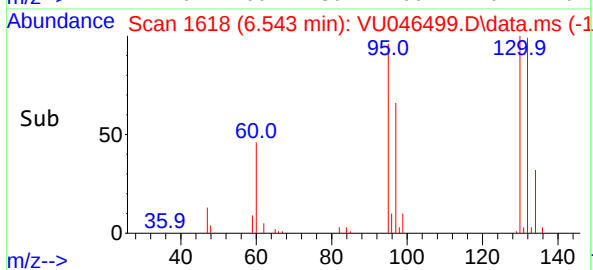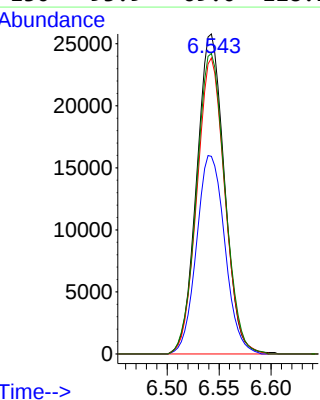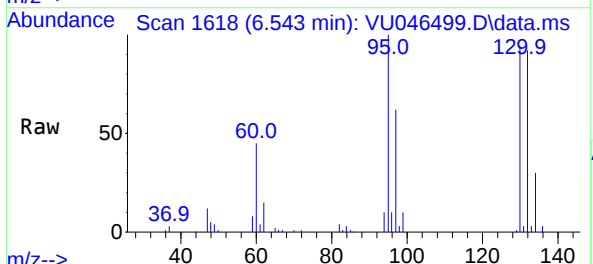

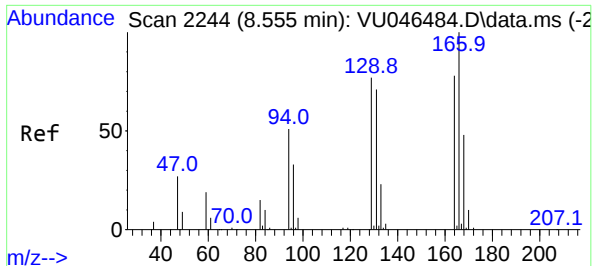

#46
Tetrachloroethene
Concen: 53.951 ug/L
RT: 8.555 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU046499.D
Acq: 19 Dec 2021 16:53

Instrument :
MSVOA_U
ClientSampleId :
BGL06ME

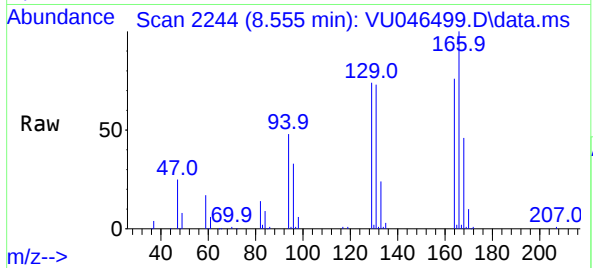

Tgt Ion:164 Resp: 50780
Ion Ratio Lower Upper
164 100
129 98.5 71.1 132.1
131 97.1 67.8 126.0
166 132.4 90.6 168.2

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/20/2021
Supervised By :Mahesh Dadoda 12/21/2021

