

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
 Data File : VU046497.D
 Acq On : 19 Dec 2021 16:08
 Operator : SY/MD
 Sample : M5066-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW142DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rBV	61757	75604	14.00%	1.646%
2	1.729	119	121	125	rVB	276	147	0.03%	0.003%
3	1.919	172	180	201	rBV	46640	66052	12.24%	1.438%
4	2.041	216	218	223	rBV	195	130	0.02%	0.003%
5	2.208	267	270	273	rBV	169	160	0.03%	0.003%
6	2.317	302	304	306	rBV	184	89	0.02%	0.002%
7	2.379	319	323	328	rBV2	263	183	0.03%	0.004%
8	2.417	332	335	343	rVB	235	211	0.04%	0.005%
9	2.575	372	384	400	rBV	108767	180520	33.44%	3.929%
10	2.739	432	435	438	rBB	175	142	0.03%	0.003%
11	2.761	439	442	445	rBB	132	118	0.02%	0.003%
12	2.819	456	460	462	rBB	134	114	0.02%	0.002%
13	2.887	478	481	484	rBV	130	139	0.03%	0.003%
14	3.051	527	532	533	rBV	425	286	0.05%	0.006%
15	3.192	565	576	586	rBB2	1747	3666	0.68%	0.080%
16	3.240	589	591	594	rBB	127	90	0.02%	0.002%
17	3.362	623	629	633	rBB2	380	427	0.08%	0.009%
18	3.459	656	659	661	rBB	123	89	0.02%	0.002%
19	4.668	1013	1035	1068	rBV2	100713	321044	59.47%	6.988%
20	4.809	1075	1079	1082	rVB2	333	311	0.06%	0.007%
21	4.851	1090	1092	1095	rVV	188	112	0.02%	0.002%
22	5.067	1144	1159	1179	rBV2	102725	222156	41.15%	4.836%
23	5.256	1216	1218	1221	rBB	130	91	0.02%	0.002%
24	5.359	1246	1250	1253	rBB	167	155	0.03%	0.003%
25	5.729	1344	1365	1389	rBV2	199658	539837	100.00%	11.750%
26	5.813	1389	1391	1395	rVB	320	220	0.04%	0.005%
27	6.086	1473	1476	1478	rBV	120	106	0.02%	0.002%
28	6.250	1512	1527	1551	rBV	170695	319349	59.16%	6.951%
29	6.546	1607	1619	1632	rBB2	38064	70676	13.09%	1.538%
30	6.694	1651	1665	1688	rBB	124463	242141	44.85%	5.271%
31	7.185	1812	1818	1821	rBV2	363	415	0.08%	0.009%
32	7.568	1925	1937	1957	rBV	67098	116031	21.49%	2.526%
33	7.639	1957	1959	1960	rVV	265	149	0.03%	0.003%
34	7.677	1968	1971	1972	rBV	139	95	0.02%	0.002%
35	7.690	1972	1975	1979	rVB2	289	249	0.05%	0.005%
36	7.735	1984	1989	1992	rBB	164	178	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
 Data File : VU046497.D
 Acq On : 19 Dec 2021 16:08
 Operator : SY/MD
 Sample : M5066-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW142DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.841	2019	2022	2024	rBB	144	99	0.02%	0.002%
38	7.899	2027	2040	2055	rBV	242604	415343	76.94%	9.041%
39	7.967	2057	2061	2072	rVB2	3082	5090	0.94%	0.111%
40	8.009	2072	2074	2076	rBB	242	113	0.02%	0.002%
41	8.182	2116	2128	2145	rBV	47654	79042	14.64%	1.720%
42	8.337	2173	2176	2178	rBV	151	124	0.02%	0.003%
43	8.427	2201	2204	2207	rBV	142	144	0.03%	0.003%
44	8.555	2232	2244	2257	rBV	68704	114813	21.27%	2.499%
45	8.636	2257	2269	2293	rBV	176298	300551	55.67%	6.542%
46	8.780	2312	2314	2317	rBV	182	94	0.02%	0.002%
47	8.851	2334	2336	2339	rBB	163	110	0.02%	0.002%
48	9.009	2382	2385	2386	rBV	145	102	0.02%	0.002%
49	9.095	2409	2412	2415	rBV	153	150	0.03%	0.003%
50	9.137	2423	2425	2428	rBV	136	112	0.02%	0.002%
51	9.417	2498	2512	2531	rBV	249876	411095	76.15%	8.948%
52	9.520	2540	2544	2546	rVB	221	137	0.03%	0.003%
53	9.533	2546	2548	2550	rBV	135	98	0.02%	0.002%
54	9.616	2572	2574	2577	rBV	125	112	0.02%	0.002%
55	9.668	2587	2590	2593	rBV	130	136	0.03%	0.003%
56	9.693	2595	2598	2602	rVV	173	150	0.03%	0.003%
57	9.809	2630	2634	2640	rBV	165	253	0.05%	0.006%
58	9.899	2659	2662	2665	rBB	138	116	0.02%	0.003%
59	9.954	2675	2679	2683	rBB	163	188	0.03%	0.004%
60	9.996	2688	2692	2695	rBV	137	143	0.03%	0.003%
61	10.105	2721	2726	2733	rBV	181	288	0.05%	0.006%
62	10.192	2750	2753	2757	rBV	159	178	0.03%	0.004%
63	10.269	2774	2777	2780	rBB	157	126	0.02%	0.003%
64	10.314	2788	2791	2796	rBB	183	196	0.04%	0.004%
65	10.372	2807	2809	2811	rBV	135	94	0.02%	0.002%
66	10.555	2864	2866	2868	rBV	143	97	0.02%	0.002%
67	10.571	2869	2871	2874	rVB	163	107	0.02%	0.002%
68	10.607	2879	2882	2884	rBV	153	128	0.02%	0.003%
69	10.671	2897	2902	2910	rVB2	797	738	0.14%	0.016%
70	10.758	2916	2929	2945	rVB	188473	302543	56.04%	6.585%
71	10.902	2970	2974	2981	rBV2	353	430	0.08%	0.009%
72	11.031	3010	3014	3016	rBV	144	149	0.03%	0.003%
73	11.240	3077	3079	3082	rBV	165	136	0.03%	0.003%
74	11.398	3123	3128	3131	rBV	154	208	0.04%	0.005%
75	11.462	3137	3148	3156	rBV3	549	878	0.16%	0.019%
76	11.529	3165	3169	3173	rBV	179	222	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
 Data File : VU046497.D
 Acq On : 19 Dec 2021 16:08
 Operator : SY/MD
 Sample : M5066-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW142DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.677	3209	3215	3217	rBV	196	211	0.04%	0.005%
78	11.690	3217	3219	3222	rBV	157	128	0.02%	0.003%
79	11.812	3242	3257	3276	rBV	260264	403076	74.67%	8.774%
80	11.934	3292	3295	3297	rBV2	178	122	0.02%	0.003%
81	12.192	3362	3375	3396	rVB	241013	389240	72.10%	8.472%
82	12.774	3549	3556	3563	rBV2	677	934	0.17%	0.020%
83	13.568	3800	3803	3805	rBV	139	99	0.02%	0.002%
84	13.918	3908	3912	3917	rBV	119	153	0.03%	0.003%
85	14.581	4109	4118	4124	rBV	653	938	0.17%	0.020%
86	15.201	4308	4311	4315	rVB2	164	119	0.02%	0.003%
87	15.446	4383	4387	4392	rBV2	173	209	0.04%	0.005%
88	15.561	4420	4423	4425	rVB	180	97	0.02%	0.002%
89	15.600	4433	4435	4438	rVB	155	97	0.02%	0.002%
90	15.632	4442	4445	4447	rVV	193	117	0.02%	0.003%
91	15.661	4451	4454	4457	rBV	172	122	0.02%	0.003%
92	15.684	4457	4461	4464	rVV2	191	160	0.03%	0.003%
93	15.738	4475	4478	4484	rVB2	218	231	0.04%	0.005%
94	15.770	4484	4488	4491	rBV2	249	269	0.05%	0.006%
95	15.815	4498	4502	4504	rBV2	150	130	0.02%	0.003%
96	15.867	4515	4518	4522	rBV2	142	179	0.03%	0.004%
97	16.008	4558	4562	4563	rBV	243	196	0.04%	0.004%
98	16.741	4785	4790	4793	rBV3	333	418	0.08%	0.009%
99	16.979	4862	4864	4868	rVB2	452	172	0.03%	0.004%
100	17.548	5038	5041	5044	rBV2	545	452	0.08%	0.010%




Sum of corrected areas: 4594184

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
Data File : VU046497.D
Acq On : 19 Dec 2021 16:08
Operator : SY/MD
Sample : M5066-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW142DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

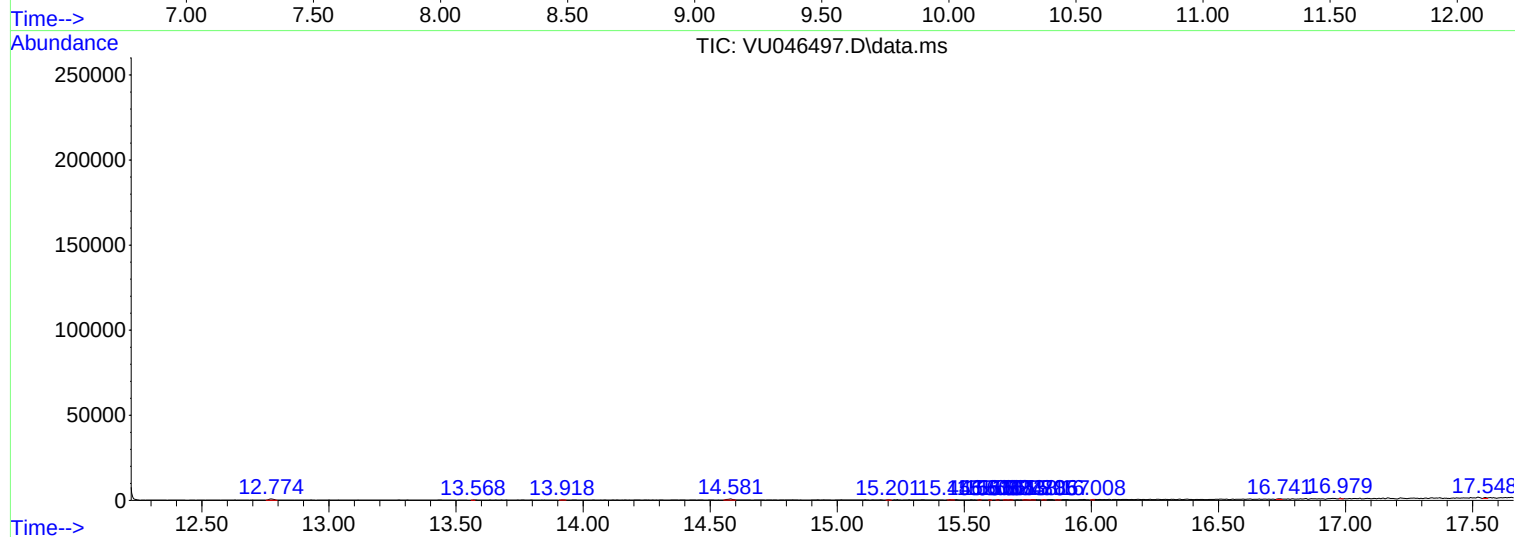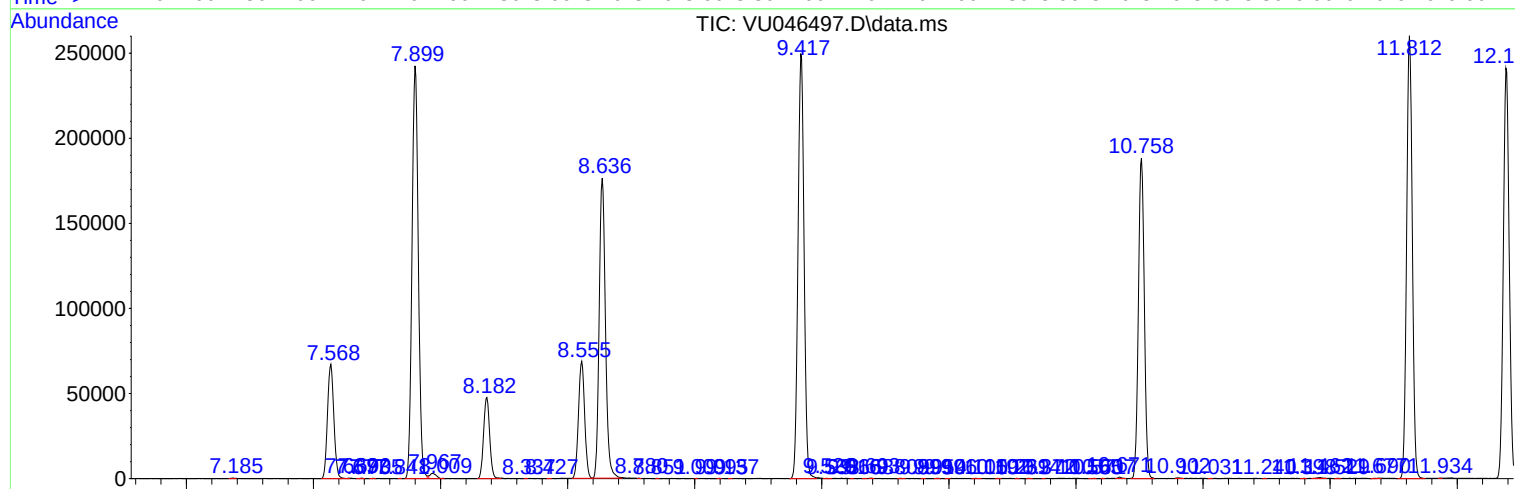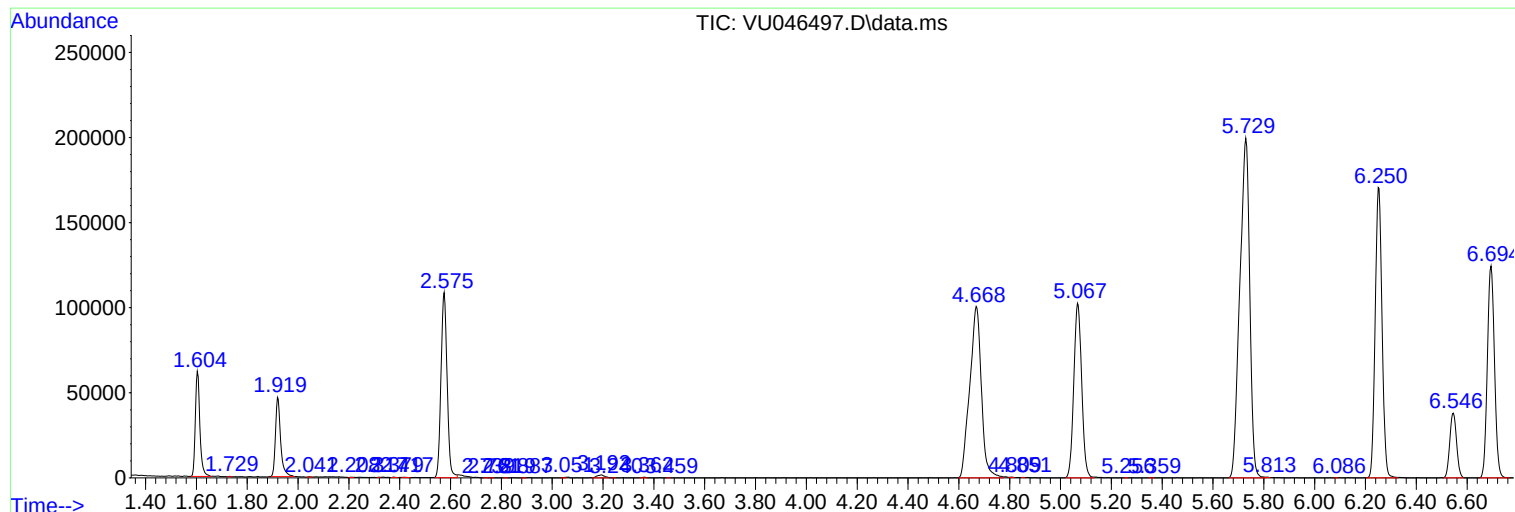

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
Data File : VU046497.D
Acq On : 19 Dec 2021 16:08
Operator : SY/MD
Sample : M5066-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW142DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
Data File : VU046497.D
Acq On : 19 Dec 2021 16:08
Operator : SY/MD
Sample : M5066-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW142DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------