

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
 Data File : VU046500.D
 Acq On : 19 Dec 2021 17:15
 Operator : SY/MD
 Sample : M5066-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	102	rVB	58725	71947	13.42%	1.700%
2	1.922	172	181	205	rBV	46700	67651	12.62%	1.598%
3	2.096	232	235	237	rBV2	332	231	0.04%	0.005%
4	2.195	264	266	269	rVB	179	99	0.02%	0.002%
5	2.292	293	296	300	rVB	158	118	0.02%	0.003%
6	2.363	315	318	320	rBV2	175	133	0.02%	0.003%
7	2.575	372	384	409	rBV	108356	181319	33.82%	4.284%
8	2.687	417	419	424	rVB2	215	136	0.03%	0.003%
9	2.771	442	445	449	rBB	145	148	0.03%	0.003%
10	3.051	529	532	535	rBV2	289	231	0.04%	0.005%
11	3.128	554	556	559	rBV	133	118	0.02%	0.003%
12	3.183	569	573	574	rBV2	417	279	0.05%	0.007%
13	4.176	880	882	886	rBB	125	114	0.02%	0.003%
14	4.642	1013	1027	1068	rBV	41440	140540	26.22%	3.321%
15	4.813	1078	1080	1084	rVB	146	125	0.02%	0.003%
16	4.919	1111	1113	1118	rBB	121	111	0.02%	0.003%
17	5.067	1144	1159	1181	rBV	101051	217855	40.64%	5.147%
18	5.176	1191	1193	1196	rBV	146	123	0.02%	0.003%
19	5.729	1344	1365	1392	rBV2	198048	536064	100.00%	12.666%
20	6.253	1514	1528	1550	rBV	171616	324354	60.51%	7.664%
21	6.530	1610	1614	1616	rBV2	374	298	0.06%	0.007%
22	6.549	1616	1620	1623	rVB2	465	429	0.08%	0.010%
23	6.694	1651	1665	1684	rBV	126580	240958	44.95%	5.693%
24	6.774	1688	1690	1692	rVB	245	113	0.02%	0.003%
25	7.047	1772	1775	1778	rBB	221	132	0.02%	0.003%
26	7.186	1813	1818	1825	rBB	390	442	0.08%	0.010%
27	7.568	1925	1937	1960	rBV	65472	114142	21.29%	2.697%
28	7.687	1971	1974	1976	rBV	250	184	0.03%	0.004%
29	7.851	2022	2025	2027	rBV	169	133	0.02%	0.003%
30	7.899	2027	2040	2056	rVV	241807	412379	76.93%	9.744%
31	7.970	2058	2062	2075	rVB2	3225	4774	0.89%	0.113%
32	8.179	2117	2127	2143	rBV2	47559	78592	14.66%	1.857%
33	8.321	2168	2171	2173	rBV	122	108	0.02%	0.003%
34	8.472	2214	2218	2221	rBV	365	343	0.06%	0.008%
35	8.514	2224	2231	2234	rVV	329	365	0.07%	0.009%
36	8.555	2238	2244	2249	rVB5	1647	1937	0.36%	0.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
 Data File : VU046500.D
 Acq On : 19 Dec 2021 17:15
 Operator : SY/MD
 Sample : M5066-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.636	2257	2269	2296	rBV	172858	293486	54.75%	6.934%
38	8.748	2302	2304	2307	rVB3	291	185	0.03%	0.004%
39	8.771	2307	2311	2317	rVB	191	202	0.04%	0.005%
40	8.822	2324	2327	2329	rVB	155	105	0.02%	0.002%
41	8.848	2333	2335	2339	rBB	137	119	0.02%	0.003%
42	8.886	2344	2347	2350	rBV	157	156	0.03%	0.004%
43	8.970	2370	2373	2375	rBB	153	106	0.02%	0.003%
44	9.005	2381	2384	2388	rBB	205	182	0.03%	0.004%
45	9.050	2395	2398	2401	rBB	150	121	0.02%	0.003%
46	9.092	2408	2411	2414	rBB	142	121	0.02%	0.003%
47	9.179	2435	2438	2441	rBB	158	122	0.02%	0.003%
48	9.259	2459	2463	2465	rBB	172	143	0.03%	0.003%
49	9.366	2493	2496	2499	rVV	116	98	0.02%	0.002%
50	9.417	2499	2512	2537	rVV	255853	421924	78.71%	9.969%
51	9.697	2595	2599	2602	rVV	273	239	0.04%	0.006%
52	9.851	2644	2647	2648	rBV	148	102	0.02%	0.002%
53	9.880	2654	2656	2659	rBB	146	98	0.02%	0.002%
54	9.941	2672	2675	2679	rBV	127	132	0.02%	0.003%
55	10.099	2721	2724	2727	rBV	117	127	0.02%	0.003%
56	10.118	2727	2730	2733	rVV	124	96	0.02%	0.002%
57	10.198	2750	2755	2756	rBV	138	143	0.03%	0.003%
58	10.234	2763	2766	2771	rBV	153	205	0.04%	0.005%
59	10.372	2805	2809	2811	rBV	147	142	0.03%	0.003%
60	10.420	2821	2824	2827	rBV	132	135	0.03%	0.003%
61	10.642	2890	2893	2895	rBB	166	108	0.02%	0.003%
62	10.671	2896	2902	2911	rBV3	886	1137	0.21%	0.027%
63	10.758	2917	2929	2946	rVB	187807	299670	55.90%	7.080%
64	10.870	2962	2964	2967	rBV	218	145	0.03%	0.003%
65	10.890	2967	2970	2973	rVV2	281	256	0.05%	0.006%
66	10.909	2973	2976	2982	rVB2	233	232	0.04%	0.005%
67	11.012	3005	3008	3012	rBB	179	170	0.03%	0.004%
68	11.034	3013	3015	3018	rBV	156	125	0.02%	0.003%
69	11.227	3069	3075	3078	rBV	164	238	0.04%	0.006%
70	11.259	3082	3085	3090	rVB	123	126	0.02%	0.003%
71	11.452	3139	3145	3146	rBV2	577	456	0.09%	0.011%
72	11.812	3244	3257	3272	rBV	268308	416033	77.61%	9.830%
73	11.954	3297	3301	3303	rVV2	251	202	0.04%	0.005%
74	11.976	3303	3308	3313	rVB3	469	539	0.10%	0.013%
75	12.195	3363	3376	3393	rVV	243788	391092	72.96%	9.241%
76	12.275	3399	3401	3406	rBV	168	107	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
 Data File : VU046500.D
 Acq On : 19 Dec 2021 17:15
 Operator : SY/MD
 Sample : M5066-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.472	3456	3462	3467	rBV	108	139	0.03%	0.003%
78	12.661	3519	3521	3526	rVB	148	149	0.03%	0.004%
79	12.690	3527	3530	3535	rBV	204	256	0.05%	0.006%
80	12.774	3548	3556	3563	rBV2	588	931	0.17%	0.022%
81	12.947	3605	3610	3613	rBV	275	340	0.06%	0.008%
82	13.687	3837	3840	3844	rBV	129	107	0.02%	0.003%
83	14.240	4010	4012	4021	rVB	247	166	0.03%	0.004%
84	14.578	4110	4117	4125	rVB	583	835	0.16%	0.020%
85	15.008	4248	4251	4256	rBV	112	101	0.02%	0.002%
86	15.250	4323	4326	4329	rBV	221	133	0.02%	0.003%
87	15.340	4351	4354	4358	rVB2	233	165	0.03%	0.004%
88	15.417	4375	4378	4382	rBV2	285	225	0.04%	0.005%
89	15.439	4382	4385	4387	rBV	231	179	0.03%	0.004%
90	15.658	4451	4453	4456	rBV	181	97	0.02%	0.002%
91	15.690	4461	4463	4468	rVB	170	137	0.03%	0.003%
92	15.719	4468	4472	4473	rBV	177	105	0.02%	0.002%
93	15.803	4493	4498	4502	rVB2	192	196	0.04%	0.005%
94	15.838	4505	4509	4513	rVB2	266	238	0.04%	0.006%
95	15.867	4514	4518	4524	rBV2	293	372	0.07%	0.009%
96	15.954	4537	4545	4549	rBV2	361	488	0.09%	0.012%
97	15.979	4549	4553	4554	rBV	239	175	0.03%	0.004%
98	16.050	4572	4575	4577	rBV2	186	137	0.03%	0.003%
99	16.668	4764	4767	4769	rBV	325	193	0.04%	0.005%
100	17.211	4932	4936	4937	rBV2	400	329	0.06%	0.008%




Sum of corrected areas: 4232343

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
Data File : VU046500.D
Acq On : 19 Dec 2021 17:15
Operator : SY/MD
Sample : M5066-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

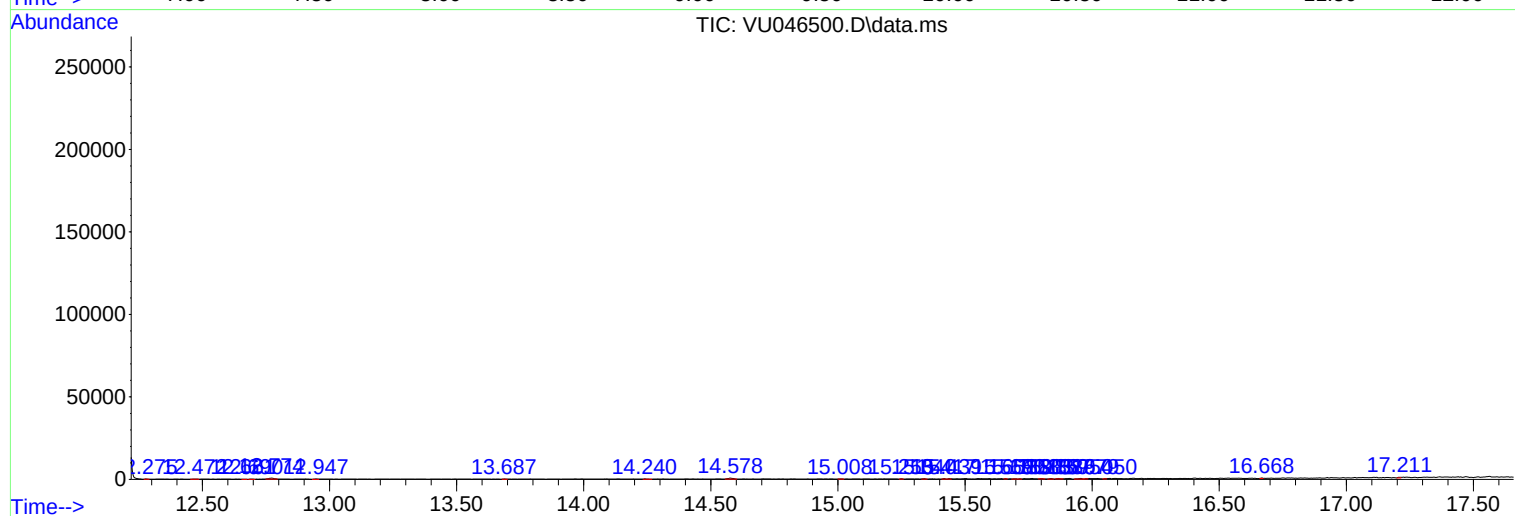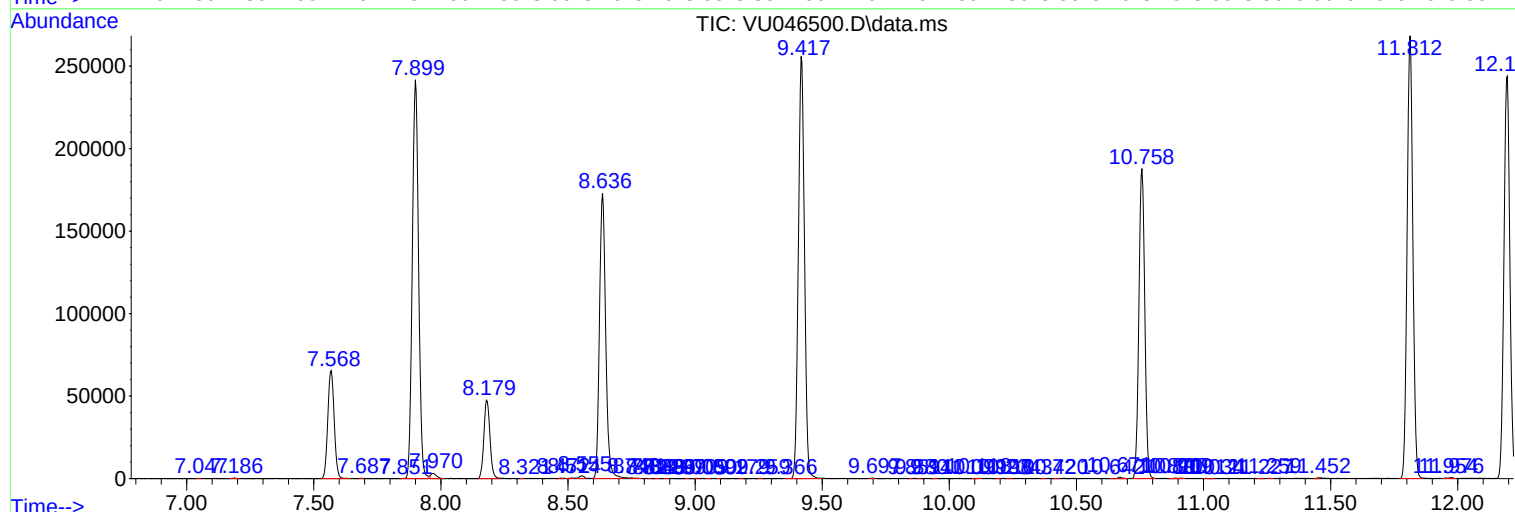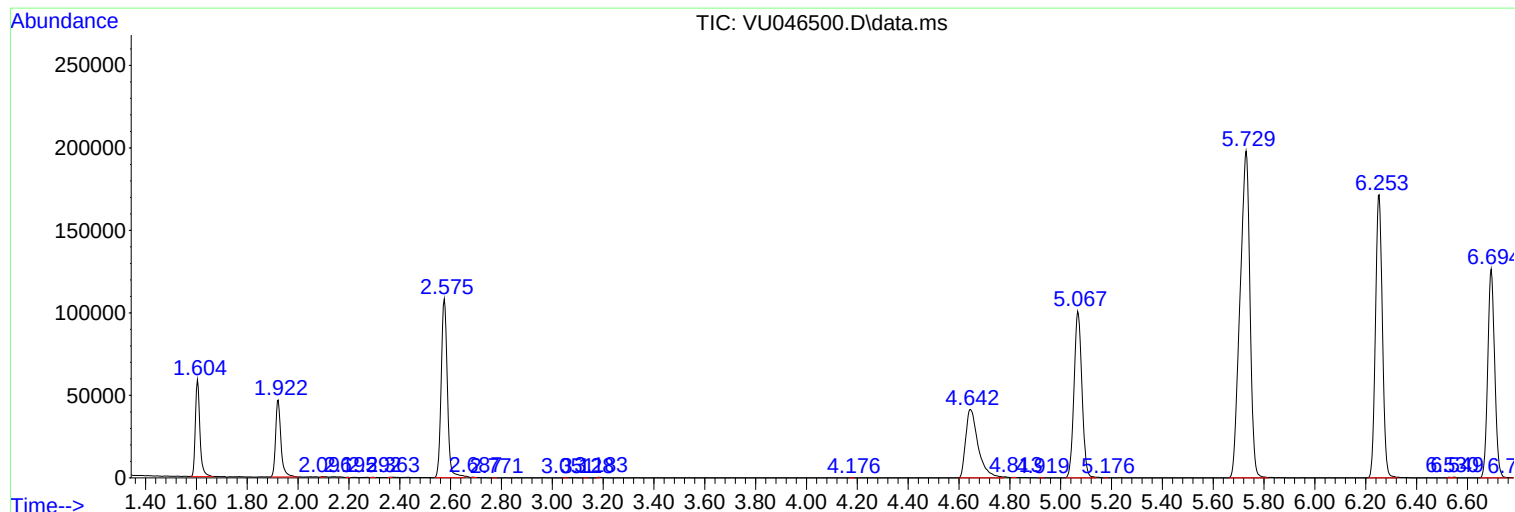

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
Data File : VU046500.D
Acq On : 19 Dec 2021 17:15
Operator : SY/MD
Sample : M5066-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
Data File : VU046500.D
Acq On : 19 Dec 2021 17:15
Operator : SY/MD
Sample : M5066-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------