


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121921\
 Data File : VU046483.D
 Acq On : 19 Dec 2021 09:54
 Operator : SY/MD
 Sample : BFB035
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB035

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 20 00:25:10 2021

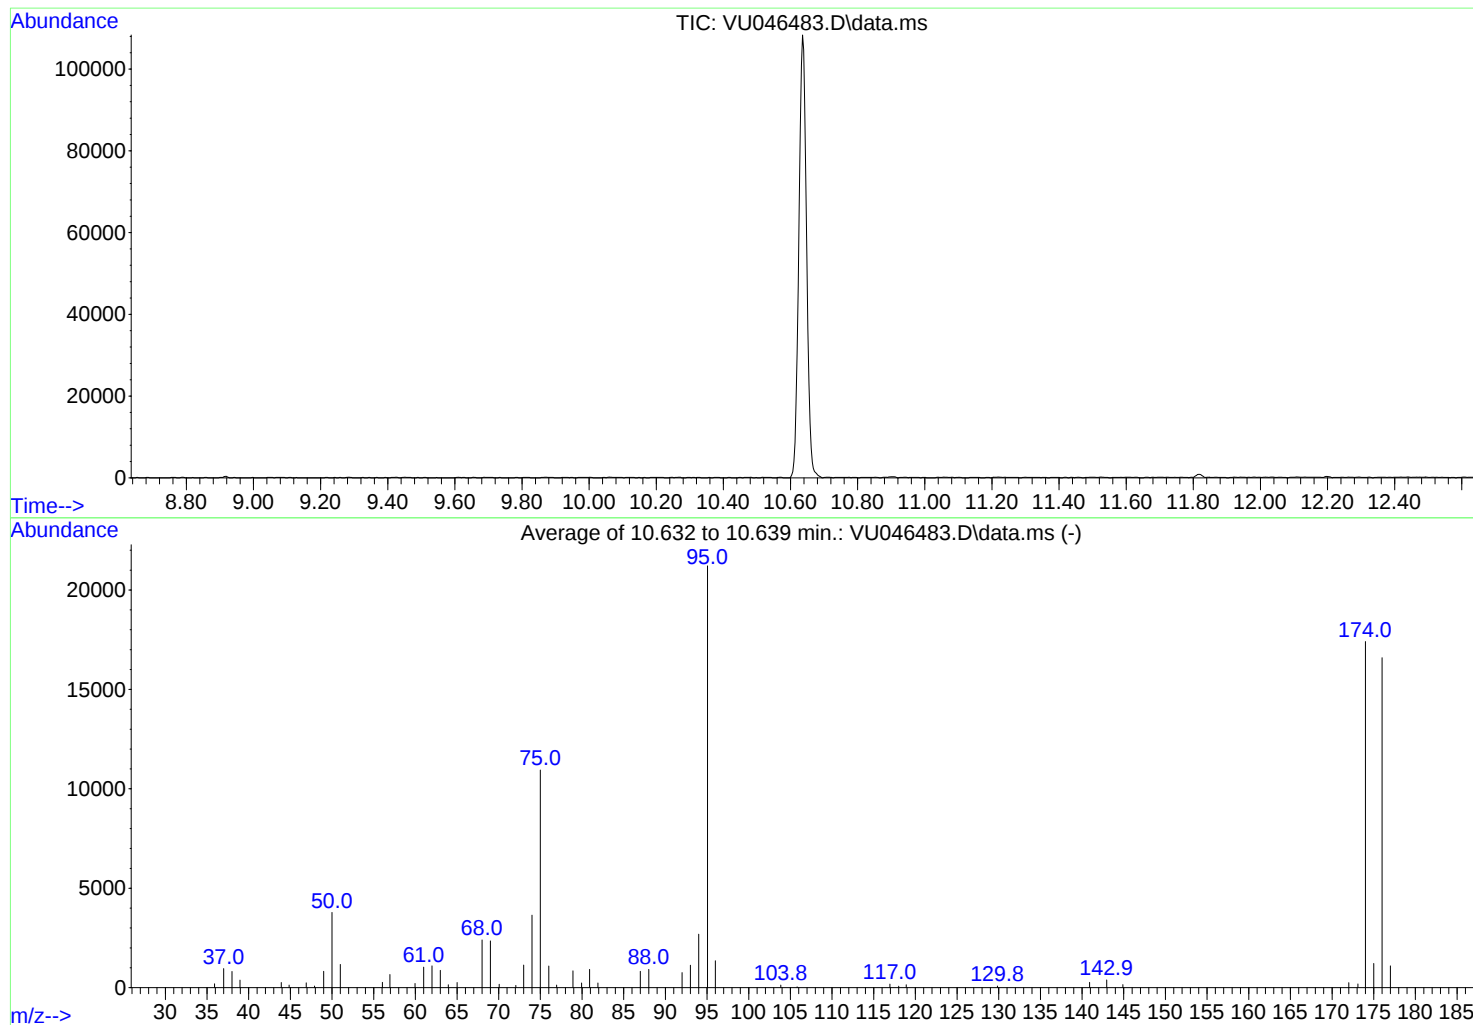

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	3781	PASS
75	95	30	80	51.6	10943	PASS
95	95	100	100	100.0	21216	PASS
96	95	5	9	6.4	1356	PASS
173	174	0.00	2	1.1	189	PASS
174	95	50	120	82.0	17405	PASS
175	174	5	9	7.0	1216	PASS
176	174	95	101	95.3	16592	PASS
177	176	5	9	6.6	1097	PASS

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	193.0
37.00	906.0
38.00	787.0
39.00	393.0
43.90	256.0
44.80	134.0
46.90	265.0
47.90	132.0
49.00	861.0
50.00	3627.0
51.00	1110.0
56.00	294.0
56.90	675.0
60.00	217.0
61.00	1002.0
62.00	978.0
63.00	826.0
64.00	166.0
65.00	243.0
68.00	2470.0
69.00	2231.0
70.00	160.0
72.00	106.0
73.00	1188.0
74.00	3487.0
75.00	10893.0
76.00	984.0
77.00	123.0
78.90	758.0
80.00	231.0
80.90	934.0
81.90	219.0
87.00	839.0
88.00	909.0
92.00	729.0
93.00	1059.0
94.00	2451.0
95.00	20696.0
96.00	1330.0
103.90	132.0
117.00	155.0
118.90	157.0
140.90	258.0
142.90	343.0
144.90	177.0
172.00	240.0
173.10	160.0
174.00	16400.0
175.00	1143.0
176.00	15809.0
177.00	1081.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	212.0
37.00	984.0
38.00	841.0
38.90	400.0
43.90	264.0
44.90	130.0
46.90	258.0
47.90	114.0
49.00	826.0
50.00	3874.0
51.00	1215.0
56.00	272.0
56.90	703.0
59.90	223.0
61.00	1061.0
62.00	1122.0
63.00	898.0
63.90	141.0
65.00	276.0
68.00	2509.0
69.00	2466.0
70.00	179.0
72.10	119.0
73.00	1197.0
74.00	3778.0
75.00	11266.0
76.00	1093.0
77.00	132.0
78.90	867.0
79.90	232.0
80.90	941.0
81.90	248.0
87.00	860.0
88.00	951.0
92.00	794.0
93.00	1169.0
94.00	2783.0
95.10	21912.0
96.00	1404.0
103.90	130.0
105.80	115.0
117.00	184.0
118.00	105.0
118.90	140.0
129.90	110.0
140.90	282.0
142.90	409.0
144.90	166.0
172.00	260.0
173.10	205.0
174.00	17952.0
175.00	1261.0
176.00	17144.0
177.00	1121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	182.0
37.00	974.0
38.00	821.0
38.90	335.0
43.90	250.0
44.90	131.0
46.90	193.0
49.00	776.0
50.00	3842.0
51.00	1188.0
56.10	237.0
57.00	612.0
59.90	187.0
61.00	1030.0
62.00	1179.0
63.00	881.0
63.90	128.0
65.00	258.0
68.00	2206.0
69.00	2346.0
70.10	158.0
72.00	111.0
73.00	1014.0
74.00	3674.0
75.00	10671.0
76.00	1176.0
76.90	122.0
78.90	908.0
79.90	240.0
80.90	885.0
81.90	226.0
87.00	762.0
88.00	895.0
92.00	741.0
93.00	1157.0
94.00	2835.0
95.10	21040.0
96.00	1333.0
103.80	122.0
116.90	203.0
118.00	103.0
118.90	141.0
129.80	140.0
140.90	259.0
143.00	412.0
144.90	116.0
172.00	252.0
173.10	202.0
174.00	17864.0
175.00	1245.0
176.00	16824.0
177.00	1089.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035