

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121922\
 Data File : VU052453.D
 Acq On : 19 Dec 2022 11:59
 Operator : JC/MD
 Sample : VU1219WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Dec 20 00:28:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	16030	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.349	117	14481	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.745	152	6789	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.599	65	9145	0.484	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	96.000%
4) 1,2-Dichloroethane-d4	5.661	65	7772	0.434	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	86.000%
7) 1,2-Dichloropropane-d6	6.639	67	8905	0.512	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	102.000%
8) Toluene-d8	7.833	98	10757	0.410	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	82.000%
10) 1,1,2,2-Tetrachloroeth...	10.683	84	9674	0.520	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
					Qvalue	
6) Trichloroethene	6.489	95	150	0.009	ug/L #	90
12) 1,2,3-Trichloropropane	10.751	75	51	0.004	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121922\
Data File : VU052453.D
Acq On : 19 Dec 2022 11:59
Operator : JC/MD
Sample : VU1219WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Dec 20 00:28:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

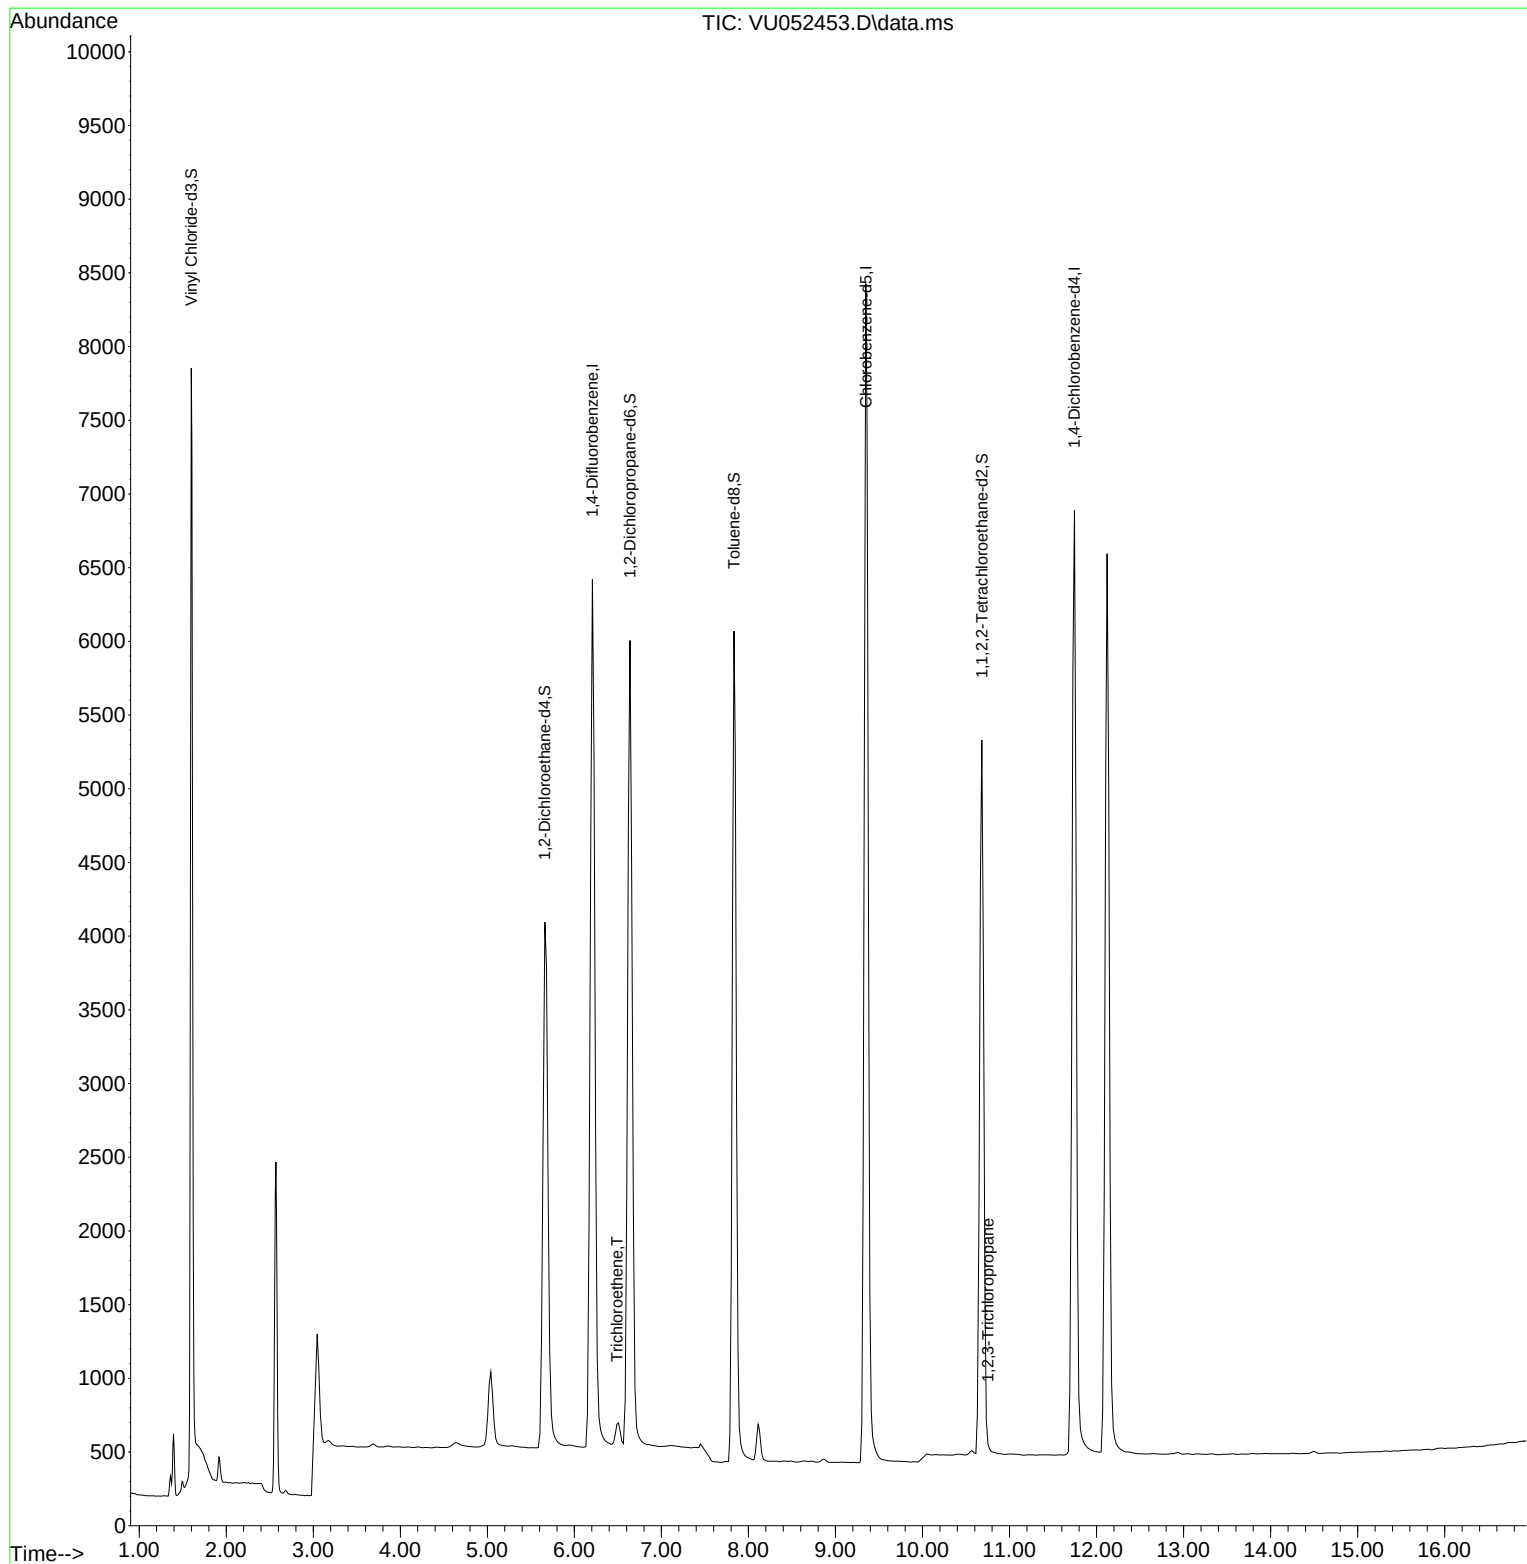

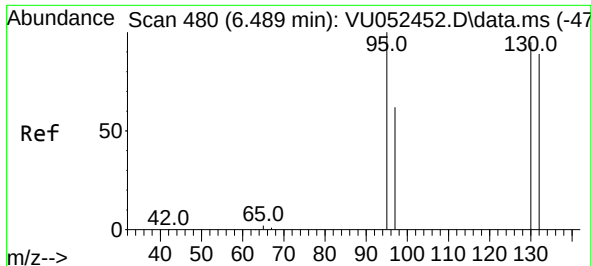




#6
 Trichloroethene
 Concen: 0.009 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052453.D
 Acq: 19 Dec 2022 11:59

Instrument :
 MSVOA_U
 ClientSampleId :

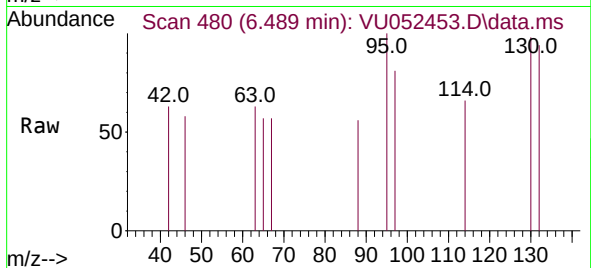

Tgt Ion: 95 Resp: 150

Ion	Ratio	Lower	Upper
95	100		
97	81.4	43.3	80.3#
132	94.2	61.0	113.2
130	97.7	66.7	123.9

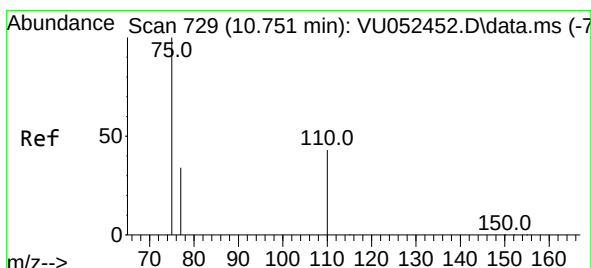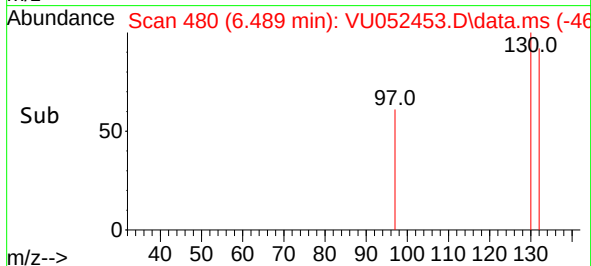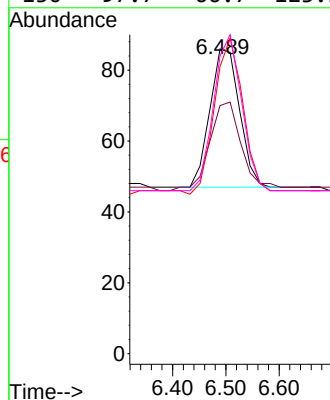

#12
 1,2,3-Trichloropropane
 Concen: 0.004 ug/L
 RT: 10.751 min Scan# 729
 Delta R.T. 0.000 min
 Lab File: VU052453.D
 Acq: 19 Dec 2022 11:59

Tgt Ion: 75 Resp: 51

Ion	Ratio	Lower	Upper
75	100		
110	29.4	32.2	48.2#
77	64.7	26.8	40.2#

