

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121922\
 Data File : VU052455.D
 Acq On : 19 Dec 2022 12:53
 Operator : JC/MD
 Sample : N6034-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Dec 20 00:28:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.207	114	15033	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.346	117	13554	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.742	152	6587	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.599	65	8998	0.508	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.661	65	8396	0.500	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
7) 1,2-Dichloropropane-d6	6.639	67	9408	0.578	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	116.000%
8) Toluene-d8	7.830	98	11322	0.461	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
10) 1,1,2,2-Tetrachloroeth...	10.679	84	10323	0.593	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	118.000%
Target Compounds						
6) Trichloroethene	6.489	95	234	0.015	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121922\
Data File : VU052455.D
Acq On : 19 Dec 2022 12:53
Operator : JC/MD
Sample : N6034-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Dec 20 00:28:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

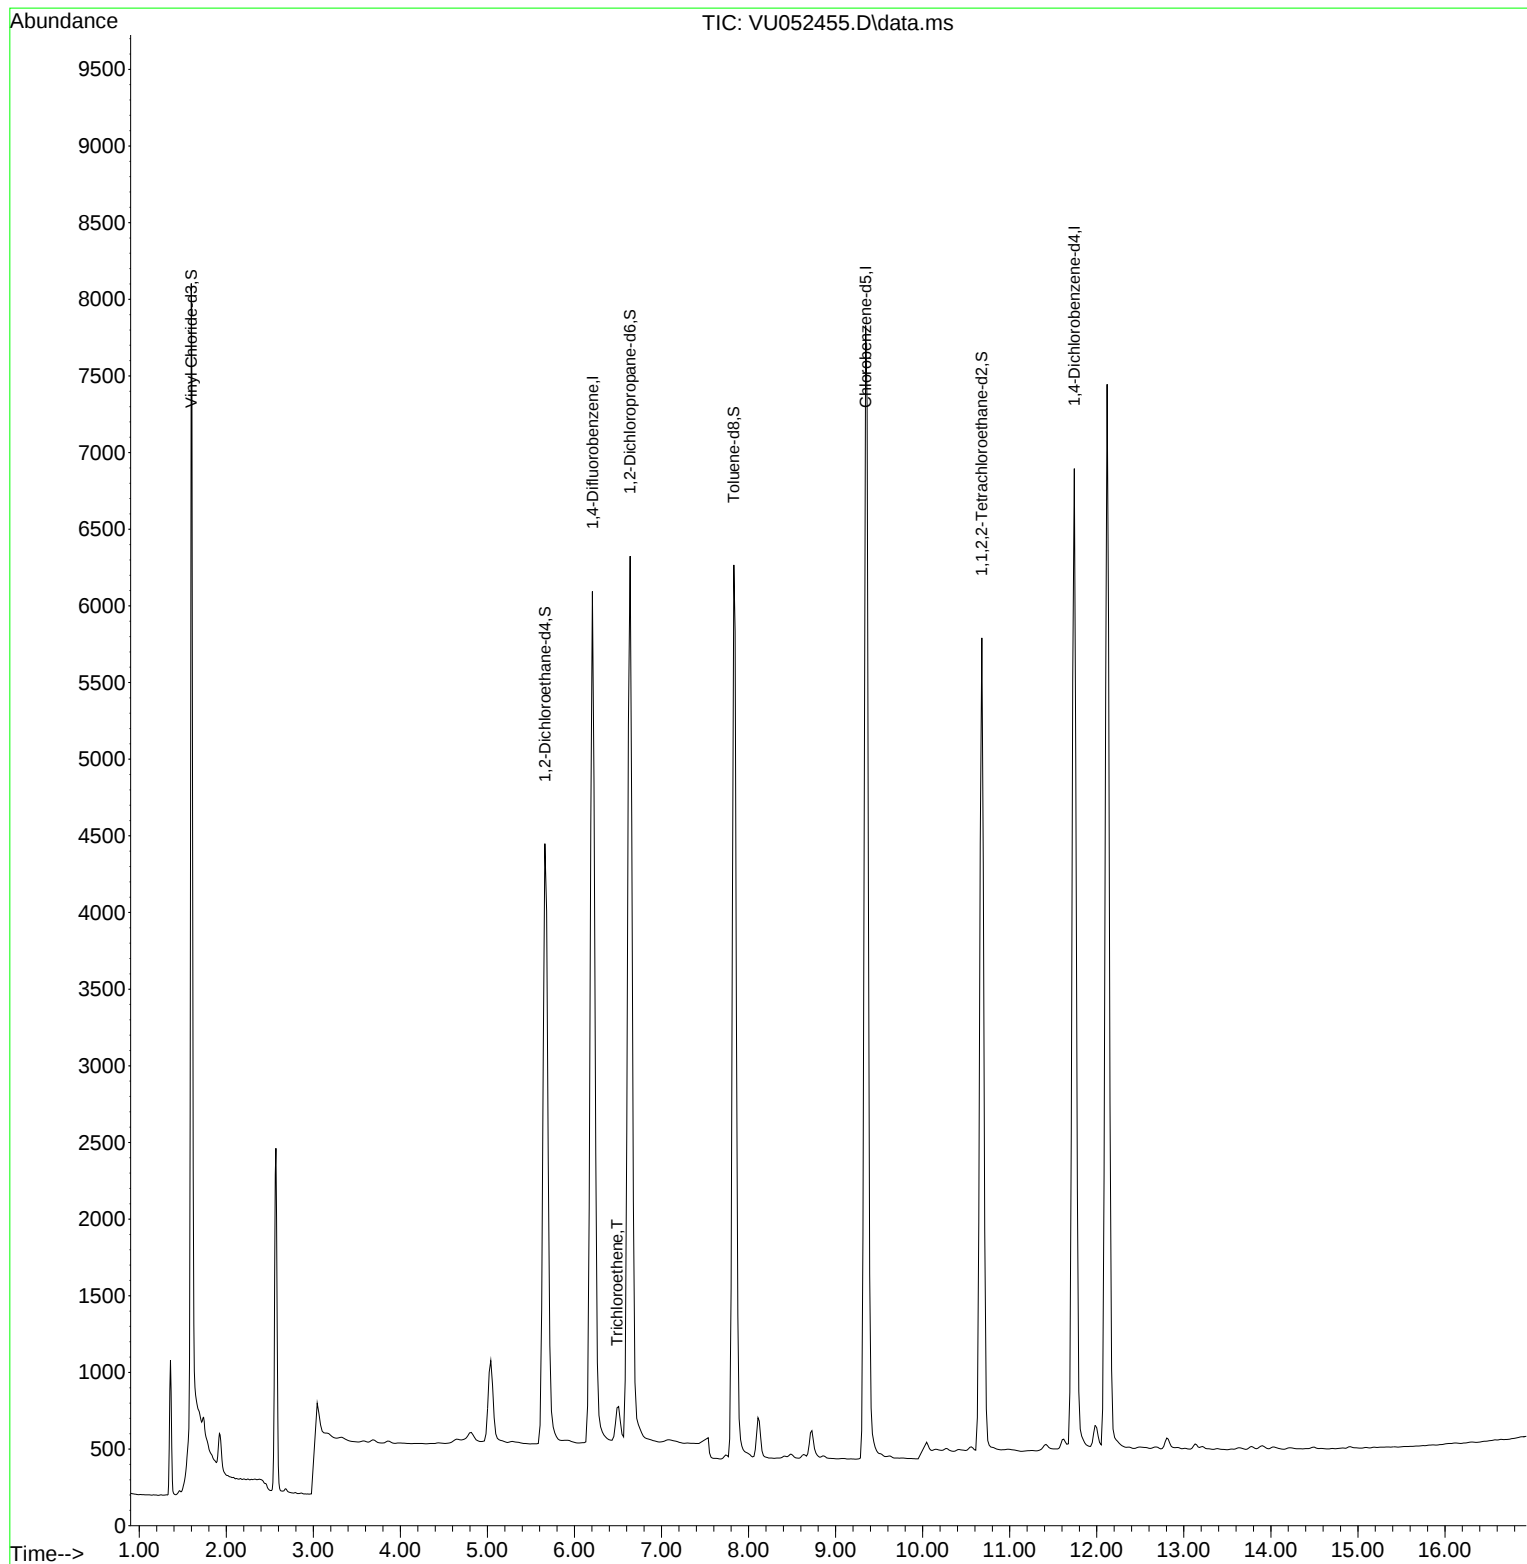

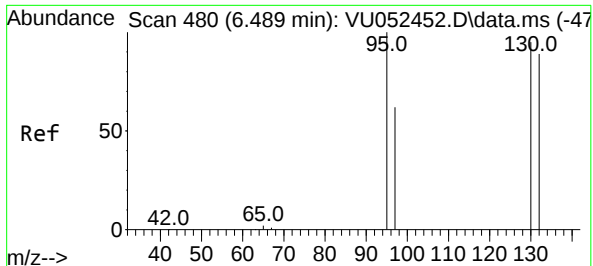

#6
 Trichloroethene
 Concen: 0.015 ug/L
 RT: 6.489 min Scan# 480
 Delta R.T. -0.000 min
 Lab File: VU052455.D
 Acq: 19 Dec 2022 12:53

Instrument :
 MSVOA_U
 ClientSampleId :

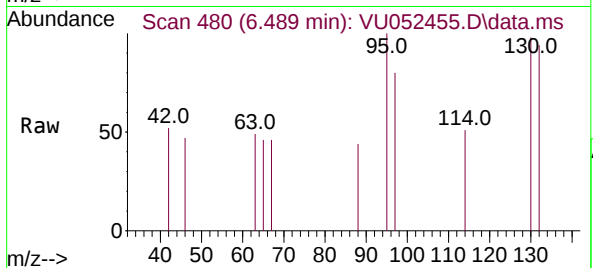

Tgt Ion: 95	Resp: 234
Ion Ratio	Lower Upper
95 100	
97 79.6	43.3 80.3
132 94.4	61.0 113.2
130 98.1	66.7 123.9

