

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121922\
 Data File : VU052456.D
 Acq On : 19 Dec 2022 13:17
 Operator : JC/MD
 Sample : N6034-17RE
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Dec 20 00:28:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	15492	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.349	117	14065	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.745	152	6860	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	128	0.007	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	2.000%#
4) 1,2-Dichloroethane-d4	5.661	65	8250	0.477	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.000%
7) 1,2-Dichloropropane-d6	6.639	67	9202	0.545	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.833	98	428	0.017	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	4.000%#
10) 1,1,2,2-Tetrachloroeth...	10.682	84	9983	0.552	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.000%
Target Compounds						
					Qvalue	
6) Trichloroethene	6.489	95	211	0.013	ug/L #	91
9) 1,2-Dibromoethane	8.761	107	203	0.017	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121922\
Data File : VU052456.D
Acq On : 19 Dec 2022 13:17
Operator : JC/MD
Sample : N6034-17RE
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Dec 20 00:28:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

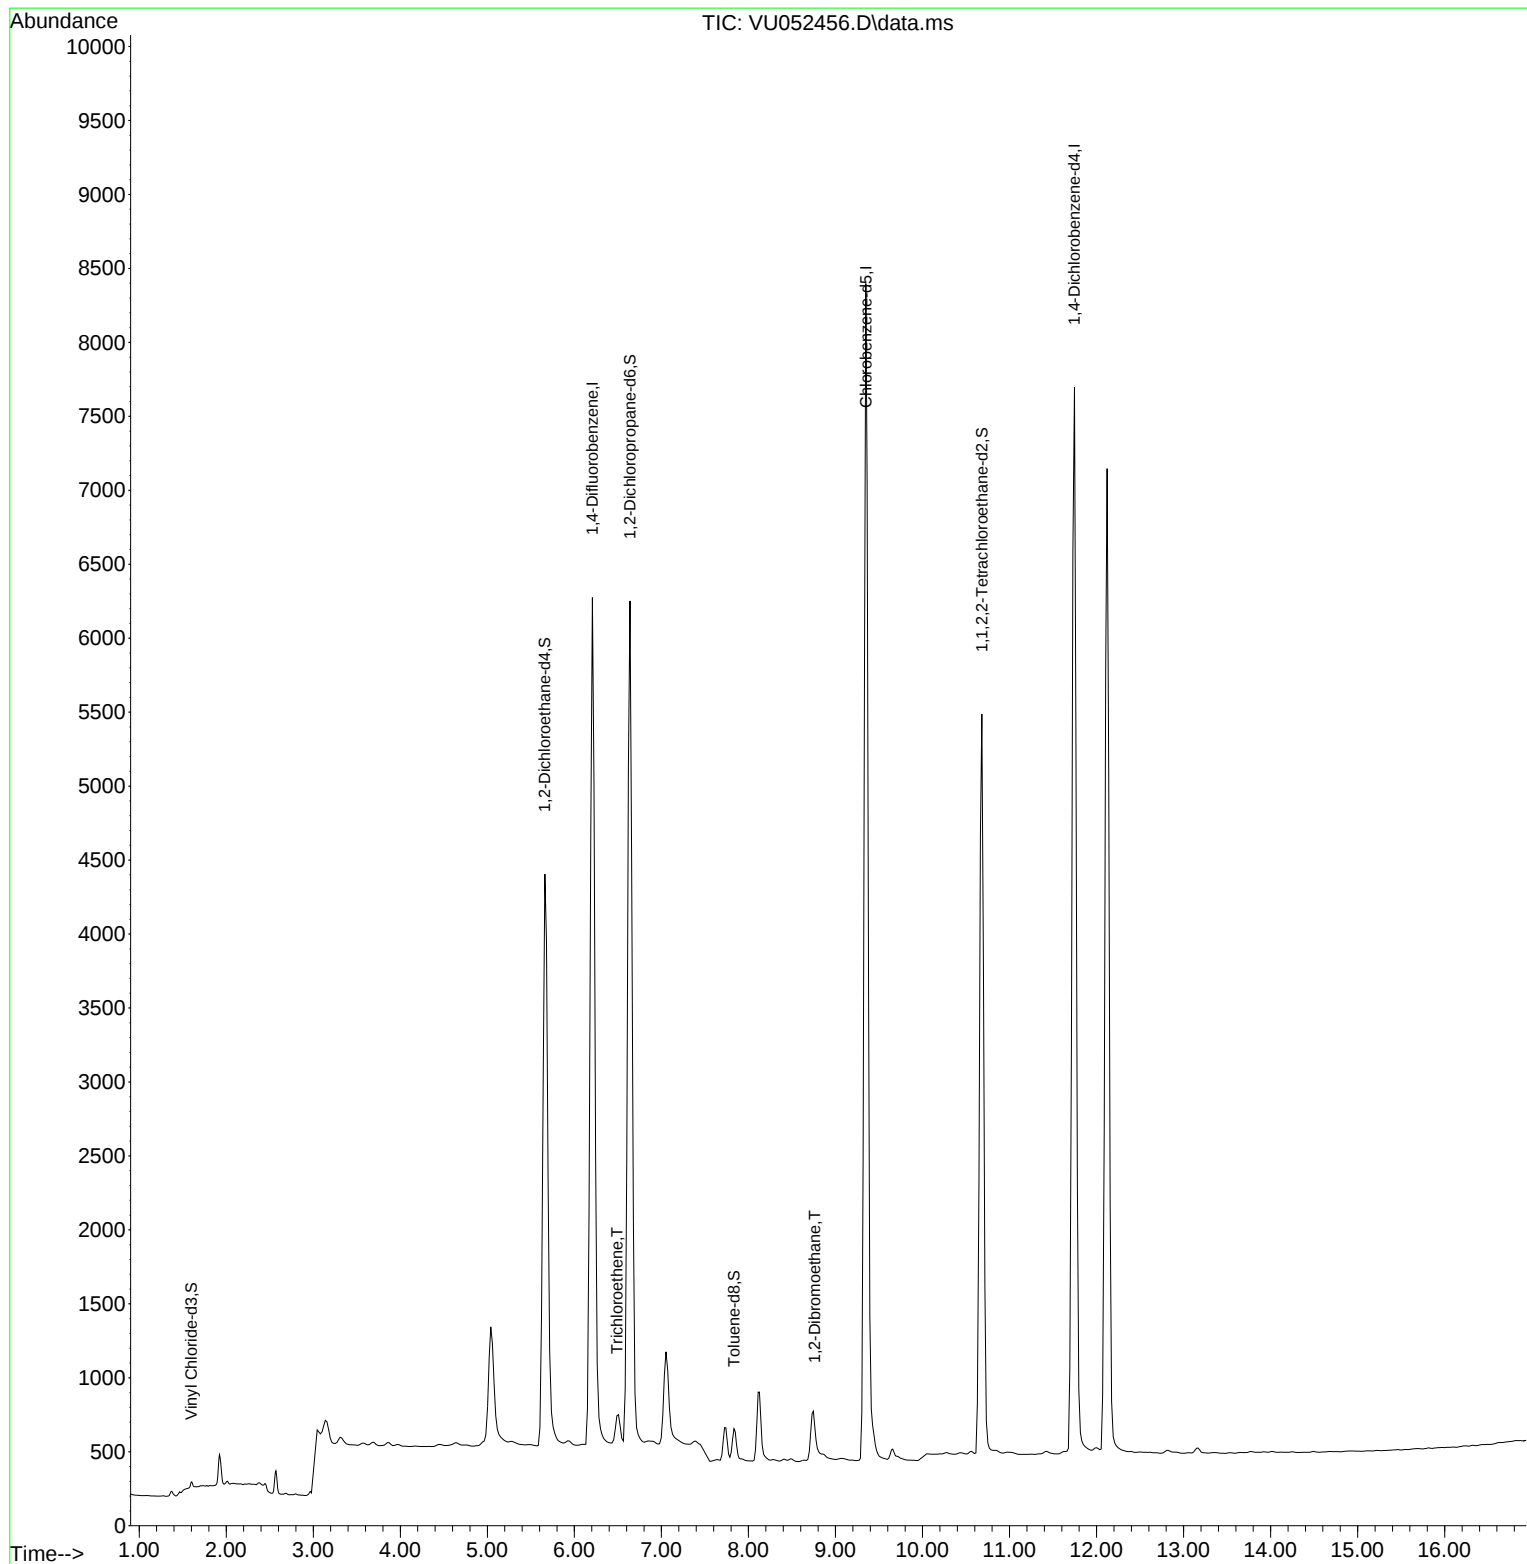

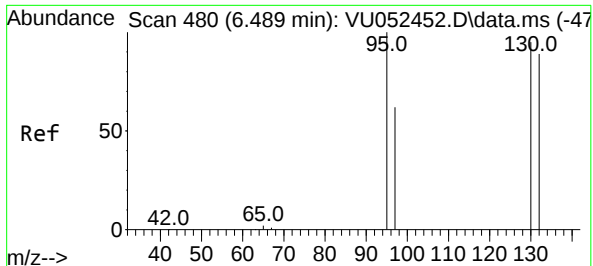




#6
 Trichloroethene
 Concen: 0.013 ug/L
 RT: 6.489 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VU052456.D
 Acq: 19 Dec 2022 13:17

Instrument :
 MSVOA_U
 ClientSampleId :

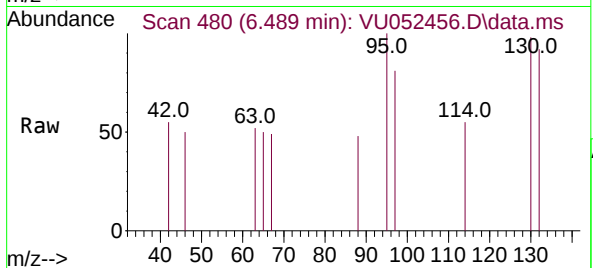


Tgt Ion: 95 Resp: 211

Ion	Ratio	Lower	Upper
95	100		
97	81.2	43.3	80.3#
132	92.1	61.0	113.2
130	98.0	66.7	123.9

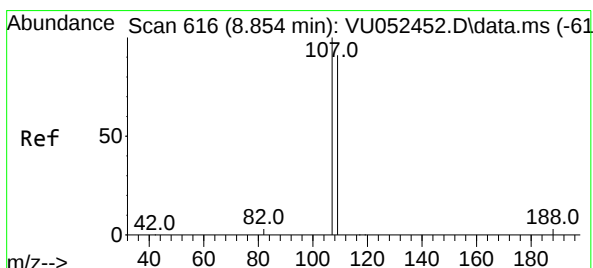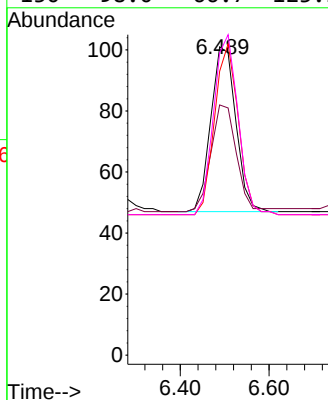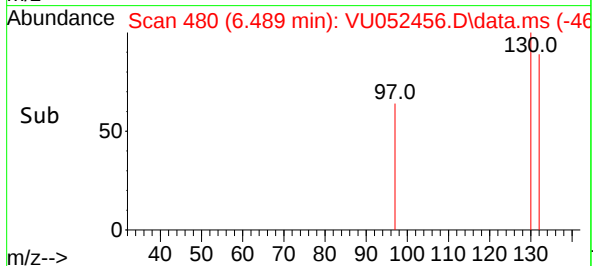

#9
 1,2-Dibromoethane
 Concen: 0.017 ug/L
 RT: 8.761 min Scan# 610
 Delta R.T. -0.093 min
 Lab File: VU052456.D
 Acq: 19 Dec 2022 13:17

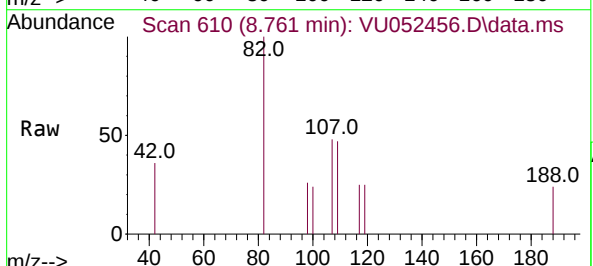

Tgt Ion: 107 Resp: 203

Ion	Ratio	Lower	Upper
107	100		
109	98.9	64.8	120.3
188	49.5	4.3	6.5#

